


Data Path : Z:\HPCHEM1\BNA F\DATA\BF080217\
 Data File : BF097270.D
 Acq On : 2 Aug 2017 13:37
 Operator : SJ/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF072517.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Thu Aug 03 12:06:13 2017

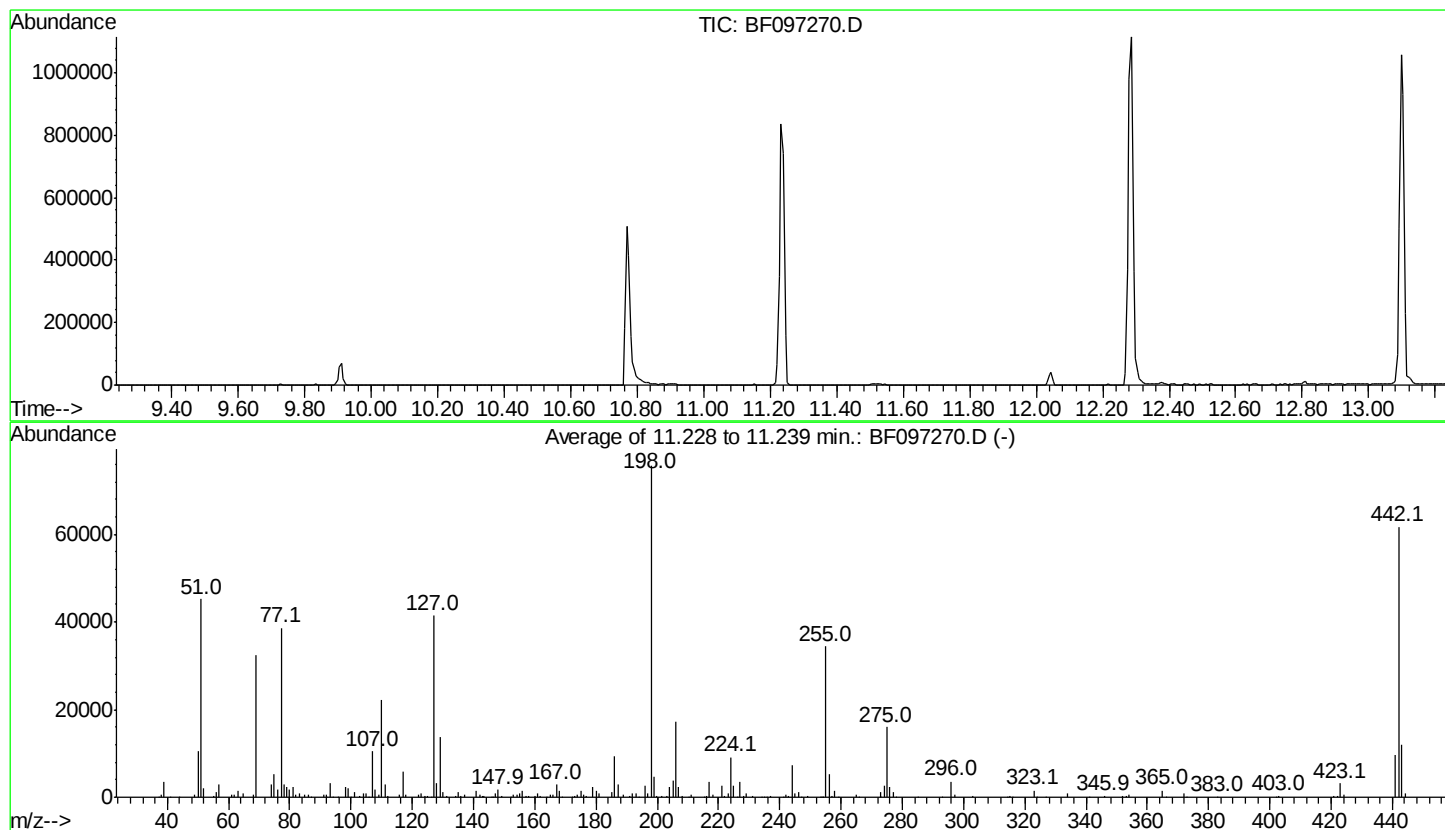

AutoFind: Scans 1588, 1589, 1590; Background Corrected with Scan 1583

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	59.7	45213	PASS
68	69	0.00	2	1.9	610	PASS
69	198	0.00	100	42.7	32309	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	54.7	41416	PASS
197	198	0.00	2	1.0	750	PASS
198	198	100	100	100.0	75706	PASS
199	198	5	9	6.3	4733	PASS
275	198	10	60	21.1	15997	PASS
365	198	1	100	2.0	1527	PASS
441	442	0.01	24	15.7	9716	PASS
442	198	50	100	81.5	61733	PASS
443	442	15	24	19.5	12056	PASS