

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF080221\
 Data File : BF124910.D
 Acq On : 2 Aug 2021 16:24
 Operator : JU/CG
 Sample : M3253-01
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 MH-1-COMP

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF072221.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BF124910.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	2.116	3	5	9	rVB	18601	18161	12.87%	2.135%
2	5.469	571	575	578	rBB	139159	117556	83.32%	13.820%
3	6.481	743	747	750	rBV	130040	120099	85.12%	14.119%
4	6.851	807	810	813	rBB	34881	26579	18.84%	3.125%
5	7.416	902	906	909	rBB	89452	77321	54.80%	9.090%
6	8.033	1009	1011	1015	rBB	3381	3151	2.23%	0.370%
7	8.139	1025	1029	1032	rBB	41262	36483	25.86%	4.289%
8	9.210	1207	1211	1214	rBV	193242	141094	100.00%	16.587%
9	9.886	1323	1326	1329	rBB	50220	42163	29.88%	4.957%
10	10.674	1457	1460	1463	rBV	80148	61912	43.88%	7.278%
11	11.374	1576	1579	1582	rBV	55255	40853	28.95%	4.803%
12	12.957	1844	1848	1851	rBB	144212	116966	82.90%	13.750%
13	14.009	2024	2027	2031	rBB	30950	25127	17.81%	2.954%
14	15.474	2272	2276	2280	rBB2	20067	23175	16.43%	2.724%




Sum of corrected areas: 850640

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF080221\
Data File : BF124910.D
Acq On : 2 Aug 2021 16:24
Operator : JU/CG
Sample : M3253-01
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
MH-1-COMP

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF072221.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

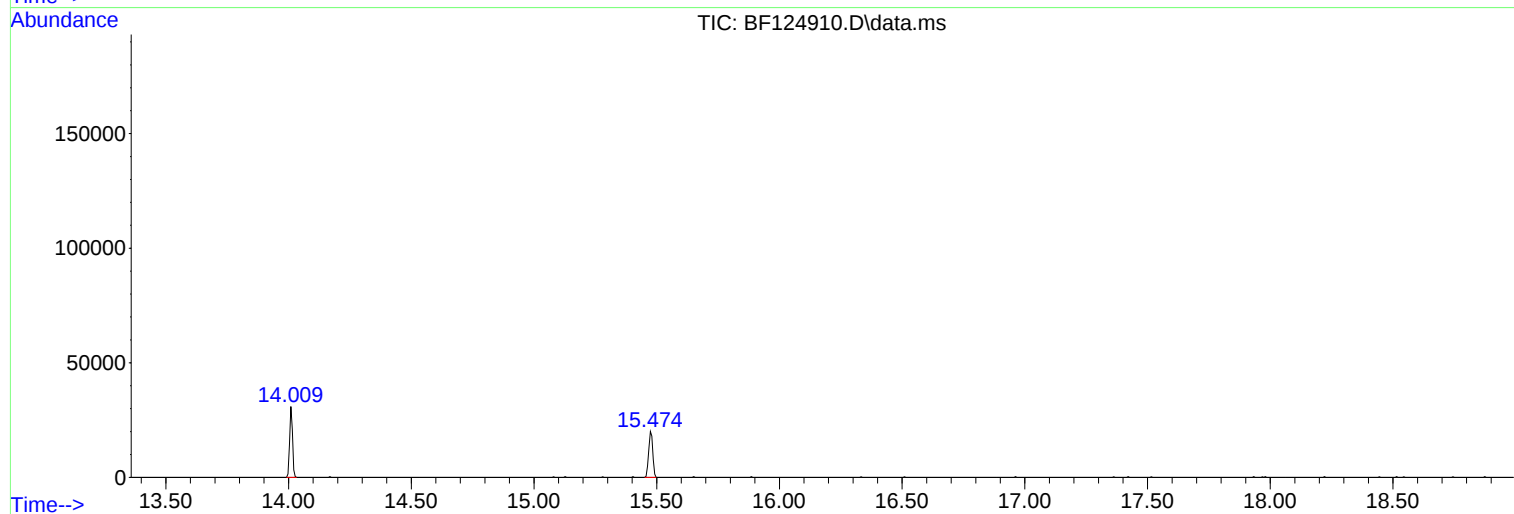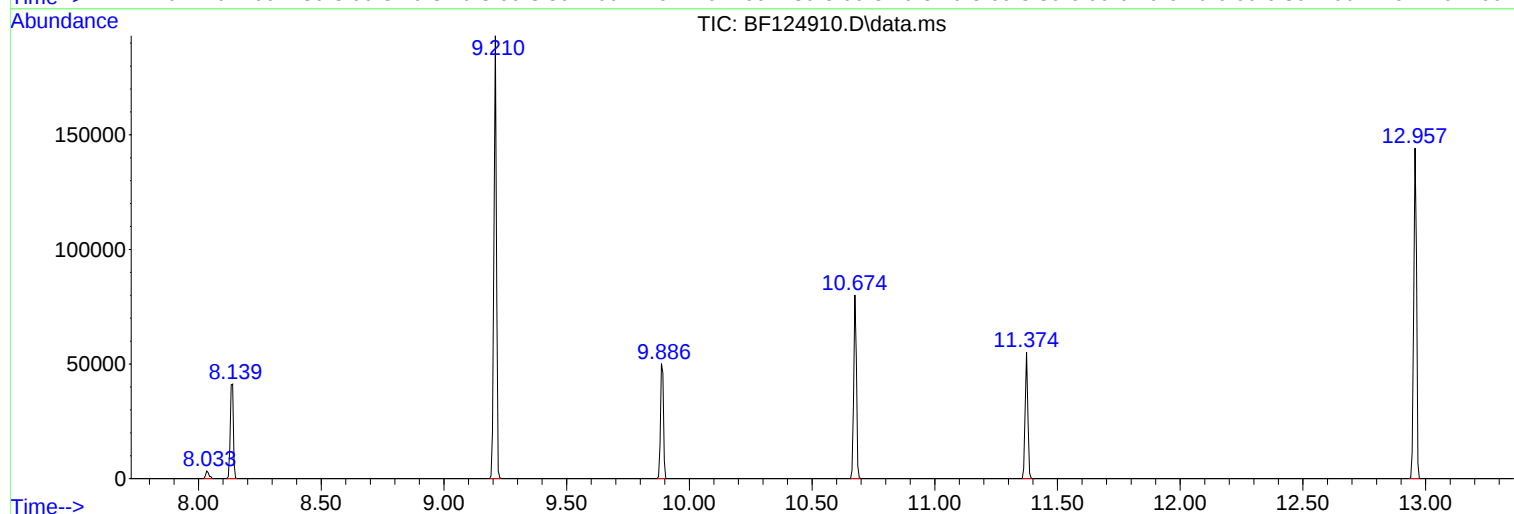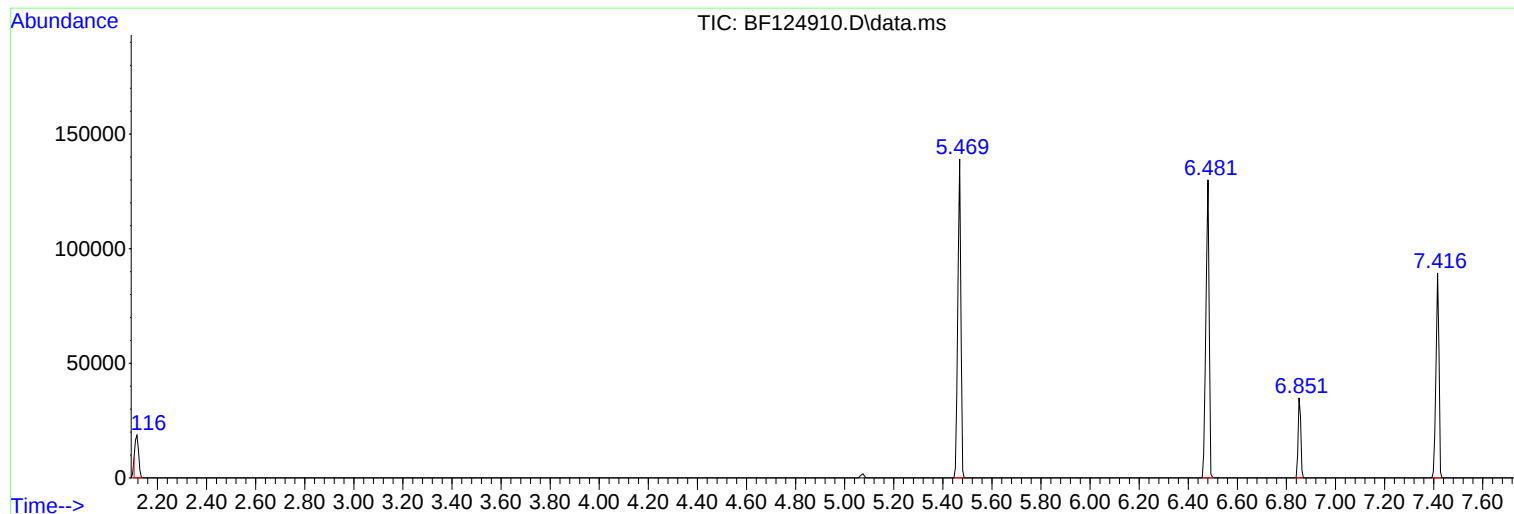

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF080221\
Data File : BF124910.D
Acq On : 2 Aug 2021 16:24
Operator : JU/CG
Sample : M3253-01
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
MH-1-COMP










Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF072221.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 Butane, 2-methoxy-2-methyl- Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
2.116	13.67 ng	18161	1,4-Dichlorobenzene-d4	6.851

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Butane, 2-methoxy-2-methyl-	102	C6H14O	000994-05-8	64
2			Isobutylamine	73	C4H11N	000078-81-9	5
3			1-Propanol, 2-methyl-	74	C4H10O	000078-83-1	4
4			1-Pentanamine	87	C5H13N	000110-58-7	4
5			2-Methyl-5-hexen-3-ol	114	C7H14O	032815-70-6	4

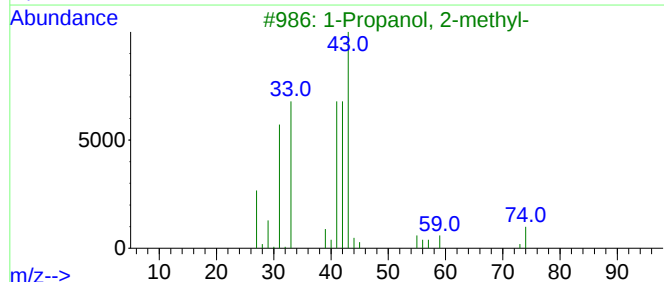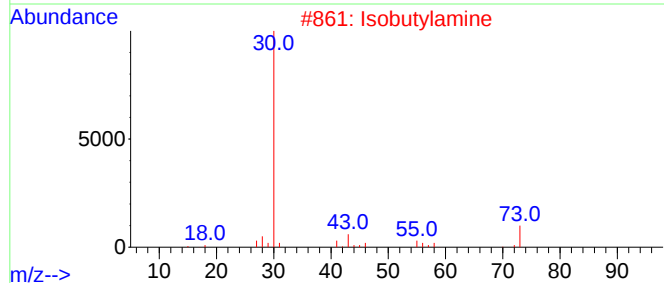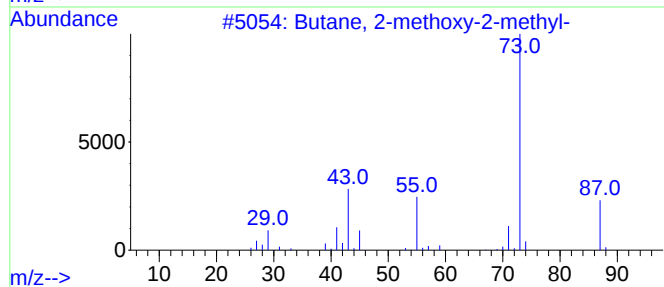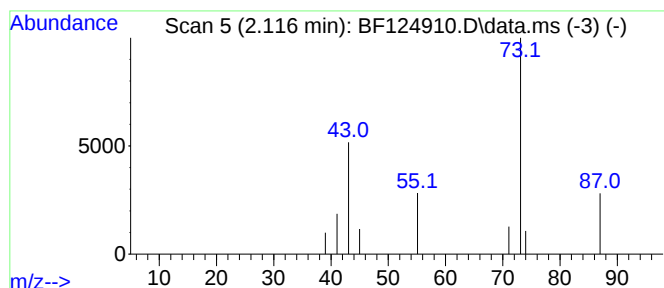

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF080221\
Data File : BF124910.D
Acq On : 2 Aug 2021 16:24
Operator : JU/CG
Sample : M3253-01
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
MH-1-COMP

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF072221.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Butane, 2-metho...	2.116	13.7	ng	18161	1	6.851	26579	20.0