
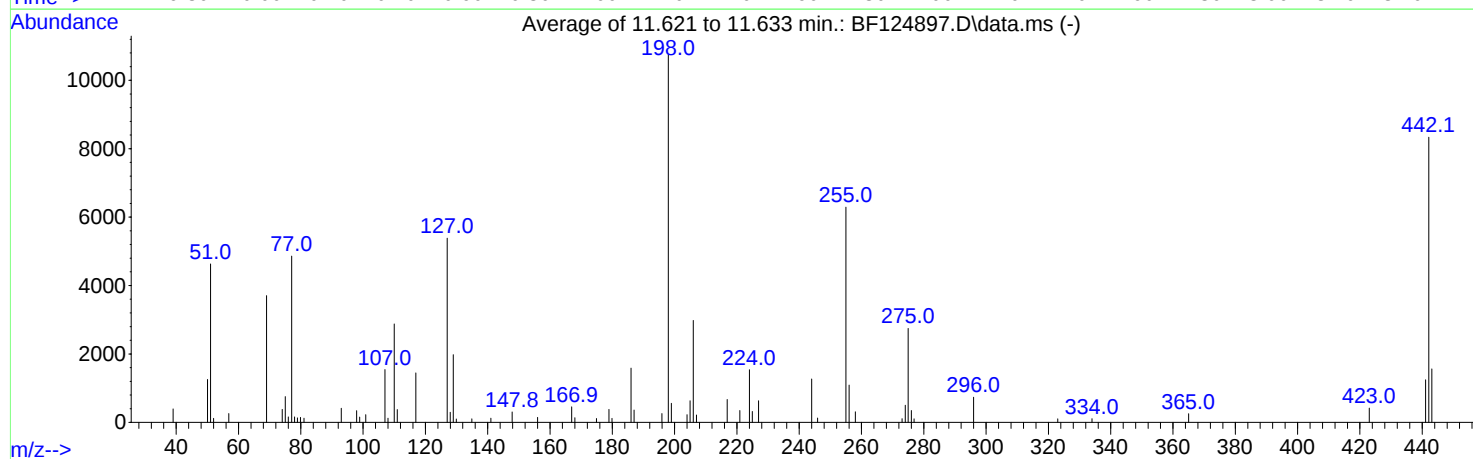


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF080221\
 Data File : BF124897.D
 Acq On : 2 Aug 2021 8:58
 Operator : JU/CG
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF072221.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Mon Aug 02 11:15:51 2021

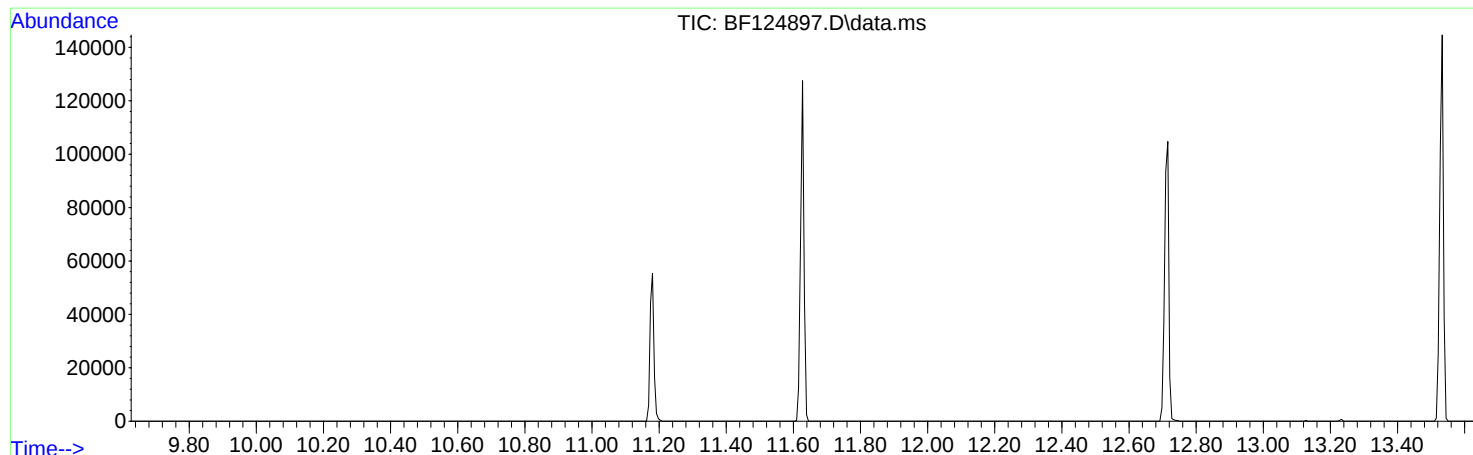




AutoFind: Scans 1621, 1622, 1623; Background Corrected with Scan 1616

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	43.1	4631	PASS
68	69	0.00	2	0.0	0	PASS
69	198	0.00	100	34.5	3707	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	50.1	5385	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	10755	PASS
199	198	5	9	5.2	556	PASS
275	198	10	60	25.5	2747	PASS
365	198	1	100	2.3	252	PASS
441	198	0.01	100	11.6	1245	PASS
442	442	50	100	100.0	8337	PASS
443	442	15	24	18.7	1563	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF080221\
 Data File : BF124897.D
 Acq On : 2 Aug 2021 8:58
 Operator : JU/CG
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Quant Time: Aug 02 11:04:32 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF072221.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Aug 02 02:31:45 2021
 Response via : Initial Calibration

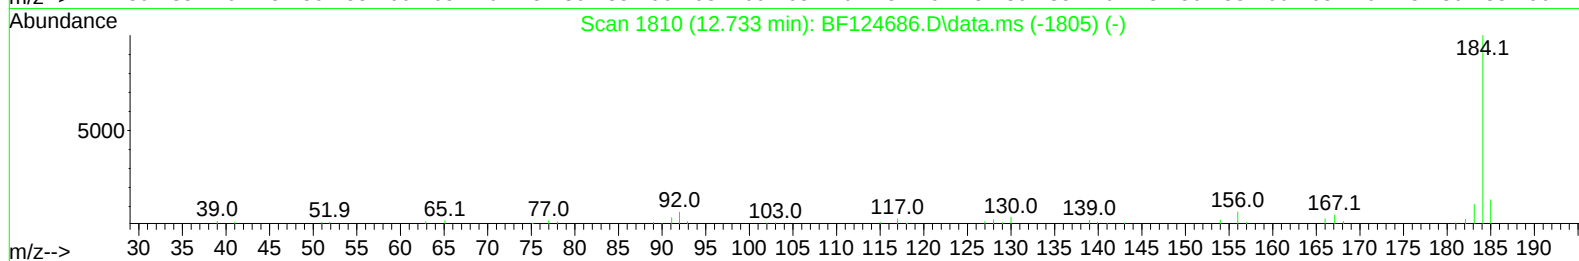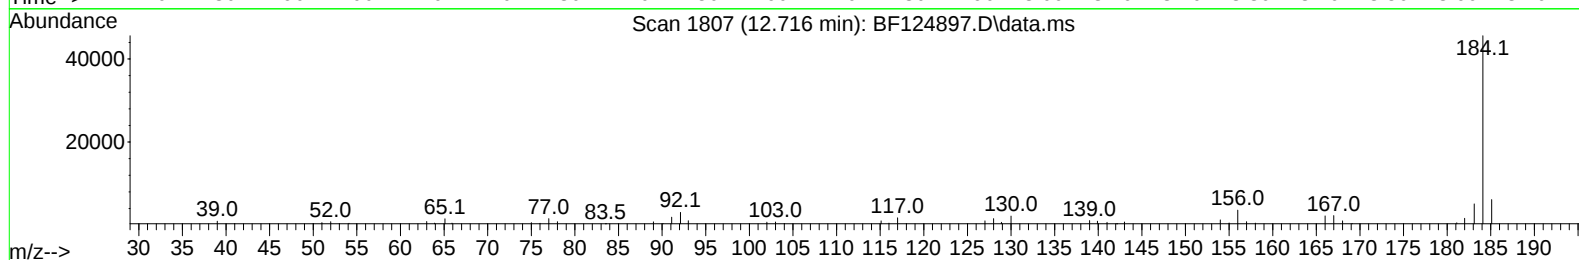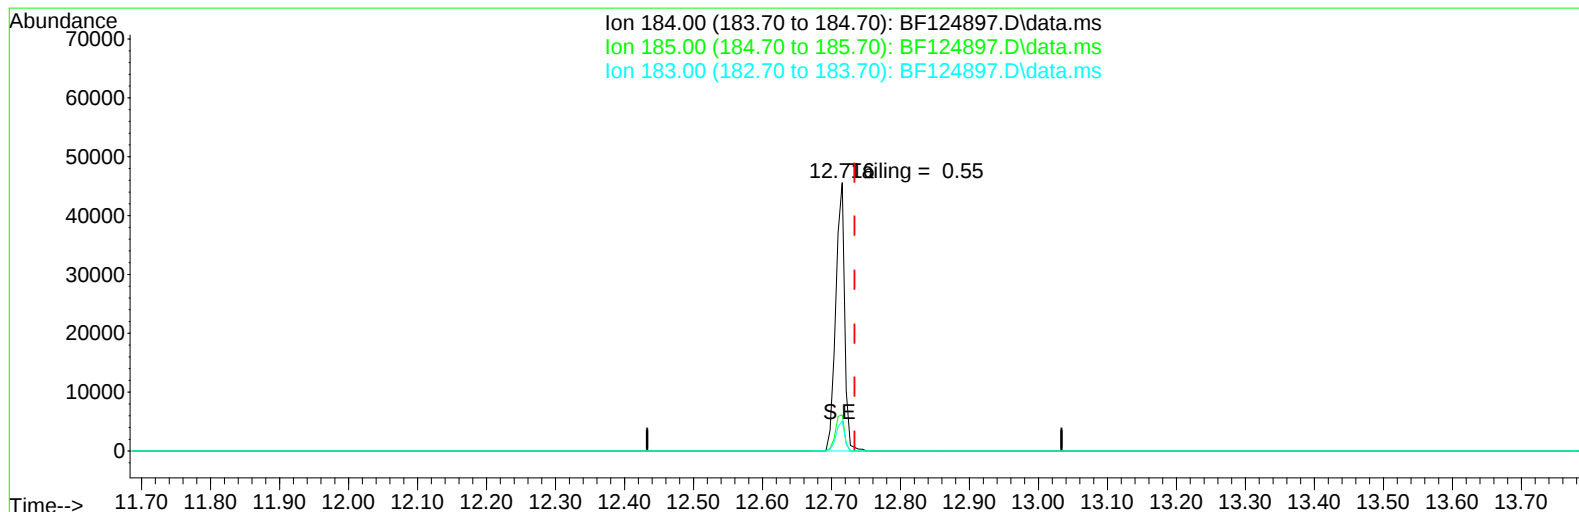

TIC: BF124897.D\data.ms

(77) Benzidine

12.716min (-0.018) 0.00 ng




response 40592

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	13.50	13.47
183.00	10.10	11.23
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF080221\
Data File : BF124897.D
Acq On : 2 Aug 2021 8:58
Operator : JU/CG
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Aug 02 11:04:32 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF072221.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Aug 02 02:31:45 2021
Response via : Initial Calibration

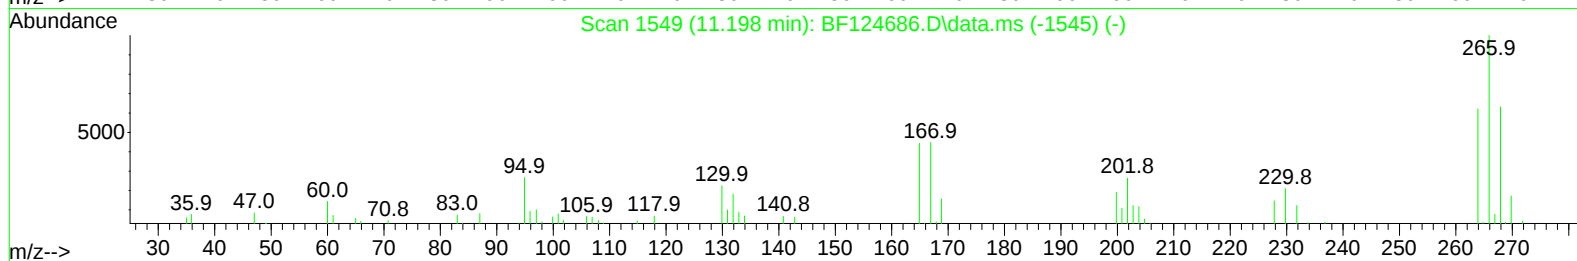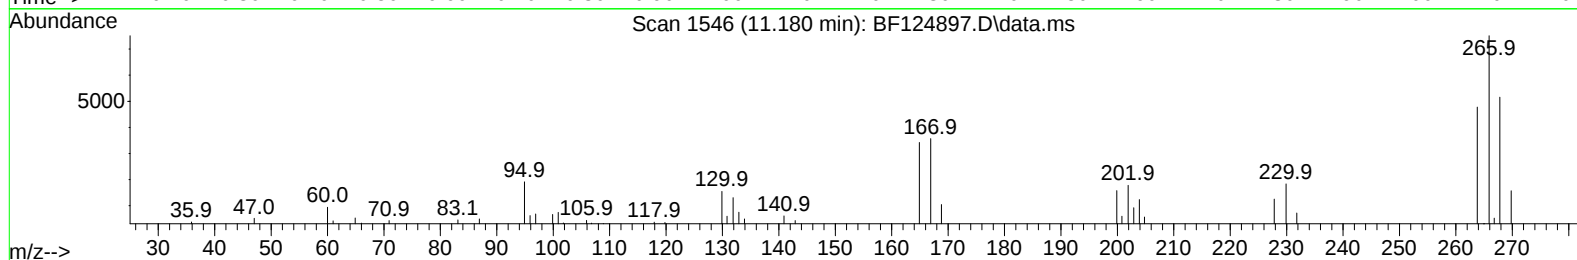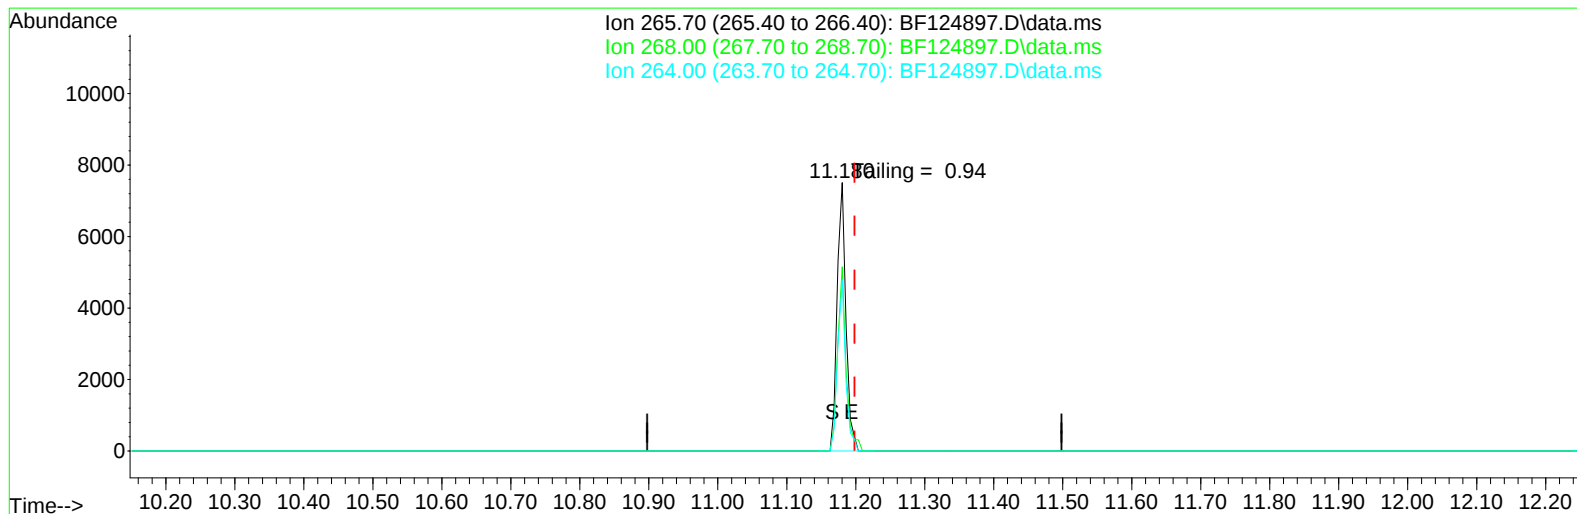

TIC: BF124897.D\data.ms

(70) Pentachlorophenol (C)

11.180min (-0.018) 0.00 ng

response 6622

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	61.10	68.64
264.00	69.90	63.62
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
2/8/2021	BNA_F	<u>BF124897.D</u>
Compound Name	Response	Retention Time
DDT	23375	13.53
DDD	244	13.23
DDE	0	12.71
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
244	23619	1.03