
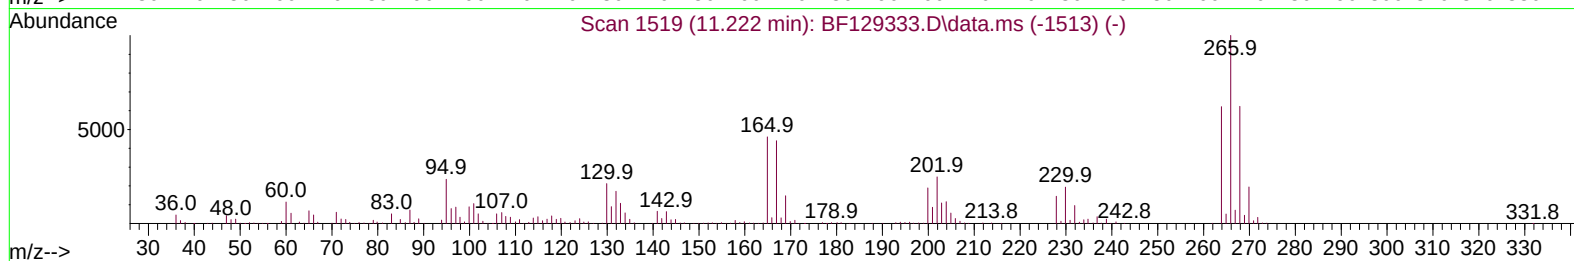
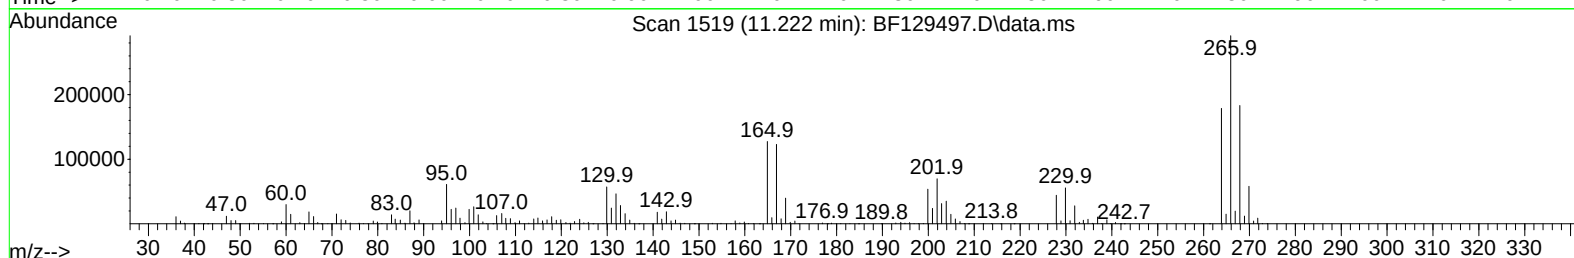


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF080222\
 Data File : BF129497.D
 Acq On : 02 Aug 2022 09:15
 Operator : CG\JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Aug 02 18:20:40 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF072522.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Aug 02 01:11:25 2022
 Response via : Initial Calibration

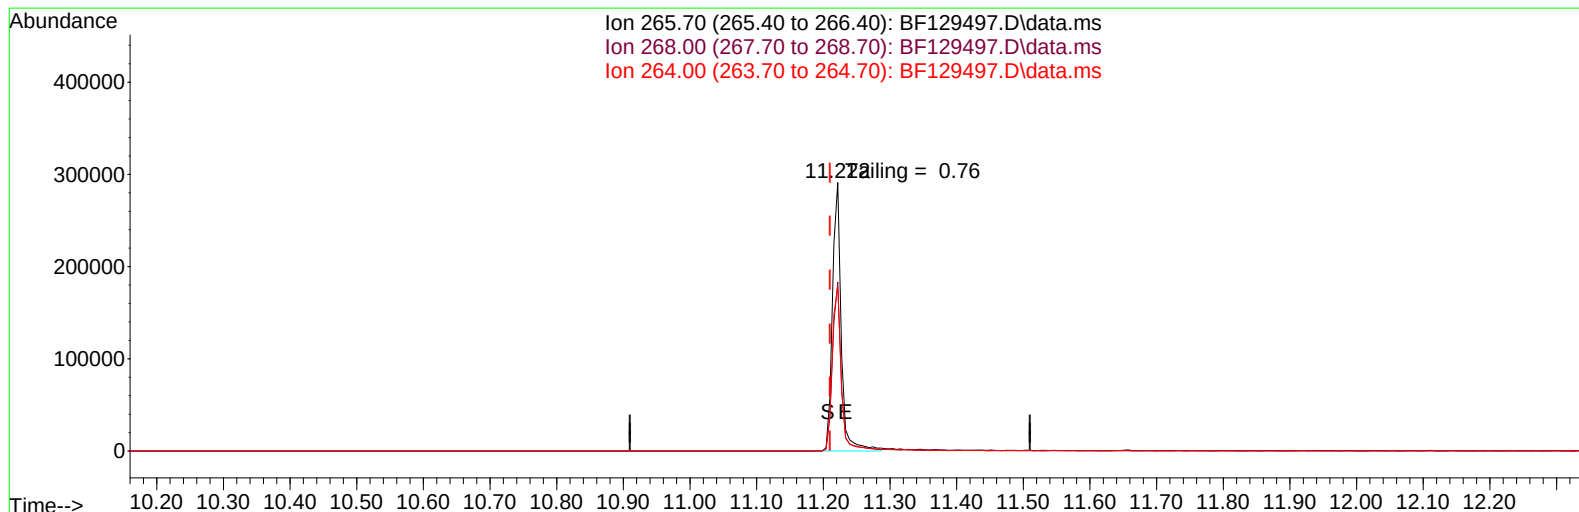

TIC: BF129497.D\data.ms

(70) Pentachlorophenol (C)




11.222min (+ 0.012) 542012.78 ng

response 272694

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.70	62.93
264.00	61.80	61.37
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF080222\
 Data File : BF129497.D
 Acq On : 02 Aug 2022 09:15
 Operator : CG\JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Aug 02 18:20:40 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF072522.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Aug 02 01:11:25 2022
 Response via : Initial Calibration

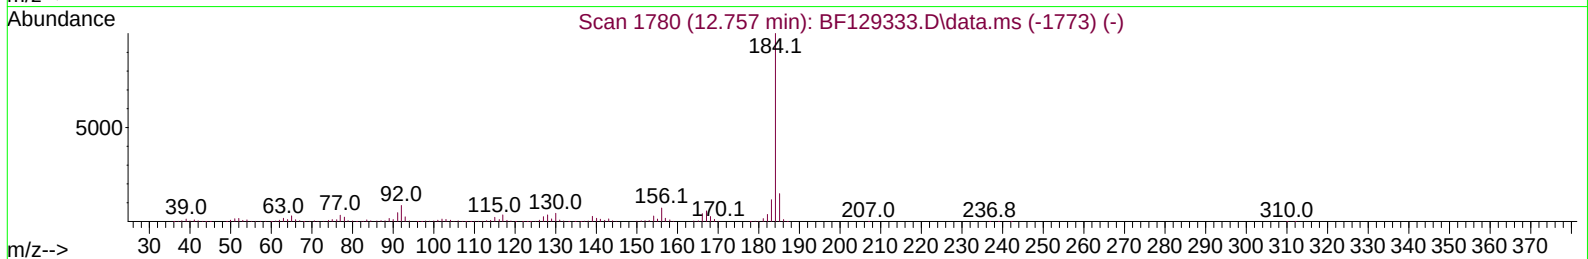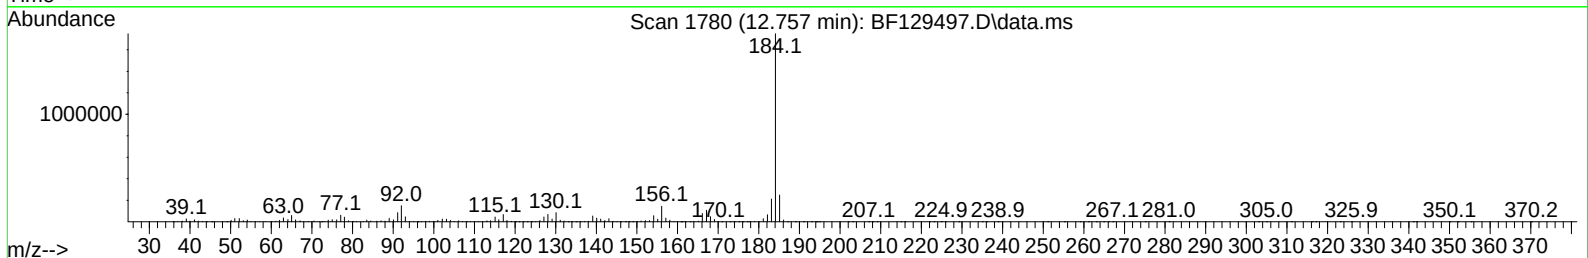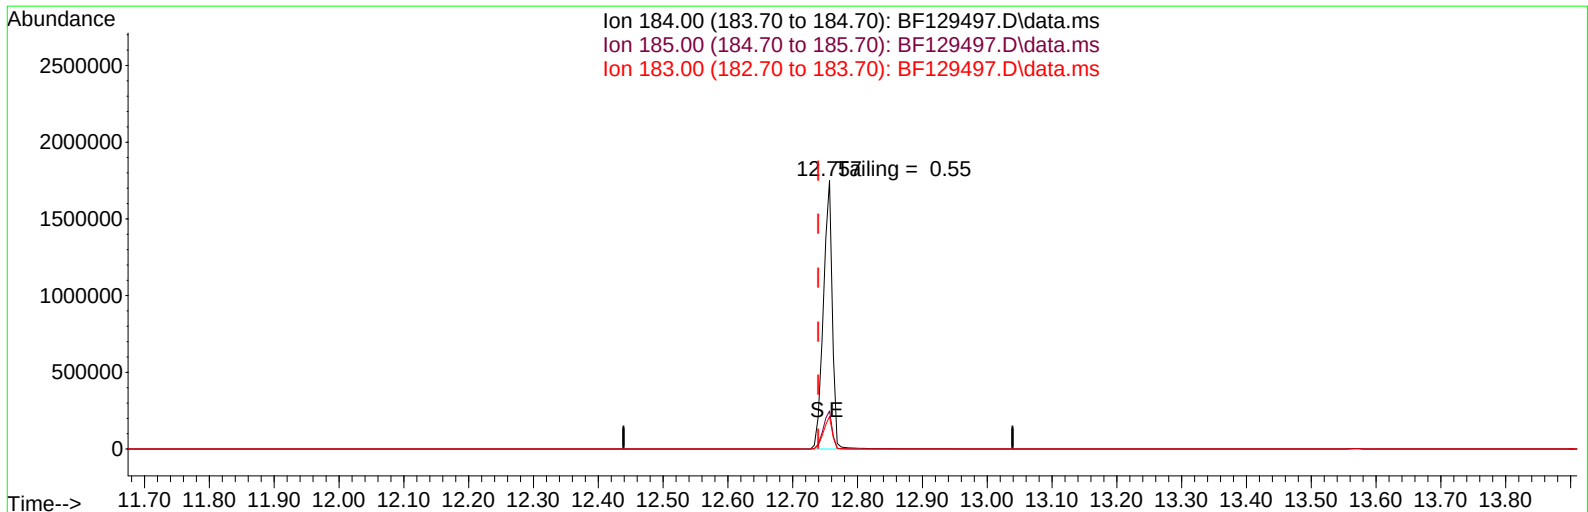

TIC: BF129497.D\data.ms

(77) Benzidine**12.757min (+ 0.018) 61368.37 ng****response 1693202**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.90	14.23
183.00	11.60	12.13
0.00	0.00	0.00