

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF080222\
 Data File : BF129504.D
 Acq On : 02 Aug 2022 13:04
 Operator : CG\JU
 Sample : N3927-06
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 RVE-79D

Quant Time: Aug 02 17:37:34 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF072522.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Aug 02 01:11:25 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	6.875	152	149837	20.000	ng	0.00
21) Naphthalene-d8	8.157	136	605610	20.000	ng	0.00
39) Acenaphthene-d10	9.916	164	310091	20.000	ng	0.00
64) Phenanthrene-d10	11.404	188	491643	20.000	ng	# 0.00
76) Chrysene-d12	14.051	240	282031	20.000	ng	0.00
86) Perylene-d12	15.533	264	311172	20.000	ng	0.00
System Monitoring Compounds						
5) 2-Fluorophenol	5.510	112	877783	95.431	ng	0.00
7) Phenol-d6	6.522	99	1103292	95.428	ng	0.00
23) Nitrobenzene-d5	7.439	82	697164	62.841	ng	0.00
42) 2,4,6-Tribromophenol	10.710	330	277300	93.013	ng	0.00
45) 2-Fluorobiphenyl	9.233	172	1274556	63.584	ng	0.00
79) Terphenyl-d14	12.986	244	1067495	71.408	ng	0.00


Target Compounds Qvalue


 (#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF080222\
Data File : BF129504.D
Acq On : 02 Aug 2022 13:04
Operator : CG\JU
Sample : N3927-06
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
RVE-79D

Quant Time: Aug 02 17:37:34 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF072522.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Aug 02 01:11:25 2022
Response via : Initial Calibration




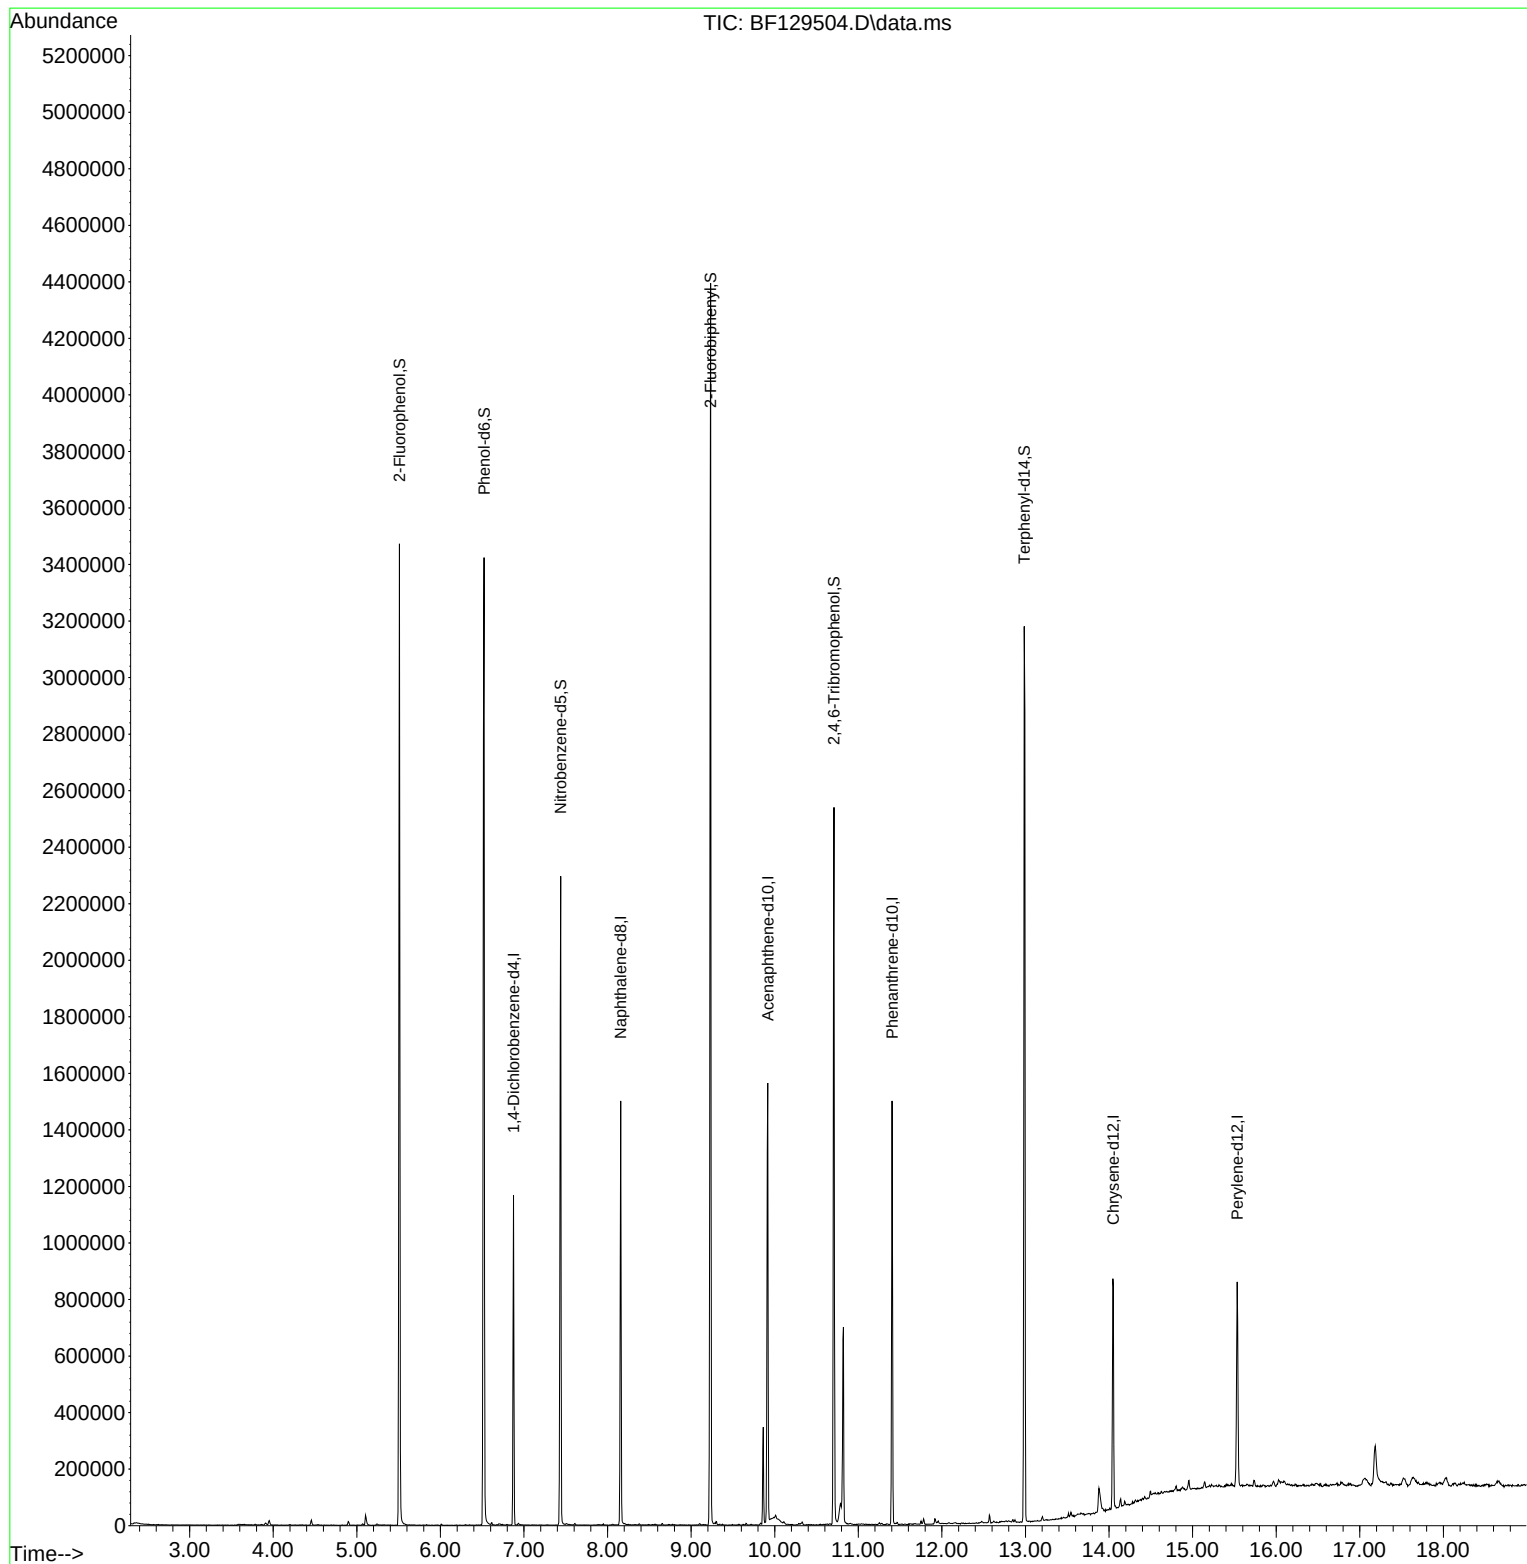


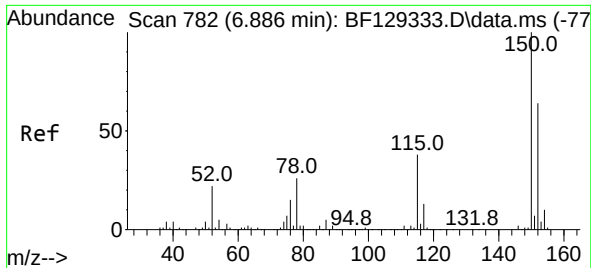

#1
1,4-Dichlorobenzene-d4
Concen: 20.000 ng
RT: 6.875 min Scan# 782
Delta R.T. -0.000 min
Lab File: BF129504.D
Acq: 02 Aug 2022 13:04




Instrument :
BNA_F
ClientSampleId :
RVE-79D


Tgt Ion:152 Resp: 149837
Ion Ratio Lower Upper
152 100
150 158.3 123.7 185.5
115 64.0 49.9 74.9

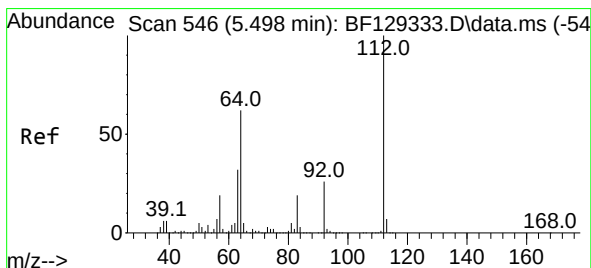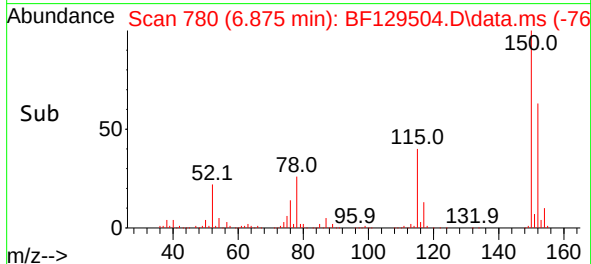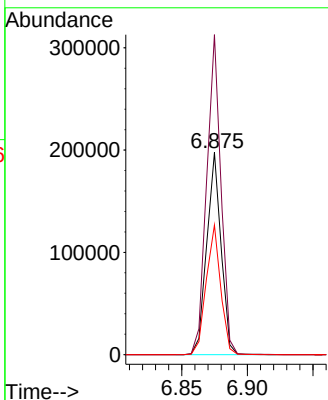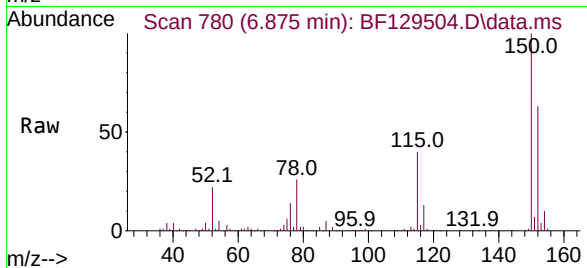

#5
2-Fluorophenol
Concen: 95.431 ng
RT: 5.510 min Scan# 548
Delta R.T. 0.006 min
Lab File: BF129504.D
Acq: 02 Aug 2022 13:04

Tgt Ion:112 Resp: 877783
Ion Ratio Lower Upper
112 100
64 61.1 53.3 79.9
63 32.0 28.0 42.0


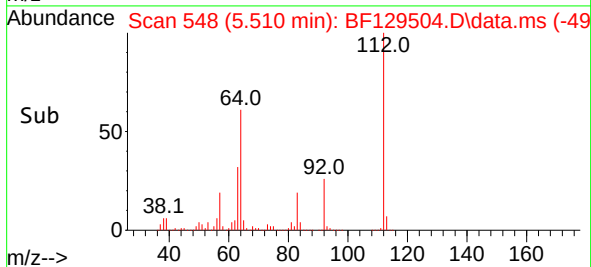
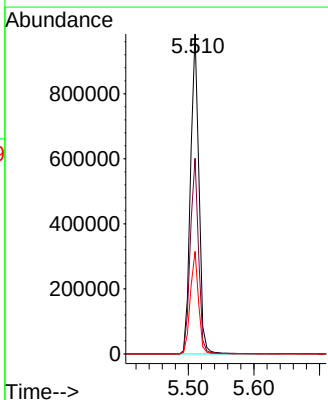
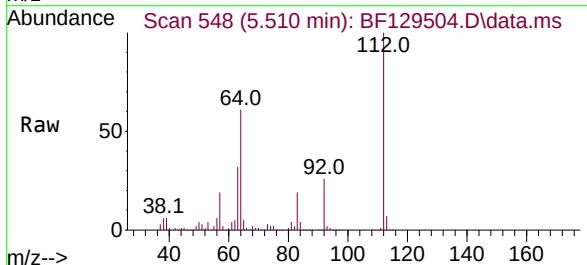


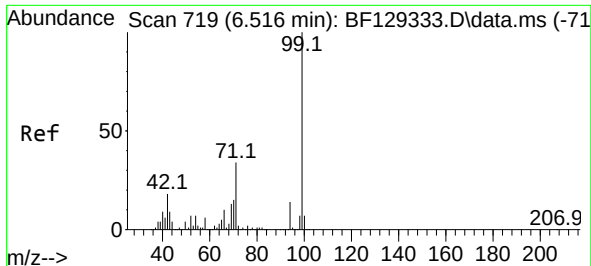

#7
Phenol-d6
Concen: 95.428 ng
RT: 6.522 min Scan# 71
Delta R.T. -0.000 min
Lab File: BF129504.D
Acq: 02 Aug 2022 13:04




Instrument :
BNA_F
ClientSampleId :
RVE-79D


Tgt Ion: 99 Resp: 1103292
Ion Ratio Lower Upper
99 100
42 18.0 17.3 25.9
71 34.3 28.9 43.3

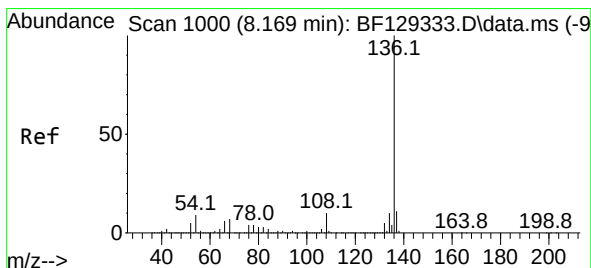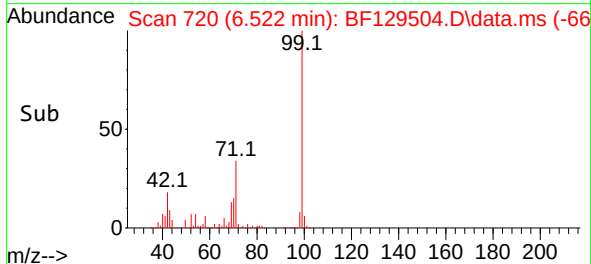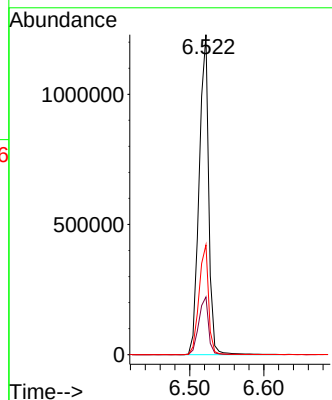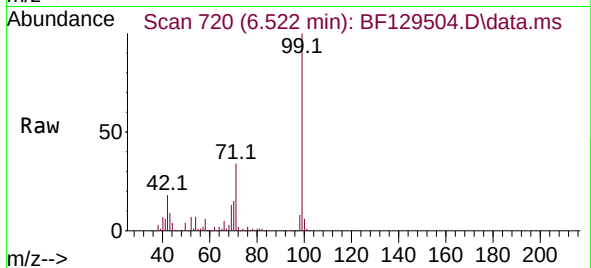

#21
Naphthalene-d8
Concen: 20.000 ng
RT: 8.157 min Scan# 998
Delta R.T. -0.006 min
Lab File: BF129504.D
Acq: 02 Aug 2022 13:04

Tgt Ion: 136 Resp: 605610
Ion Ratio Lower Upper
136 100
137 11.3 8.8 13.2
54 7.7 7.5 11.3
68 5.7 4.7 7.1


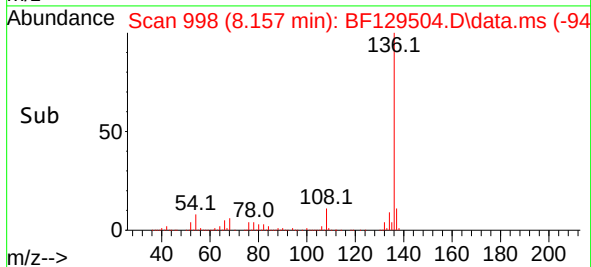
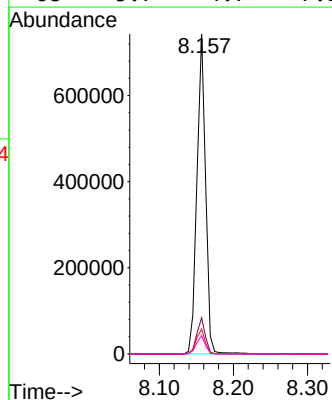
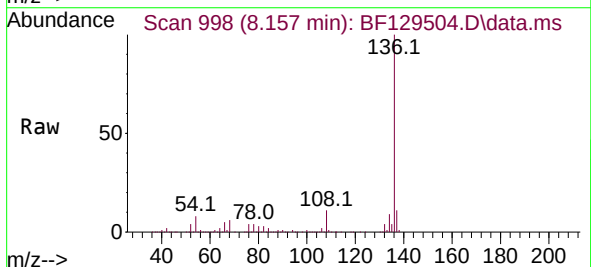


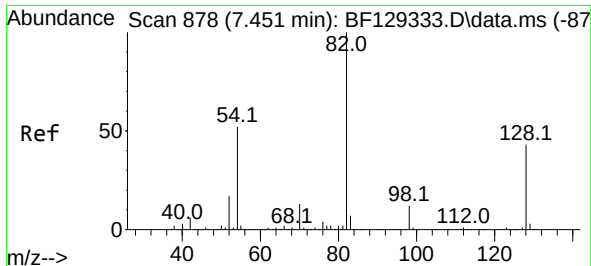

#23
Nitrobenzene-d5
Concen: 62.841 ng
RT: 7.439 min Scan# 81
Delta R.T. -0.006 min
Lab File: BF129504.D
Acq: 02 Aug 2022 13:04




Instrument :
BNA_F
ClientSampleId :
RVE-79D


Tgt Ion: 82 Resp: 697164
Ion Ratio Lower Upper
82 100
128 45.4 34.0 51.0
54 50.3 46.9 70.3

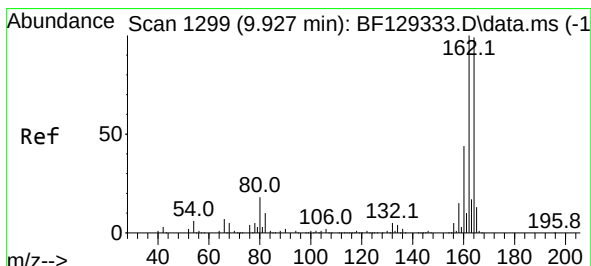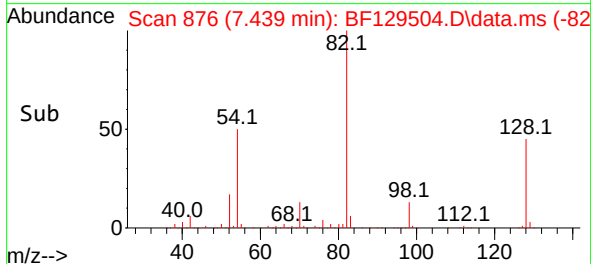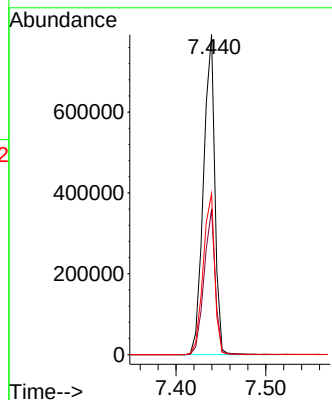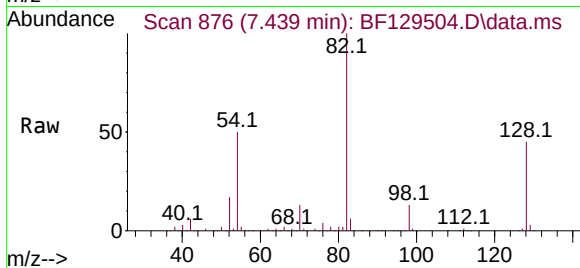

#39
Acenaphthene-d10
Concen: 20.000 ng
RT: 9.916 min Scan# 1297
Delta R.T. -0.000 min
Lab File: BF129504.D
Acq: 02 Aug 2022 13:04

Tgt Ion: 164 Resp: 310091
Ion Ratio Lower Upper
164 100
162 103.0 79.5 119.3
160 44.4 34.2 51.4

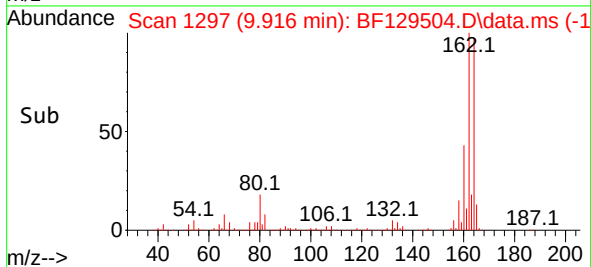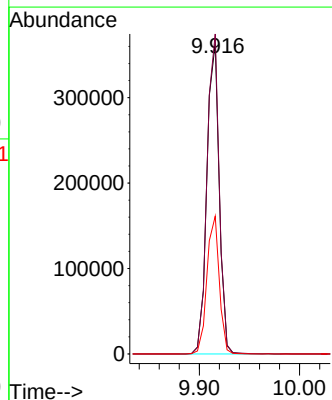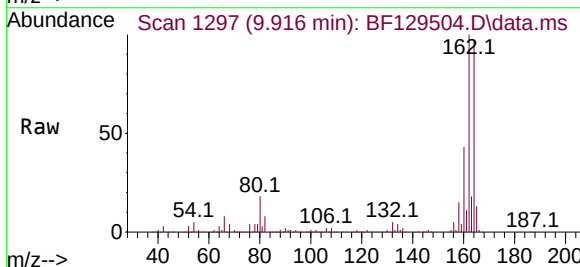

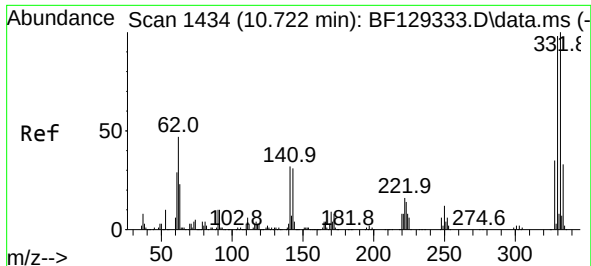

#42

2,4,6-Tribromophenol

Concen: 93.013 ng

RT: 10.710 min Scan# 1434

Delta R.T. -0.000 min

Lab File: BF129504.D

Acq: 02 Aug 2022 13:04

Instrument :

BNA_F

ClientSampleId :

RVE-79D





Tgt Ion:330 Resp: 277300

Ion Ratio Lower Upper

330 100

332 102.2 76.8 115.2

141 36.2 28.0 42.0

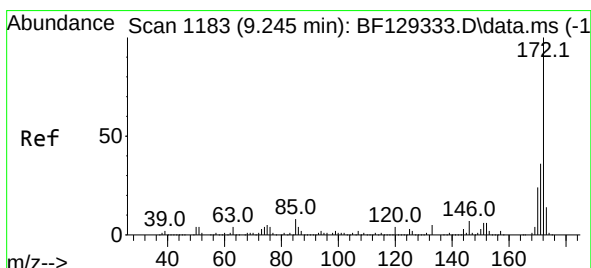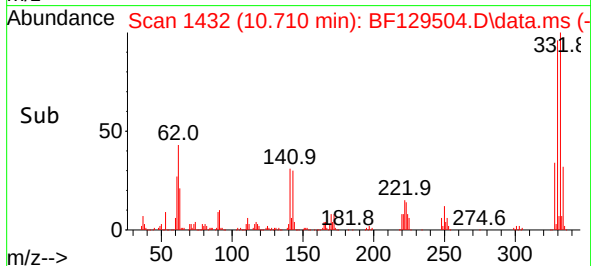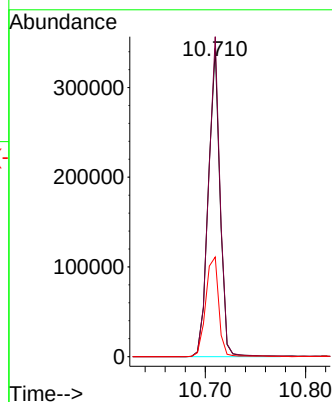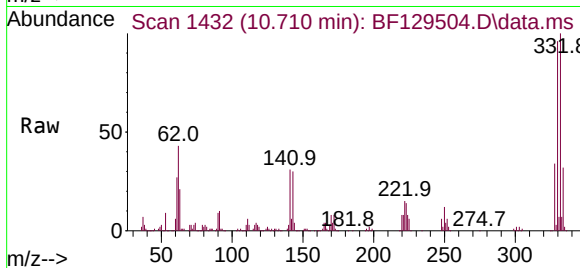

#45

2-Fluorobiphenyl

Concen: 63.584 ng

RT: 9.233 min Scan# 1181

Delta R.T. -0.000 min

Lab File: BF129504.D

Acq: 02 Aug 2022 13:04




Tgt Ion:172 Resp: 1274556


Ion Ratio Lower Upper

172 100

171 35.2 28.8 43.2

170 23.7 19.8 29.8


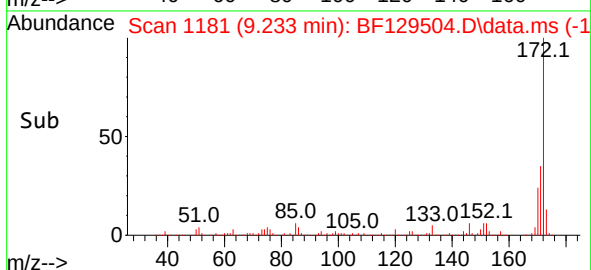
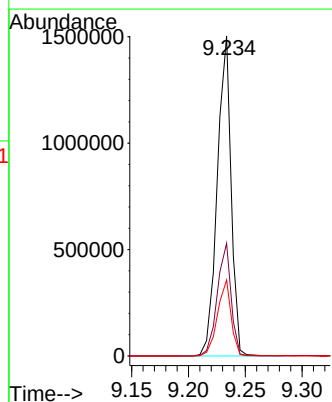
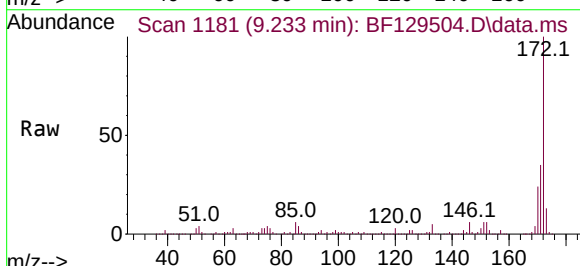


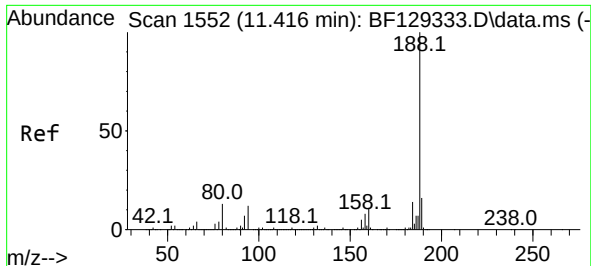

#64
Phenanthrene-d10
Concen: 20.000 ng
RT: 11.404 min Scan# 11
Delta R.T. -0.000 min
Lab File: BF129504.D
Acq: 02 Aug 2022 13:04




Instrument :
BNA_F
ClientSampleId :
RVE-79D


Tgt Ion:188 Resp: 491643
Ion Ratio Lower Upper
188 100
94 10.4 7.0 10.6
80 11.5 7.6 11.4#

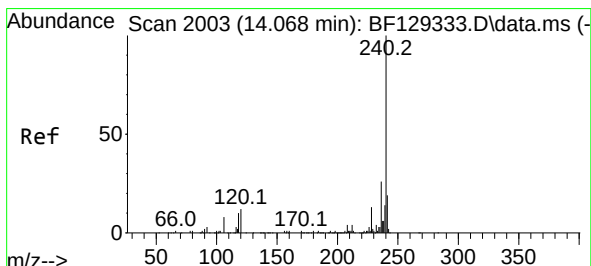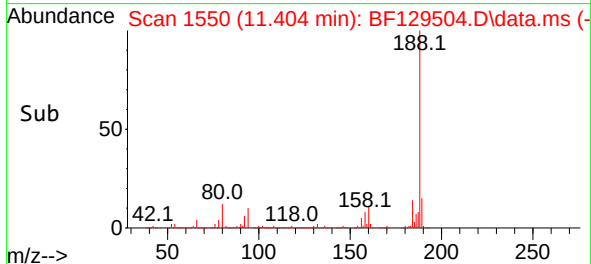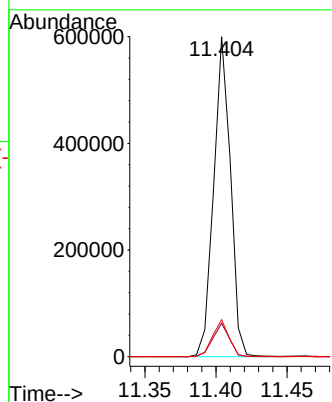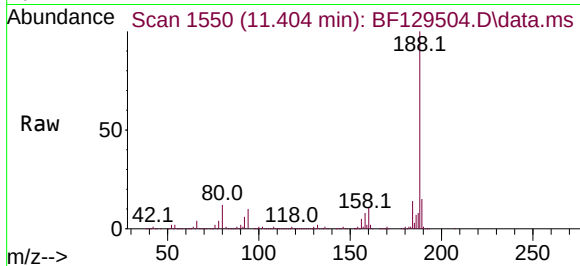

#76
Chrysene-d12
Concen: 20.000 ng
RT: 14.051 min Scan# 2000
Delta R.T. -0.000 min
Lab File: BF129504.D
Acq: 02 Aug 2022 13:04

Tgt Ion:240 Resp: 282031
Ion Ratio Lower Upper
240 100
120 10.4 8.9 13.3
236 25.3 20.8 31.2


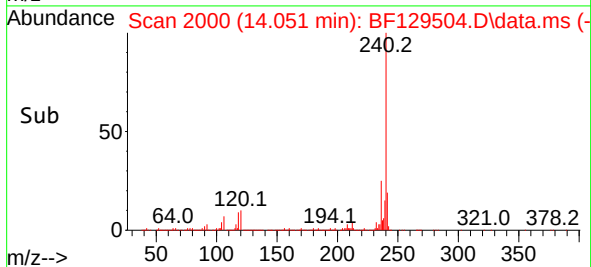
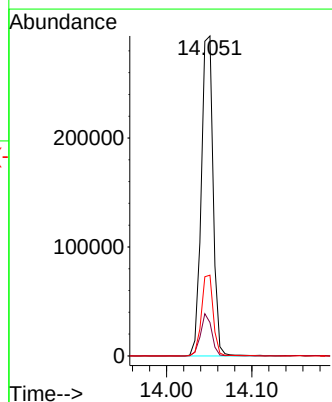
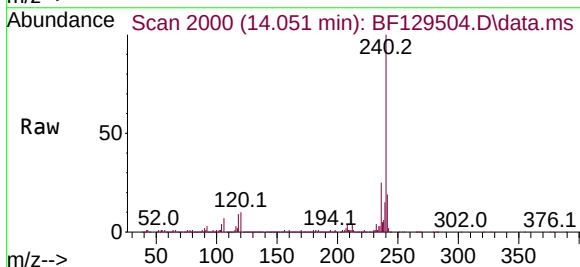


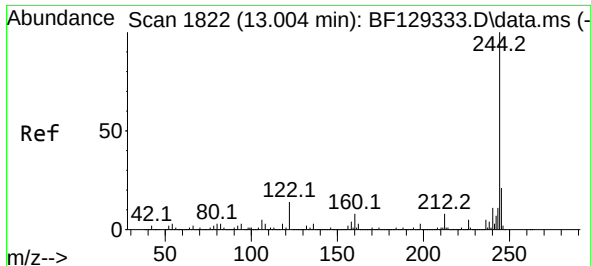

#79
 Terphenyl-d14
 Concen: 71.408 ng
 RT: 12.986 min Scan# 1819
 Delta R.T. -0.000 min
 Lab File: BF129504.D
 Acq: 02 Aug 2022 13:04

Instrument :
 BNA_F
 ClientSampleId :
 RVE-79D

Tgt Ion:244 Resp: 1067495
 Ion Ratio Lower Upper
 244 100
 212 7.0 6.1 9.1
 122 13.5 8.8 13.2#

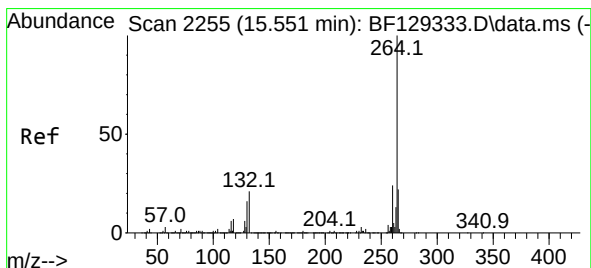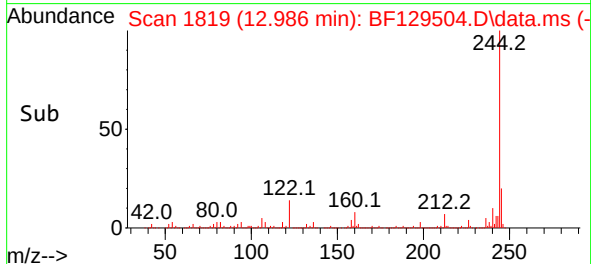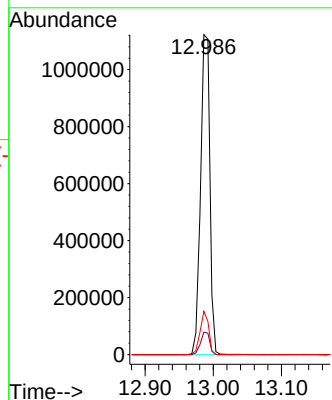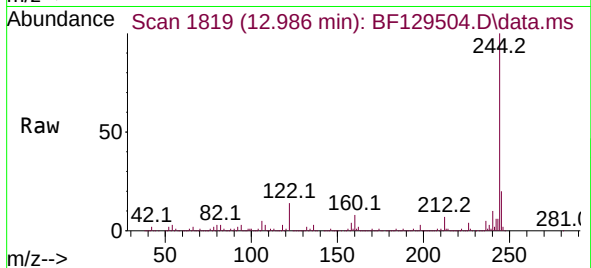

#86
 Perylene-d12
 Concen: 20.000 ng
 RT: 15.533 min Scan# 2252
 Delta R.T. 0.006 min
 Lab File: BF129504.D
 Acq: 02 Aug 2022 13:04

Tgt Ion:264 Resp: 311172
 Ion Ratio Lower Upper
 264 100
 260 24.9 18.4 27.6
 265 21.7 17.2 25.8

