

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF080222\
 Data File : BF129519.D
 Acq On : 02 Aug 2022 21:36
 Operator : CG\JU
 Sample : N3927-19
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 RVE-92

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF072522.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BF129519.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	4.446	365	367	379	rBV	61189	97877	2.11%	0.292%
2	5.116	478	481	490	rVB	45255	58577	1.26%	0.175%
3	5.516	544	549	552	rBV	4146168	4082550	87.90%	12.187%
4	6.522	715	720	723	rBV	4211903	4106112	88.41%	12.257%
5	6.875	776	780	783	rBV	1251484	955049	20.56%	2.851%
6	7.439	871	876	879	rBV	2876444	2709204	58.33%	8.087%
7	8.157	994	998	1001	rBV	1621780	1242489	26.75%	3.709%
8	9.233	1176	1181	1184	rBV	5641669	4644519	100.00%	13.864%
9	9.916	1293	1297	1300	rBV	1353328	1251524	26.95%	3.736%
10	10.704	1428	1431	1435	rBV	2320116	2190848	47.17%	6.540%
11	11.404	1546	1550	1553	rBV	1210633	964444	20.77%	2.879%
12	11.886	1629	1632	1633	rBV	68746	63393	1.36%	0.189%
13	11.922	1633	1638	1642	rVB2	499613	489456	10.54%	1.461%
14	12.616	1753	1756	1765	rBV	178149	258073	5.56%	0.770%
15	12.845	1789	1795	1801	rBV	186980	210972	4.54%	0.630%
16	12.986	1815	1819	1822	rBV	3420099	2906226	62.57%	8.675%
17	13.874	1967	1970	1977	rBV2	317721	428956	9.24%	1.280%
18	14.045	1995	1999	2002	rBV	943083	896471	19.30%	2.676%
19	14.068	2002	2003	2009	rVB	79163	72005	1.55%	0.215%
20	14.192	2021	2024	2027	rBV	50079	62531	1.35%	0.187%
21	14.492	2073	2075	2077	rBV	96682	94792	2.04%	0.283%
22	14.951	2150	2153	2158	rVB	270791	275768	5.94%	0.823%
23	15.098	2174	2178	2181	rBV	62340	101847	2.19%	0.304%
24	15.145	2182	2186	2189	rVV	171433	222482	4.79%	0.664%
25	15.186	2190	2193	2209	rVB4	100264	262590	5.65%	0.784%
26	15.533	2247	2252	2257	rBV	617885	743586	16.01%	2.220%
27	15.733	2283	2286	2291	rVB	151164	197124	4.24%	0.588%
28	15.968	2322	2326	2332	rVB	193425	290895	6.26%	0.868%
29	16.780	2460	2464	2471	rVB2	120647	215570	4.64%	0.643%
30	17.186	2526	2533	2546	rBV	1121231	2442602	52.59%	7.291%
31	17.521	2586	2590	2601	rVB5	211156	473761	10.20%	1.414%
32	18.033	2671	2677	2684	rVB3	207930	487845	10.50%	1.456%




Sum of corrected areas: 33500138

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF080222\
Data File : BF129519.D
Acq On : 02 Aug 2022 21:36
Operator : CG\JU
Sample : N3927-19
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
RVE-92

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF072522.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library :
TIC Integration Parameters: rteint.p

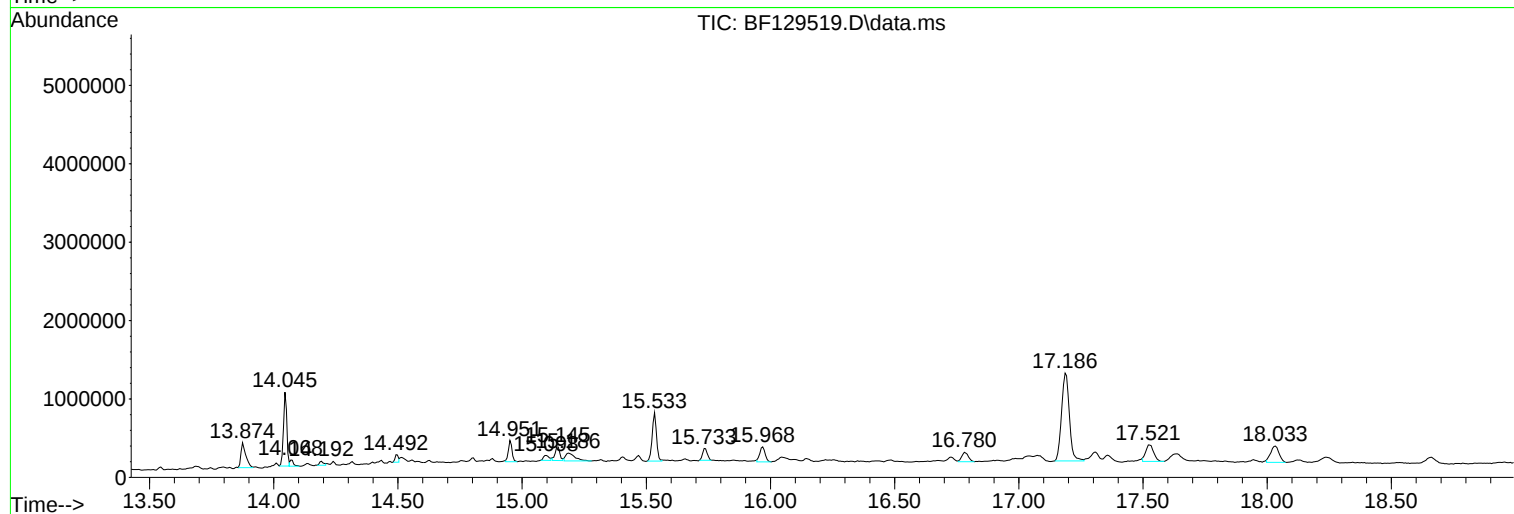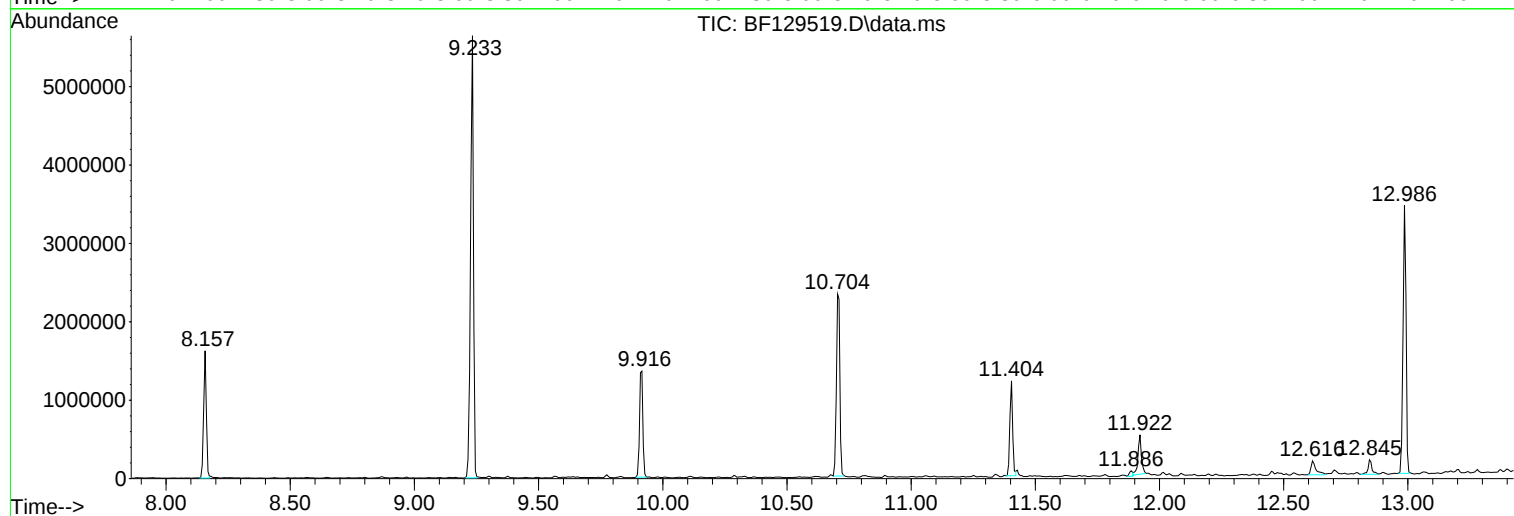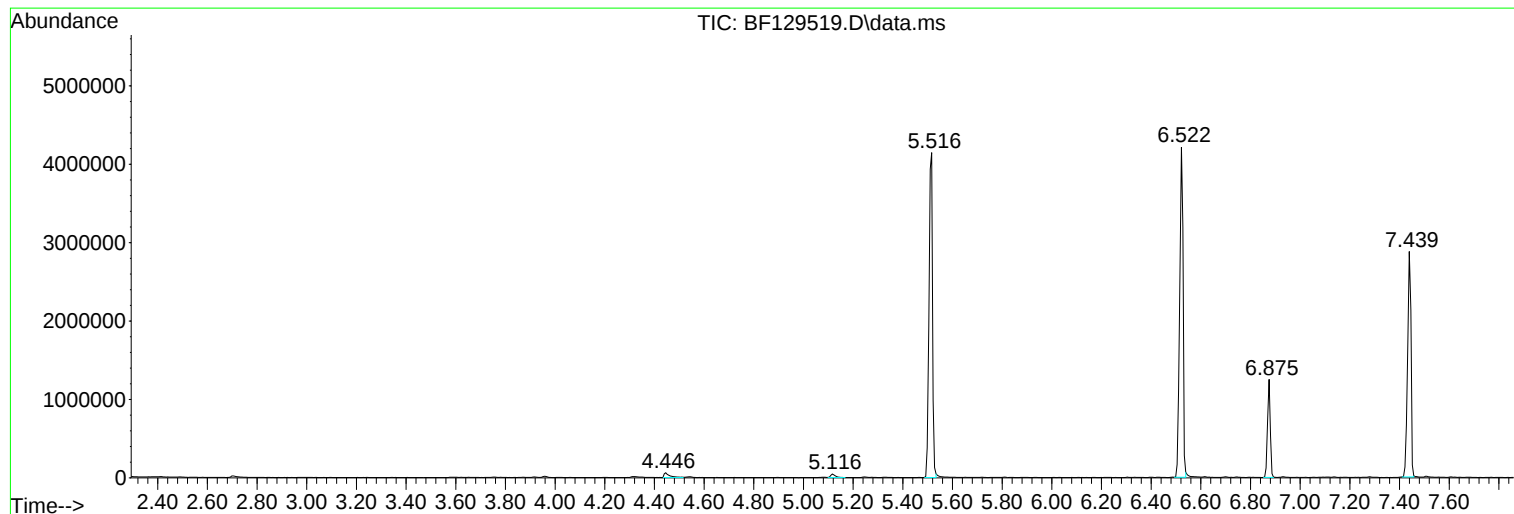

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF080222\
Data File : BF129519.D
Acq On : 02 Aug 2022 21:36
Operator : CG\JU
Sample : N3927-19
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
RVE-92

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF072522.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library :
TIC Integration Parameters: rteint.p

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF080222\
Data File : BF129519.D
Acq On : 02 Aug 2022 21:36
Operator : CG\JU
Sample : N3927-19
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
RVE-92

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF072522.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library :
TIC Integration Parameters: rteint.p

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------