

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF080222\
 Data File : BF129524.D
 Acq On : 03 Aug 2022 00:19
 Operator : CG\JU
 Sample : N3989-01
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 OK-04-080122

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF072522.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BF129524.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.098	474	478	485	rVB	32220	34250	1.71%	0.178%
2	5.510	544	548	564	rBV	2148129	2004632	100.00%	10.435%
3	6.522	716	720	733	rBV	2147812	1946252	97.09%	10.131%
4	6.875	777	780	784	rBV	1144638	868758	43.34%	4.522%
5	7.439	872	876	879	rBV	1462973	1182863	59.01%	6.157%
6	8.157	995	998	1001	rBV	1295243	1032697	51.52%	5.376%
7	9.233	1177	1181	1184	rBV	2271081	1962100	97.88%	10.214%
8	9.774	1270	1273	1278	rBV	84390	75565	3.77%	0.393%
9	9.916	1293	1297	1300	rVV	1211219	962066	47.99%	5.008%
10	9.945	1300	1302	1306	rVB	43090	36469	1.82%	0.190%
11	10.116	1327	1331	1335	rBV2	21065	26123	1.30%	0.136%
12	10.316	1362	1365	1371	rVB8	20161	36099	1.80%	0.188%
13	10.369	1371	1374	1377	rBV	17385	21914	1.09%	0.114%
14	10.463	1387	1390	1397	rVB	42004	46320	2.31%	0.241%
15	10.710	1428	1432	1435	rBV	1072182	1005405	50.15%	5.234%
16	10.816	1446	1450	1459	rVB5	30550	68036	3.39%	0.354%
17	11.010	1480	1483	1486	rBV2	18209	21831	1.09%	0.114%
18	11.304	1531	1533	1536	rVB	32378	26794	1.34%	0.139%
19	11.404	1547	1550	1552	rBV	1047125	867211	43.26%	4.514%
20	11.427	1552	1554	1558	rVB	432685	341354	17.03%	1.777%
21	11.480	1560	1563	1566	rBV	149427	120478	6.01%	0.627%
22	11.639	1587	1590	1593	rBV	29362	30746	1.53%	0.160%
23	11.698	1598	1600	1603	rVB	30598	22925	1.14%	0.119%
24	11.739	1604	1607	1611	rVB2	35525	36427	1.82%	0.190%
25	11.780	1612	1614	1618	rBV4	31517	30319	1.51%	0.158%
26	11.921	1632	1638	1639	rBV2	119807	202297	10.09%	1.053%
27	11.980	1646	1648	1651	rBV	43764	37787	1.88%	0.197%
28	12.021	1651	1655	1657	rBV2	160991	189171	9.44%	0.985%
29	12.198	1683	1685	1688	rBV	68992	59622	2.97%	0.310%
30	12.233	1688	1691	1693	rVB	55875	52515	2.62%	0.273%
31	12.333	1705	1708	1709	rBV3	26780	22809	1.14%	0.119%
32	12.457	1726	1729	1731	rBV	93837	96042	4.79%	0.500%
33	12.545	1741	1744	1748	rBV2	70608	97459	4.86%	0.507%
34	12.621	1753	1757	1760	rBV	715639	596672	29.76%	3.106%
35	12.774	1781	1783	1785	rVB	39578	23986	1.20%	0.125%
36	12.798	1785	1787	1790	rVB4	41385	36710	1.83%	0.191%

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF080222\
Data File : BF129524.D
Acq On : 03 Aug 2022 00:19
Operator : CG\JU
Sample : N3989-01
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
OK-04-080122

Integration Parameters: rteint.p
Integrator: RTE
Smoothing : ON Filtering: 5
Sampling : 1 Min Area: 3 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF072522.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

37	12.851	1790	1796	1802	rBV	876650	870892	43.44%	4.533%
38	12.986	1816	1819	1823	rBV	1845414	1557356	77.69%	8.107%
39	13.068	1830	1833	1838	rBV2	67669	103661	5.17%	0.540%
40	13.174	1845	1851	1854	rBV	125625	213310	10.64%	1.110%
41	13.245	1861	1863	1865	rVB	71844	53212	2.65%	0.277%
42	13.280	1867	1869	1873	rVV	85685	91005	4.54%	0.474%
43	13.374	1883	1885	1888	rBV	92263	79780	3.98%	0.415%
44	13.404	1888	1890	1893	rBV	87008	89521	4.47%	0.466%
45	13.880	1968	1971	1977	rBV2	140311	234294	11.69%	1.220%
46	14.051	1995	2000	2002	rBV2	807992	962096	47.99%	5.008%
47	14.074	2002	2004	2010	rVB	225243	217435	10.85%	1.132%
48	15.539	2250	2253	2258	rVB	395467	515444	25.71%	2.683%




Sum of corrected areas: 19210710

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF080222\
Data File : BF129524.D
Acq On : 03 Aug 2022 00:19
Operator : CG\JU
Sample : N3989-01
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
OK-04-080122

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF072522.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library :
TIC Integration Parameters: rteint.p

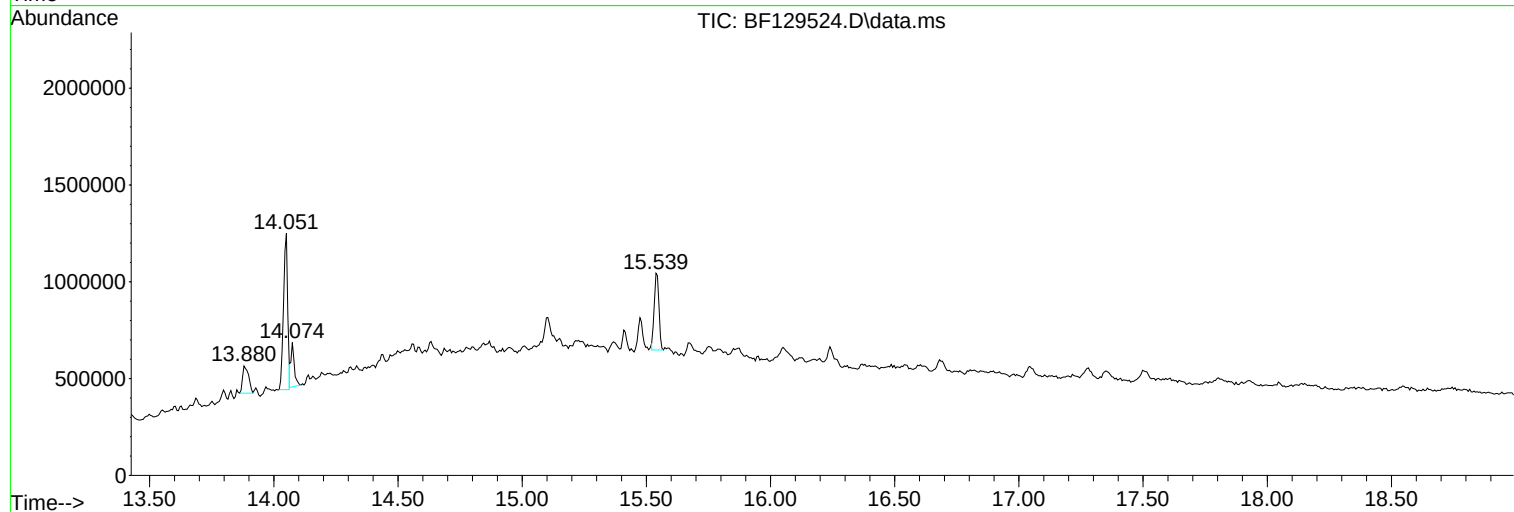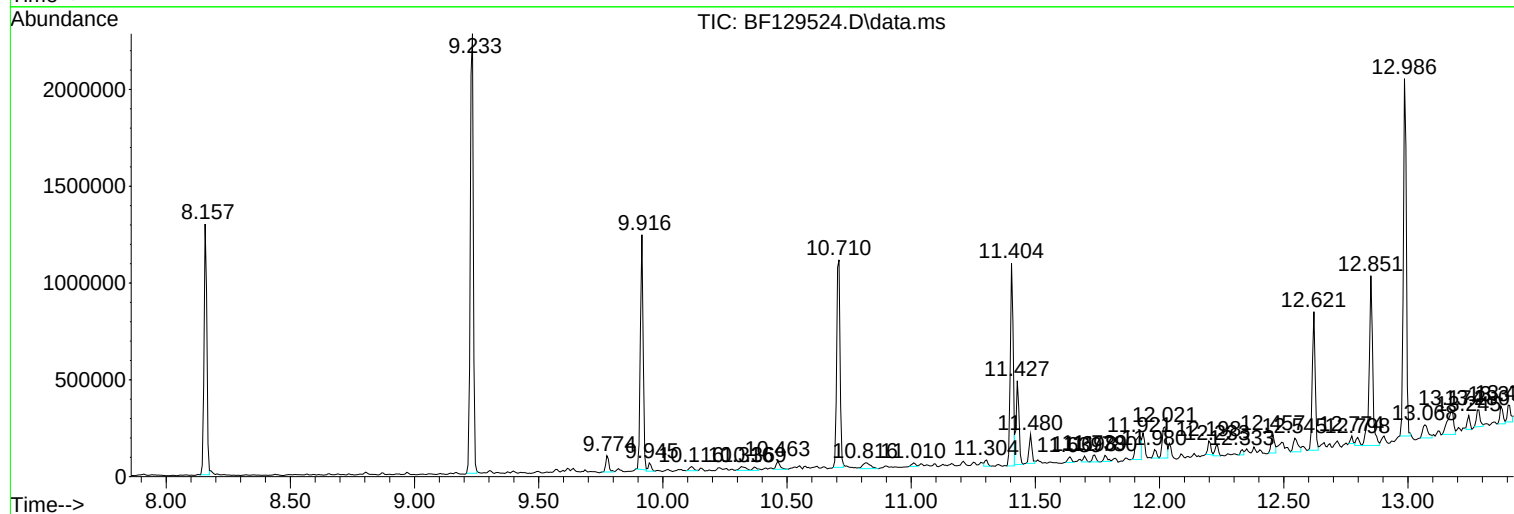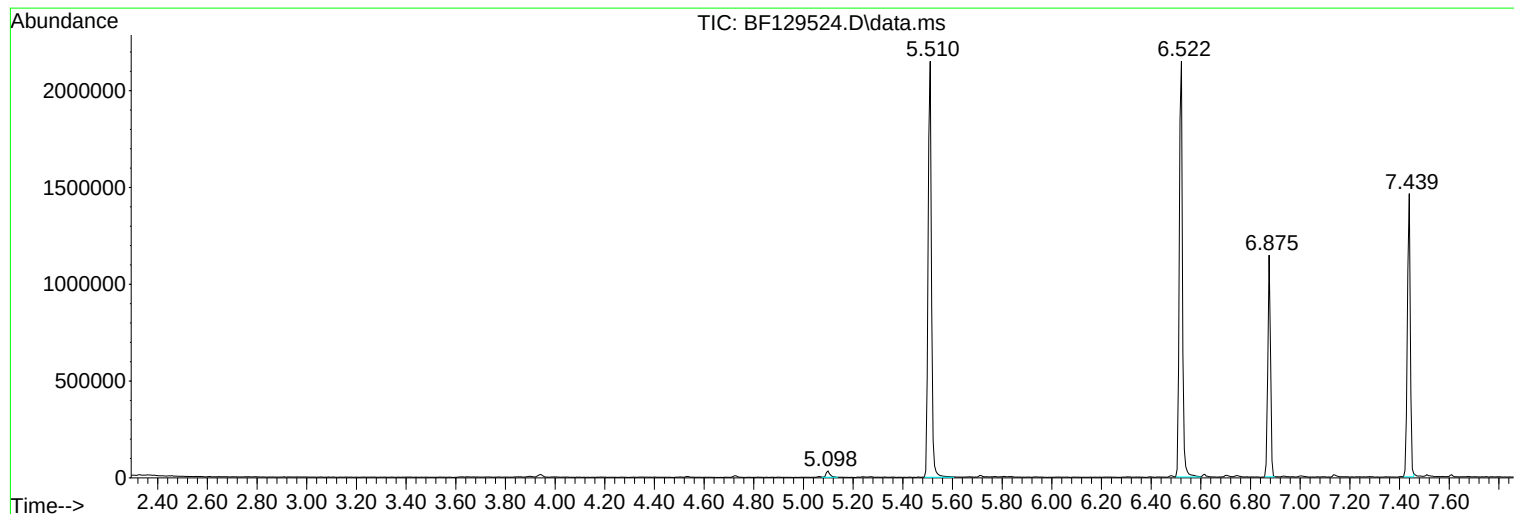

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF080222\
Data File : BF129524.D
Acq On : 03 Aug 2022 00:19
Operator : CG\JU
Sample : N3989-01
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
OK-04-080122

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF072522.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library :
TIC Integration Parameters: rteint.p

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF080222\
Data File : BF129524.D
Acq On : 03 Aug 2022 00:19
Operator : CG\JU
Sample : N3989-01
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
OK-04-080122

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF072522.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library :
TIC Integration Parameters: rteint.p

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------