
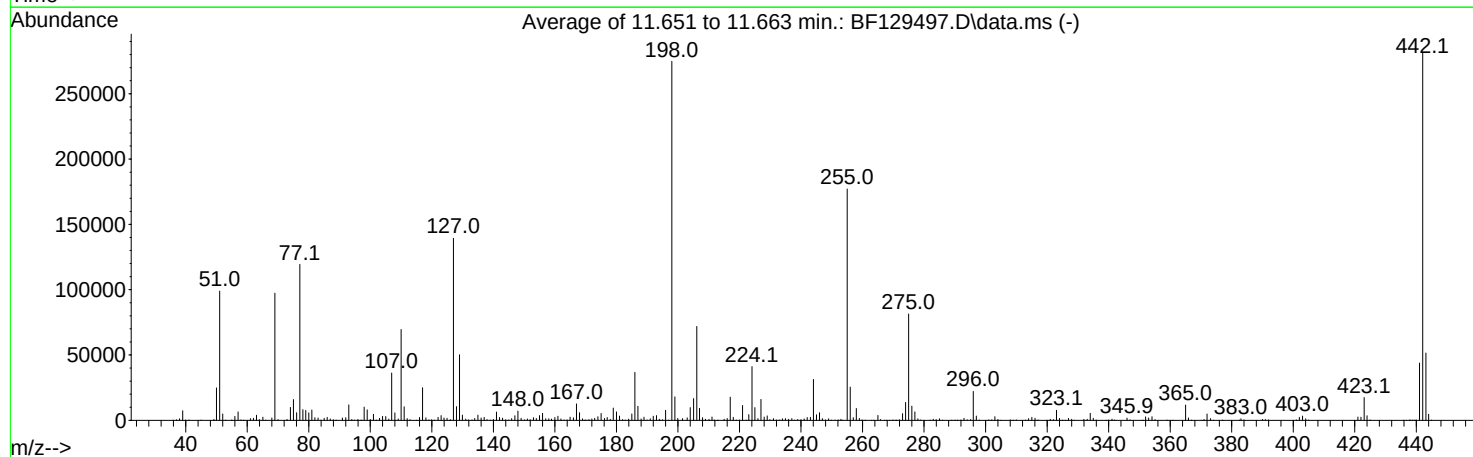


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF080222\
 Data File : BF129497.D
 Acq On : 02 Aug 2022 09:15
 Operator : CG\JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF072522.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Tue Aug 02 01:11:25 2022

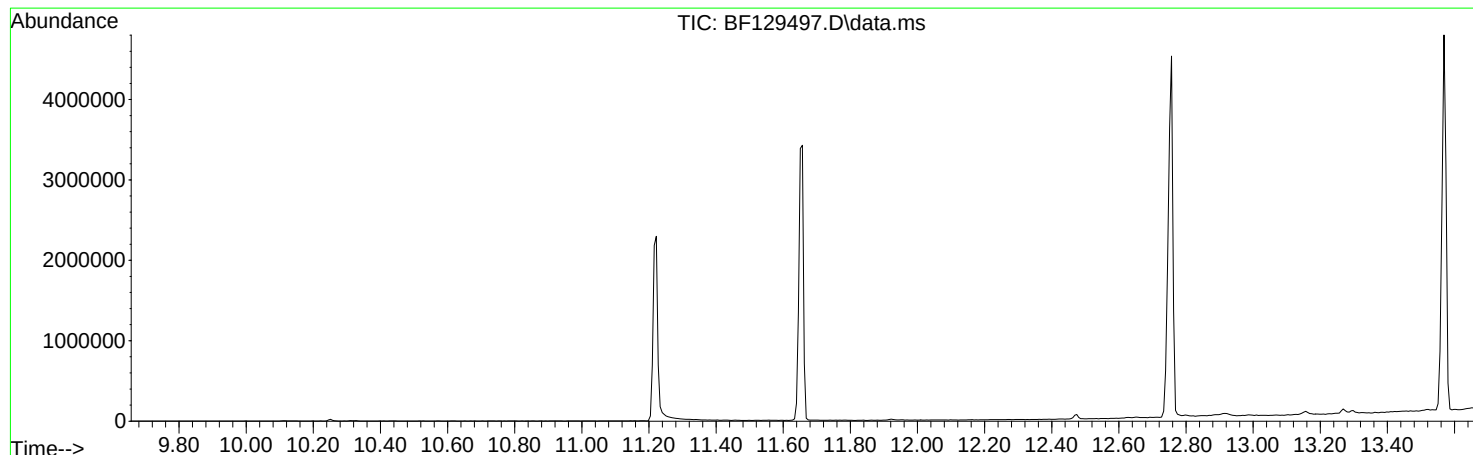




AutoFind: Scans 1592, 1593, 1594; Background Corrected with Scan 1585

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	36.0	98908	PASS
68	69	0.00	2	1.9	1806	PASS
69	198	0.00	100	35.4	97381	PASS
70	69	0.00	2	0.6	570	PASS
127	198	10	80	50.7	139400	PASS
197	198	0.00	2	0.1	222	PASS
198	198	100	100	100.0	274835	PASS
199	198	5	9	6.5	17912	PASS
275	198	10	60	29.6	81413	PASS
365	198	1	100	4.2	11661	PASS
441	198	0.01	100	15.9	43819	PASS
442	442	50	100	100.0	281664	PASS
443	442	15	24	18.3	51515	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF080222\
Data File : BF129497.D
Acq On : 02 Aug 2022 09:15
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Aug 02 18:20:40 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF072522.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Aug 02 01:11:25 2022
Response via : Initial Calibration

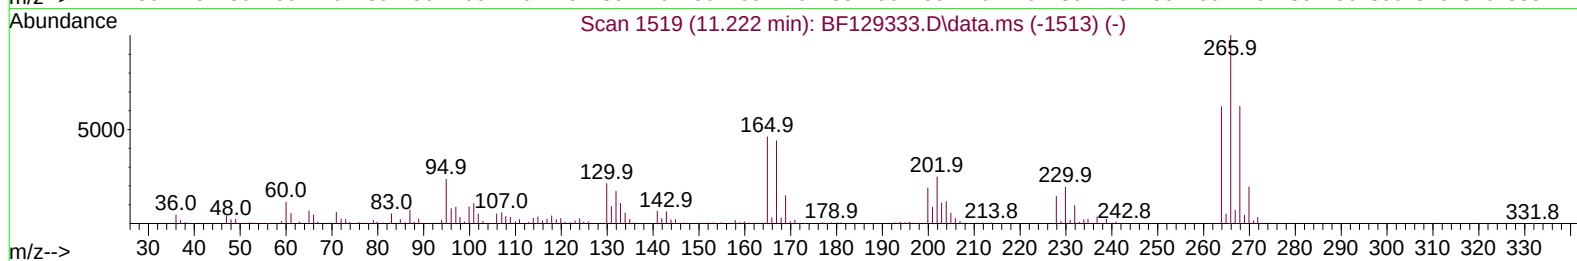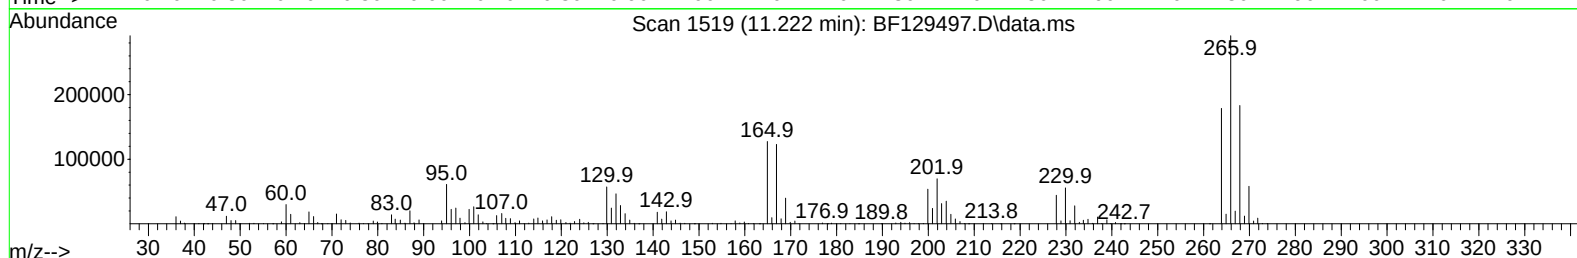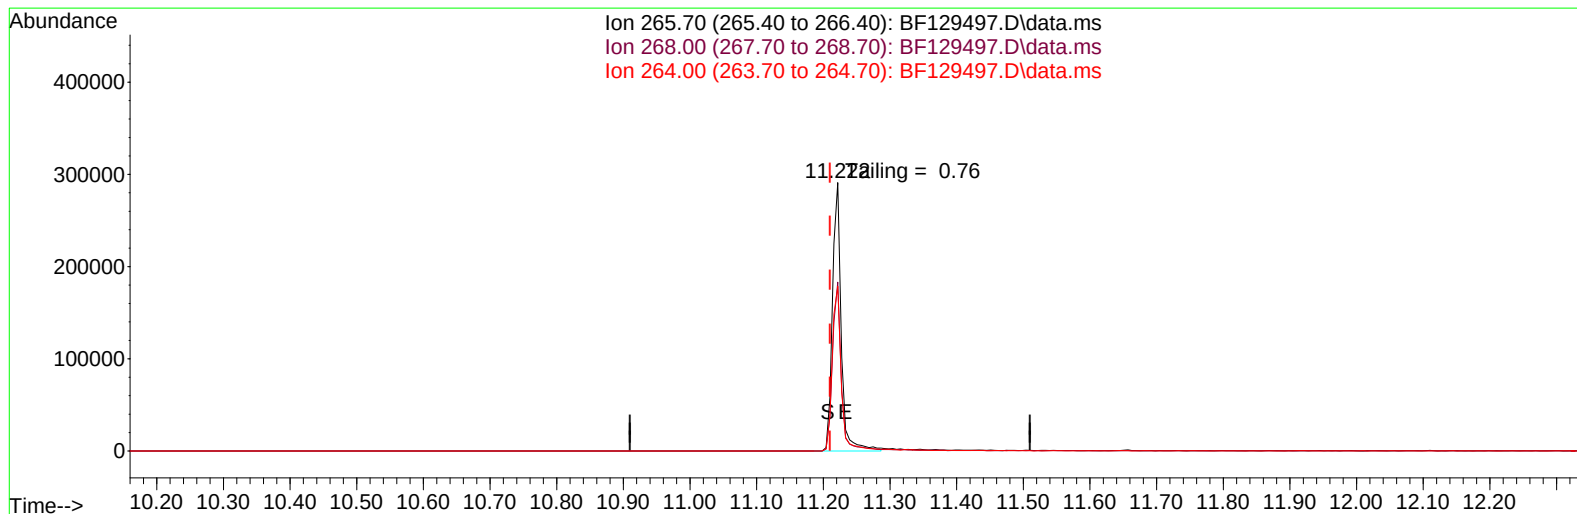

TIC: BF129497.D\data.ms

(70) Pentachlorophenol (C)

11.222min (+ 0.012) 542012.78 ng




response 272694

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.70	62.93
264.00	61.80	61.37
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF080222\
 Data File : BF129497.D
 Acq On : 02 Aug 2022 09:15
 Operator : CG\JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Quant Time: Aug 02 18:20:40 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF072522.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Aug 02 01:11:25 2022
 Response via : Initial Calibration

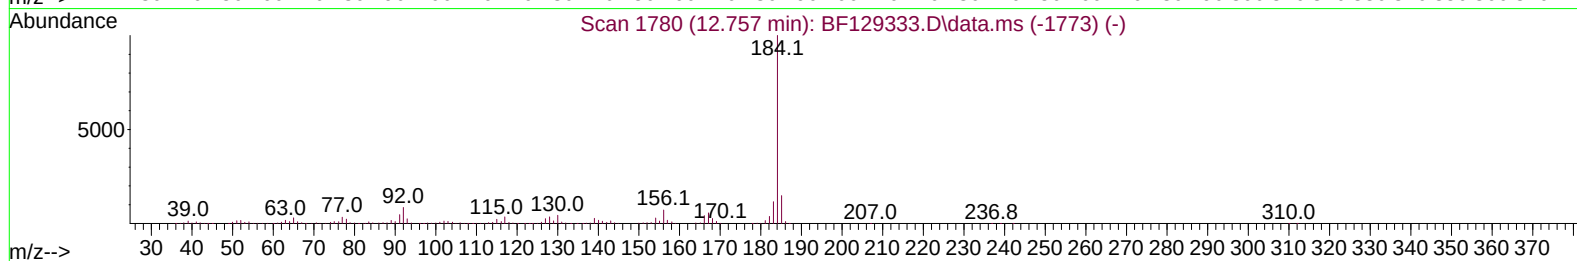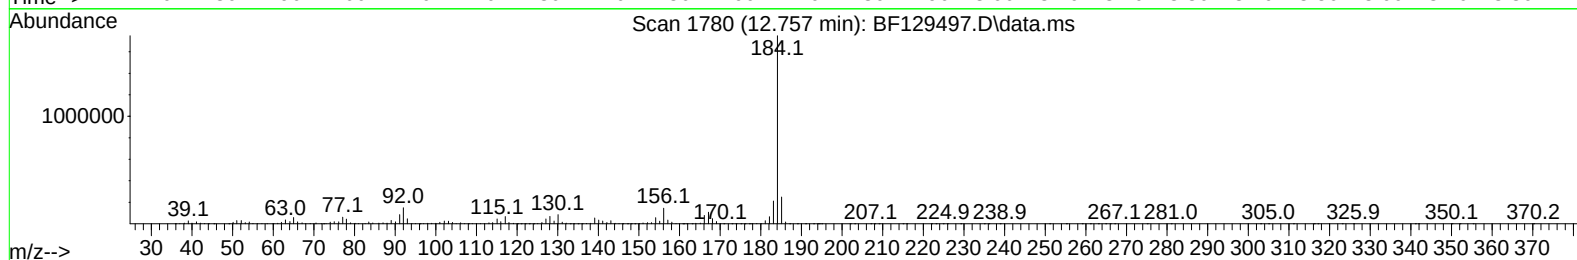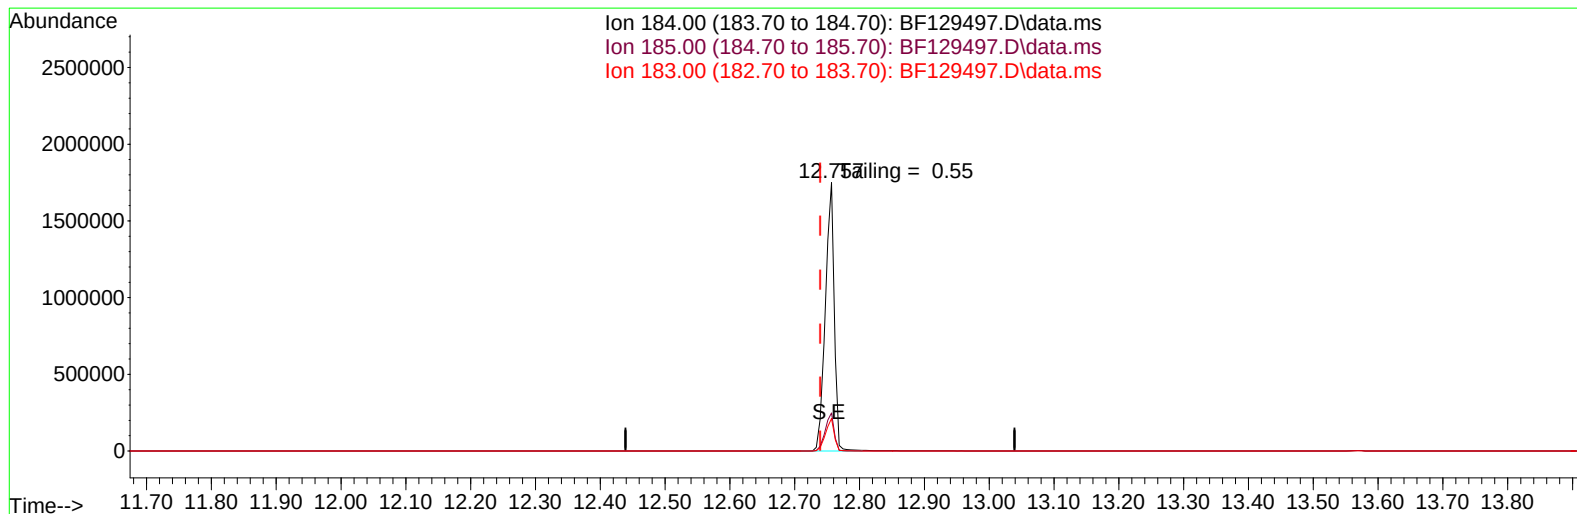

TIC: BF129497.D\data.ms

(77) Benzidine

12.757min (+ 0.018) 61368.37 ng

response 1693202

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.90	14.23
183.00	11.60	12.13
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
8/2/2022	BNA_F	<u>BF129497.D</u>
Compound Name	Response	Retention Time
DDT	784504	13.56
DDD	8860	13.26
DDE	1793	12.92
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
10653	795157	1.34

Instrument :
BNA_F
ClientSampleId :
DFTPP