


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF080222\
 Data File : BF129509.D
 Acq On : 02 Aug 2022 16:02
 Operator : CG\JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF072522.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Tue Aug 02 01:11:25 2022

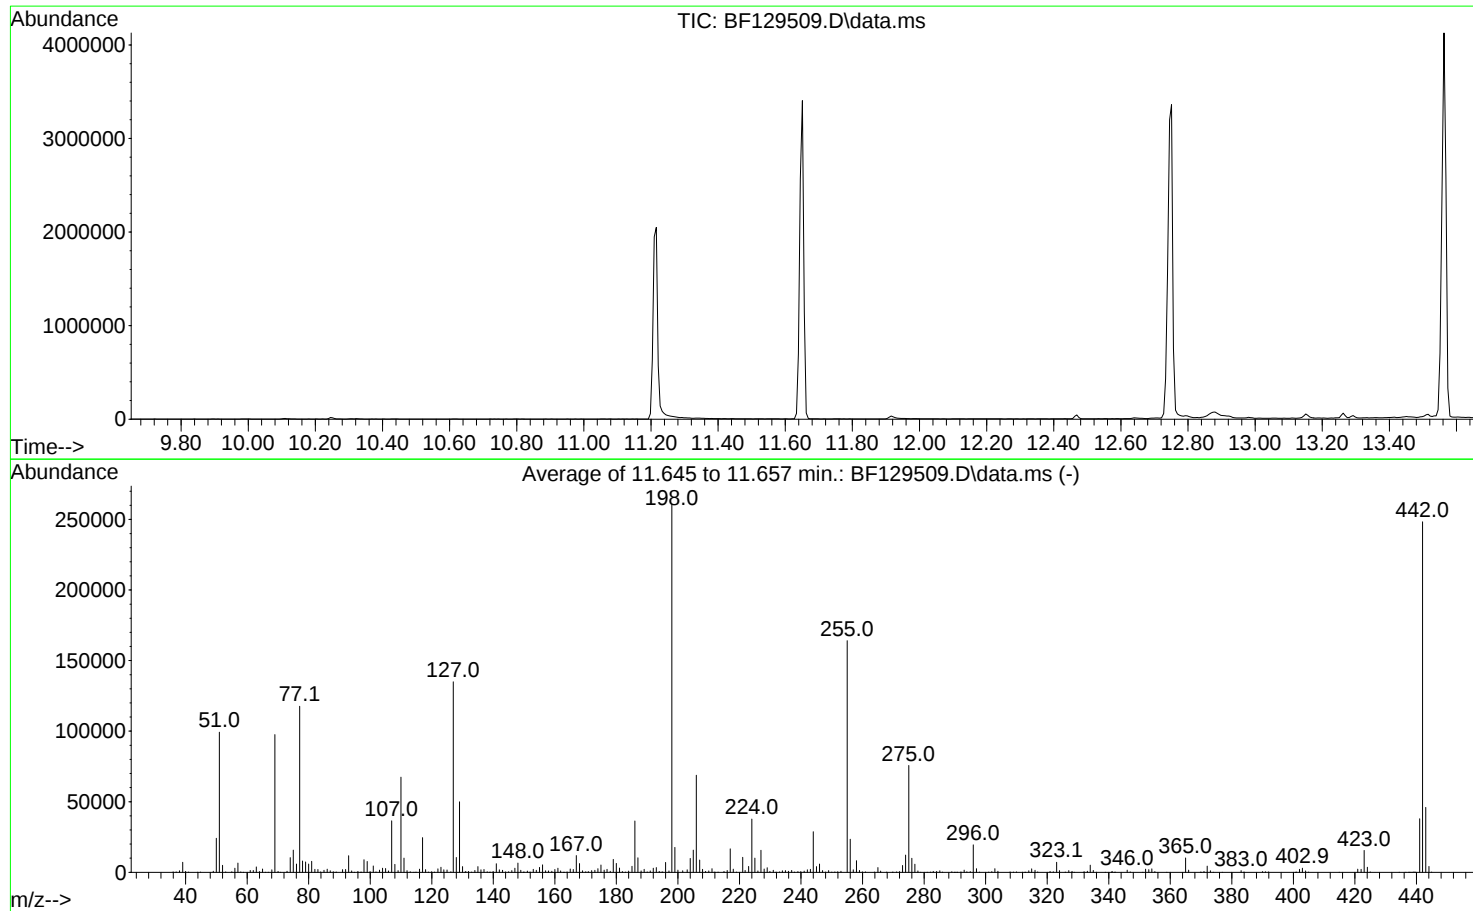




AutoFind: Scans 1591, 1592, 1593; Background Corrected with Scan 1585

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	38.1	99232	PASS
68	69	0.00	2	1.8	1714	PASS
69	198	0.00	100	37.4	97549	PASS
70	69	0.00	2	0.6	610	PASS
127	198	10	80	51.8	135029	PASS
197	198	0.00	2	0.4	969	PASS
198	198	100	100	100.0	260656	PASS
199	198	5	9	6.8	17663	PASS
275	198	10	60	29.0	75675	PASS
365	198	1	100	3.9	10108	PASS
441	198	0.01	100	14.6	37944	PASS
442	442	50	100	100.0	248384	PASS
443	442	15	24	18.5	45992	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF080222\
Data File : BF129509.D
Acq On : 02 Aug 2022 16:02
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Aug 02 18:19:04 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF072522.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Aug 02 01:11:25 2022
Response via : Initial Calibration

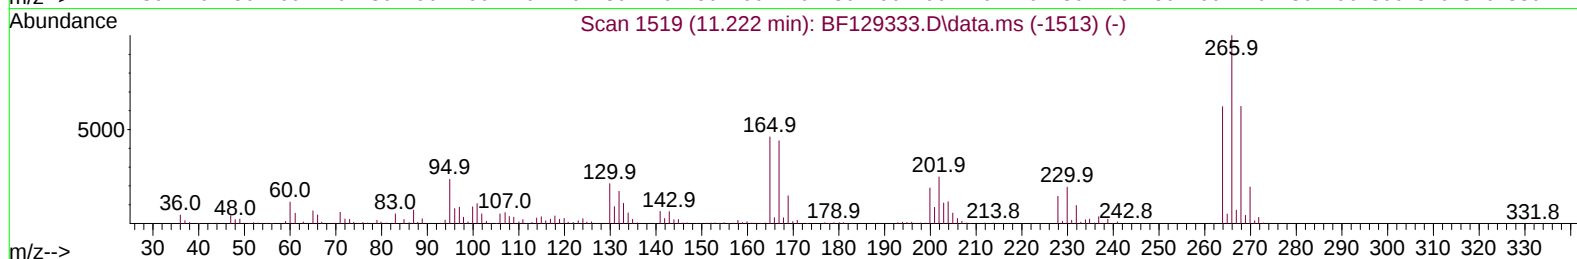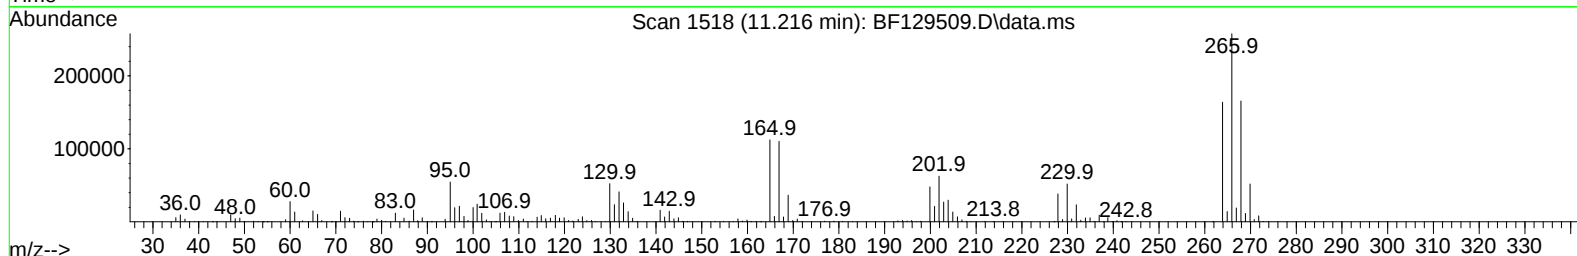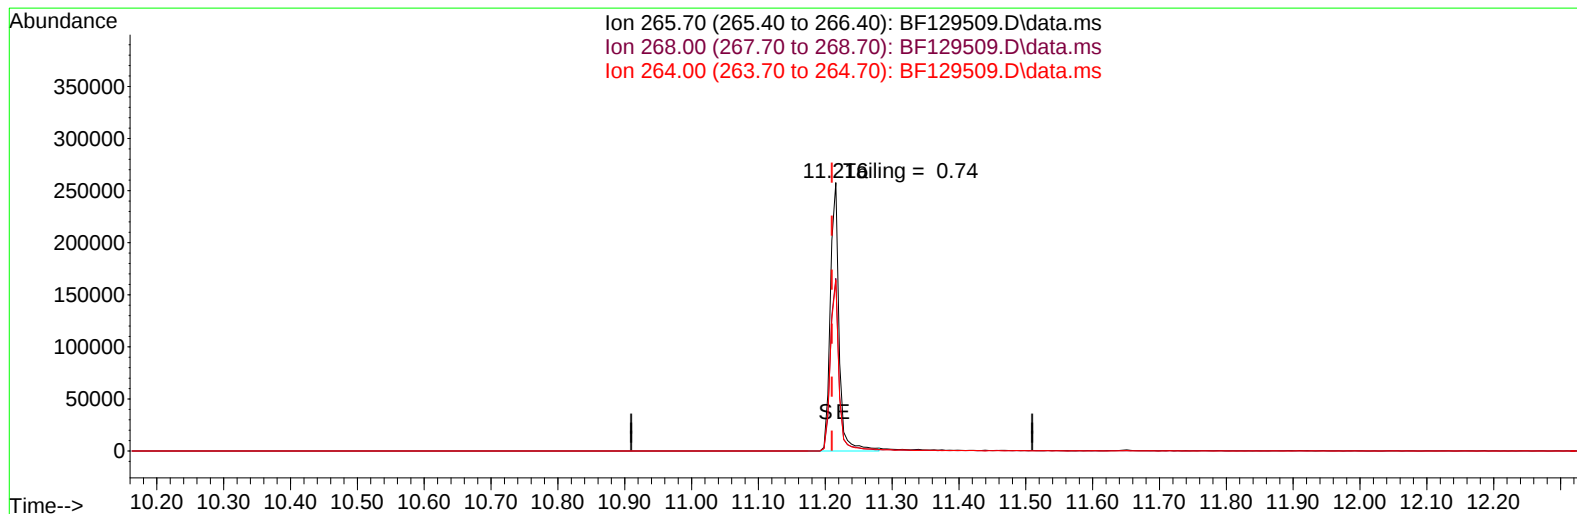

TIC: BF129509.D\data.ms

(70) Pentachlorophenol (C)

11.216min (+ 0.006) 271634.24 ng




response 238284

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.70	64.28
264.00	61.80	63.56
0.00	0.00	0.00

```
Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF080222\  
Data File : BF129509.D  
Acq On    : 02 Aug 2022  16:02  
Operator  : CG\JU  
Sample    : DFTPP  
Misc      :  
ALS Vial  : 1    Sample Multiplier: 1
```

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Aug 02 18:19:04 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF072522.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Aug 02 01:11:25 2022
Response via : Initial Calibration

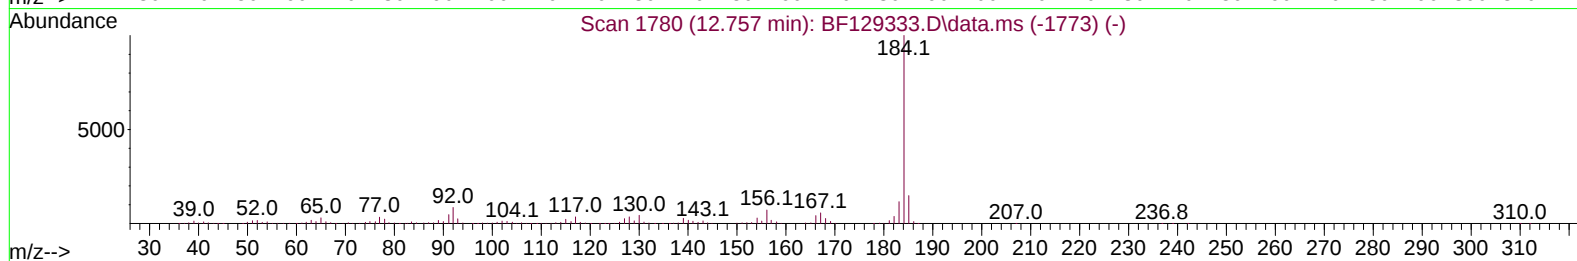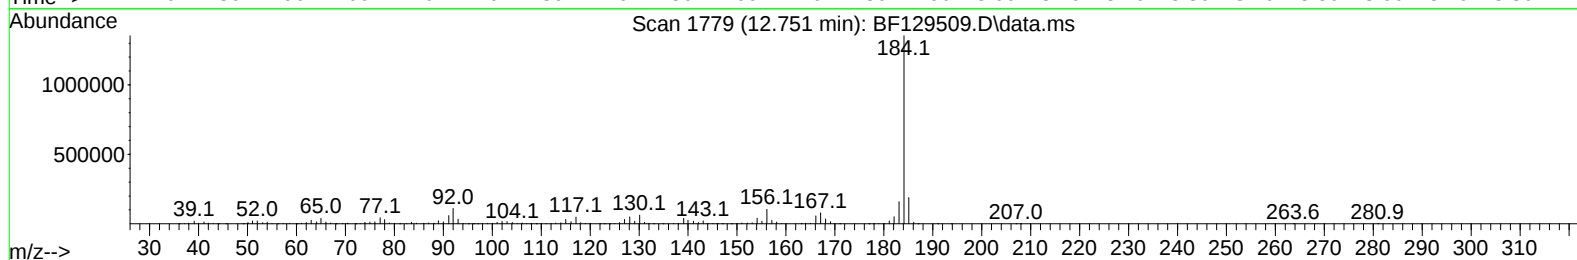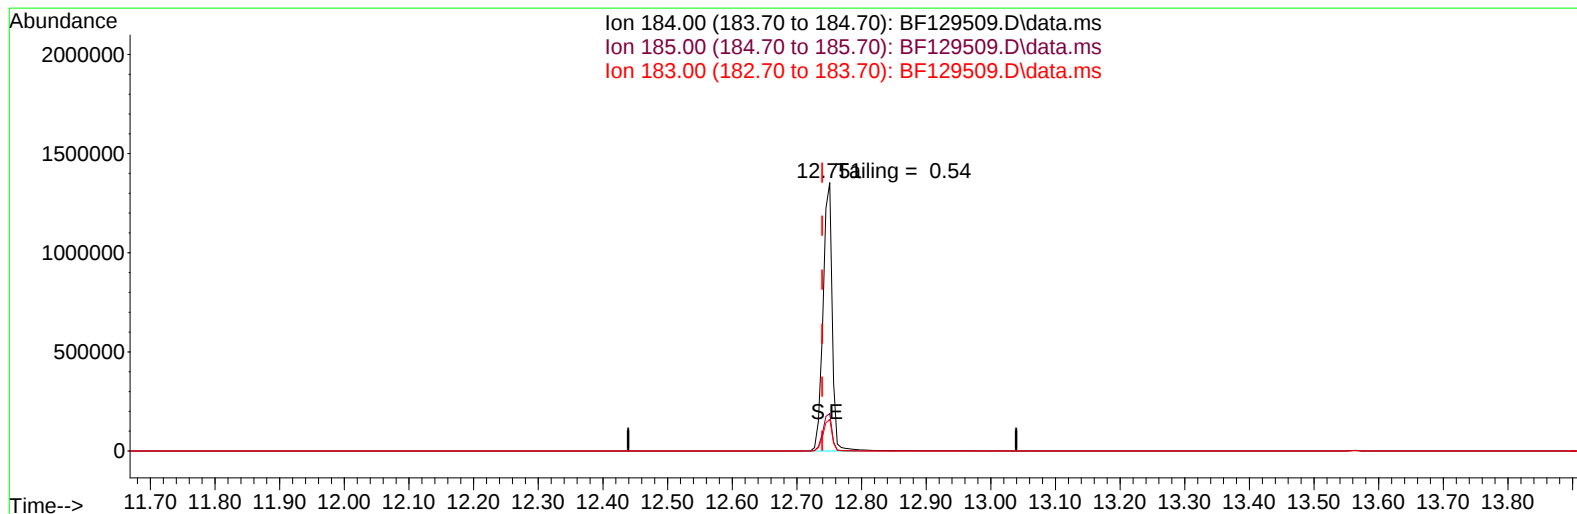

TIC: BF129509.D\data.ms

(77) Benzidine

12.751min (+ 0.012) 87009.73 ng

response 1346341

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.90	13.96
183.00	11.60	11.79
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
8/2/2022	BNA_F	<u>BF129509.D</u>
Compound Name	Response	Retention Time
DDT	688971	13.56
DDD	7883	13.26
DDE	1999	12.92
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
9882	698853	1.41

Instrument :
BNA_F
ClientSampleId :
DFTPP