
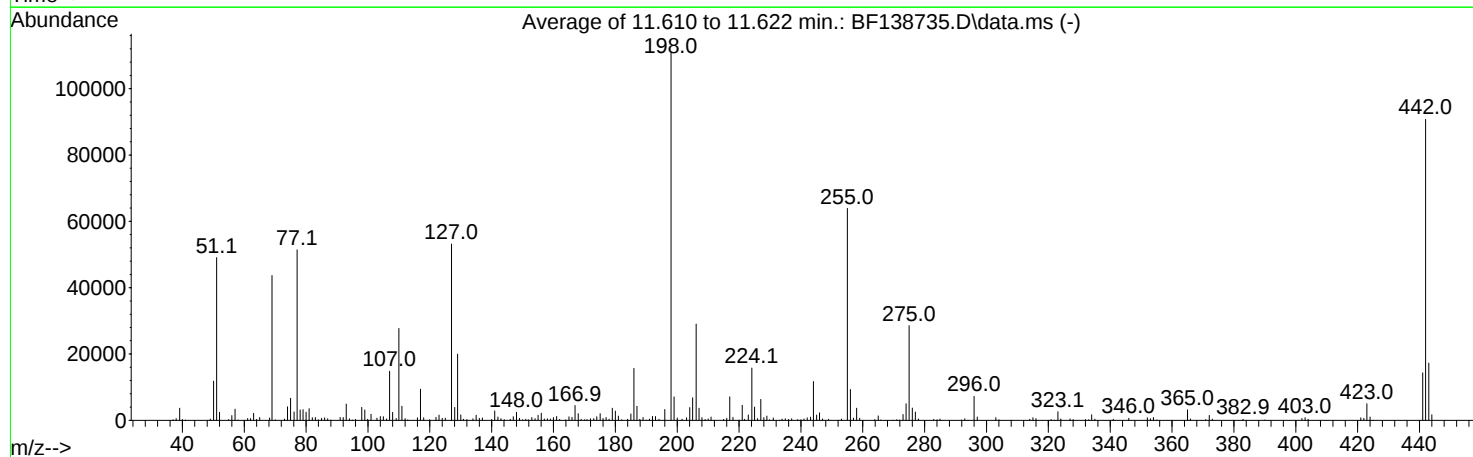


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF080224\
Data File : BF138735.D
Acq On : 02 Aug 2024 08:43
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF073024.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Tue Jul 30 17:50:01 2024

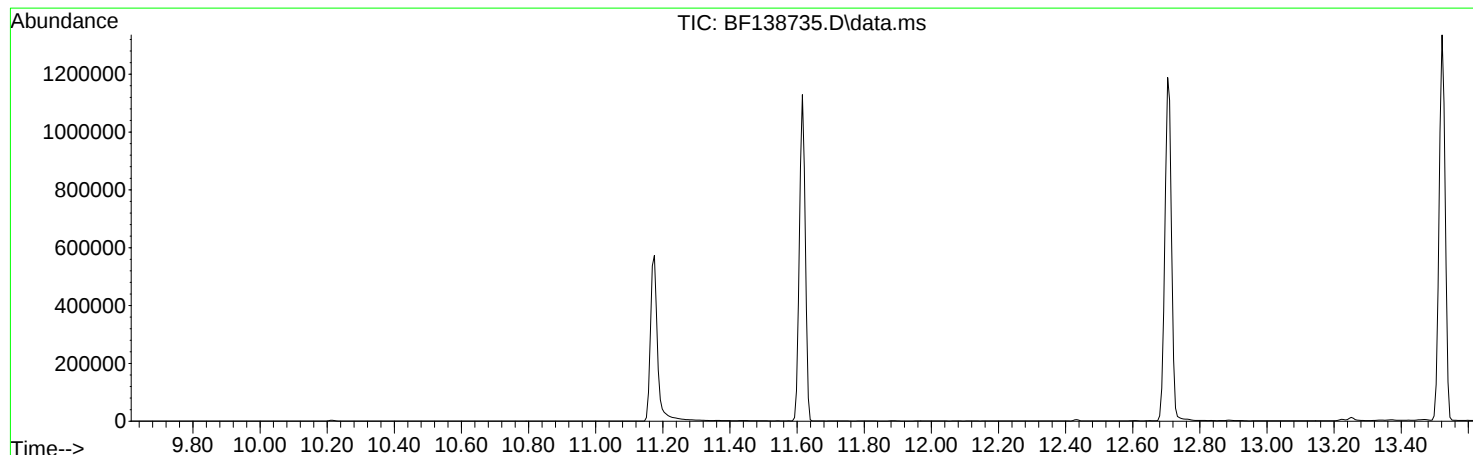

AutoFind: Scans 1618, 1619, 1620; Background Corrected with Scan 1612

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	44.2	49064	PASS
68	69	0.00	2	1.6	711	PASS
69	198	0.00	100	39.4	43651	PASS
70	69	0.00	2	0.3	151	PASS
127	198	10	80	47.9	53157	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	110901	PASS
199	198	5	9	6.4	7081	PASS
275	198	10	60	25.8	28565	PASS
365	198	1	100	2.9	3164	PASS
441	198	0.01	100	12.9	14342	PASS
442	442	50	100	100.0	90739	PASS
443	442	15	24	19.0	17272	PASS

DDT Breakdown




Date	Instrument Name	DFTPP Data File
8/2/2024	BNA_F	<u>BF138735.D</u>
Compound Name	Response	Retention Time
DDT	324820	13.522
DDD	5979	13.251
DDE	1238	12.886
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
7217	332037	2.17

Instrument :
BNA_F
ClientSampleId :
DFTPP

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF080224\
Data File : BF138735.D
Acq On : 02 Aug 2024 08:43
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Aug 02 10:56:08 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF073024.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Jul 30 17:50:01 2024
Response via : Initial Calibration

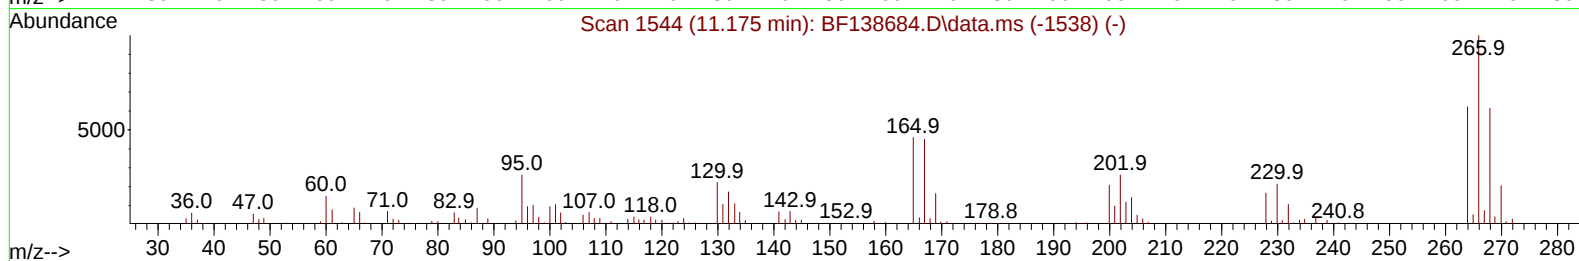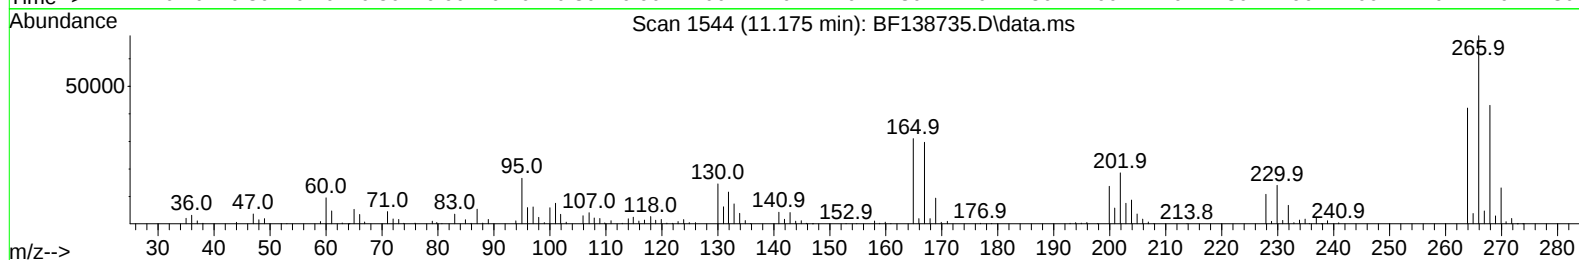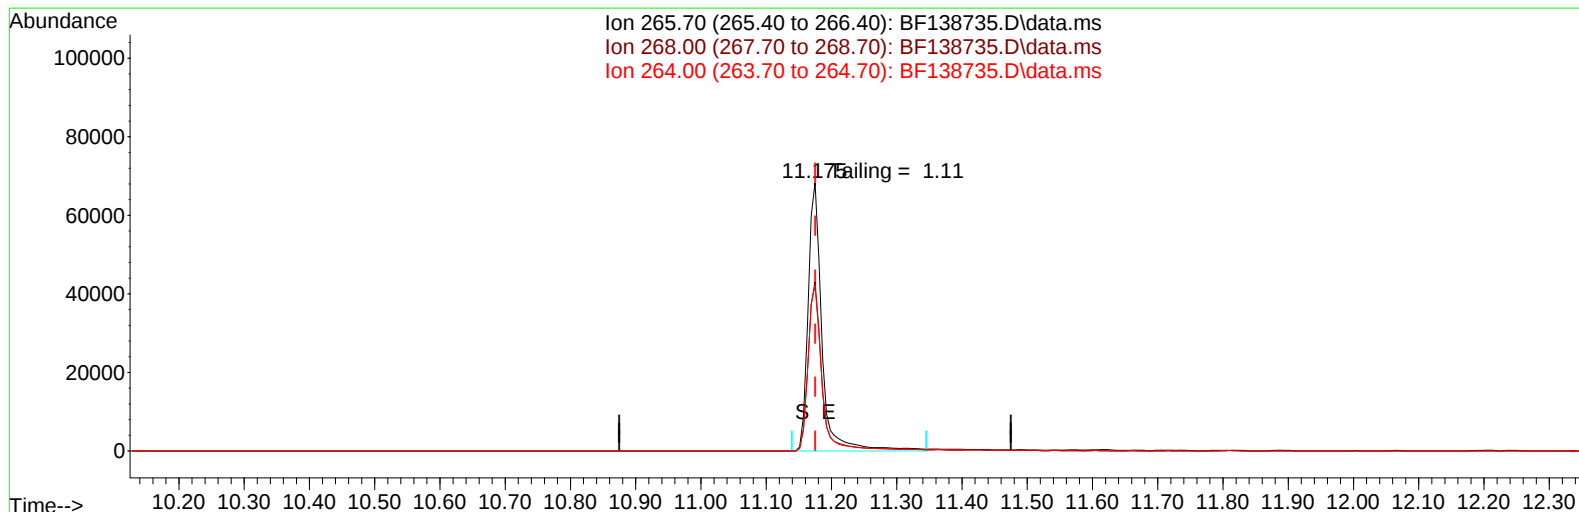

TIC: BF138735.D\data.ms

(70) Pentachlorophenol (C)

11.175min (-0.000) 48840.11 ng




response 101637

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	61.50	63.03
264.00	62.20	61.62
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF080224\
Data File : BF138735.D
Acq On : 02 Aug 2024 08:43
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Aug 02 10:56:08 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF073024.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Jul 30 17:50:01 2024
Response via : Initial Calibration

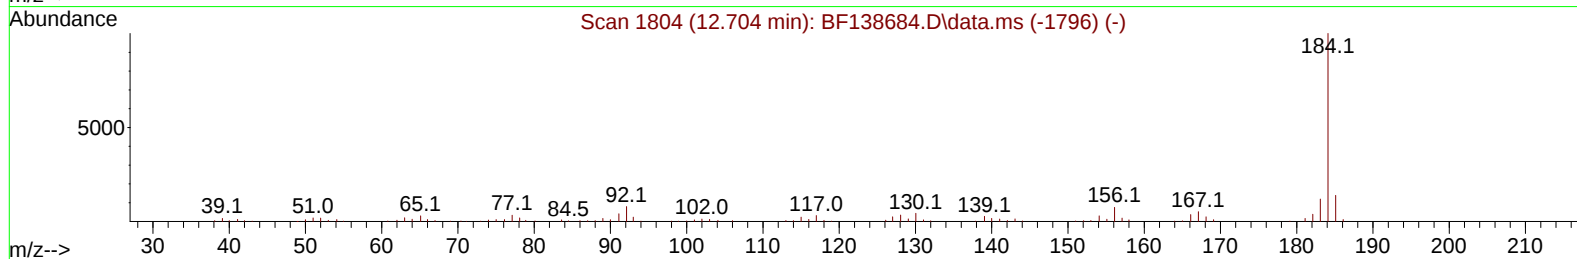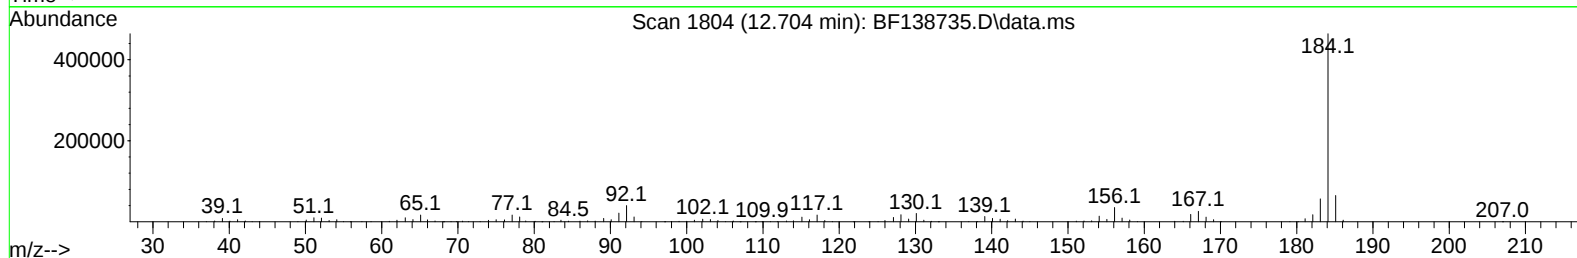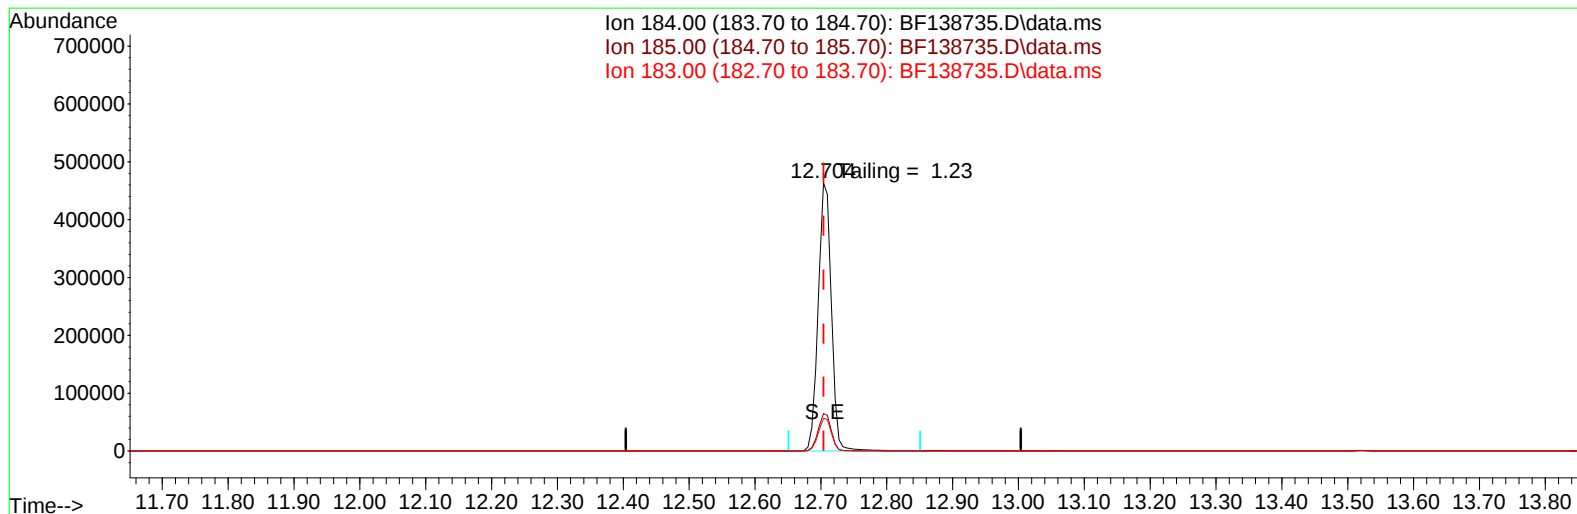

TIC: BF138735.D\data.ms

(77) Benzidine

12.704min (0.000) 0.00 ng

response 643592

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	13.90	13.99
183.00	12.00	12.20
0.00	0.00	0.00