
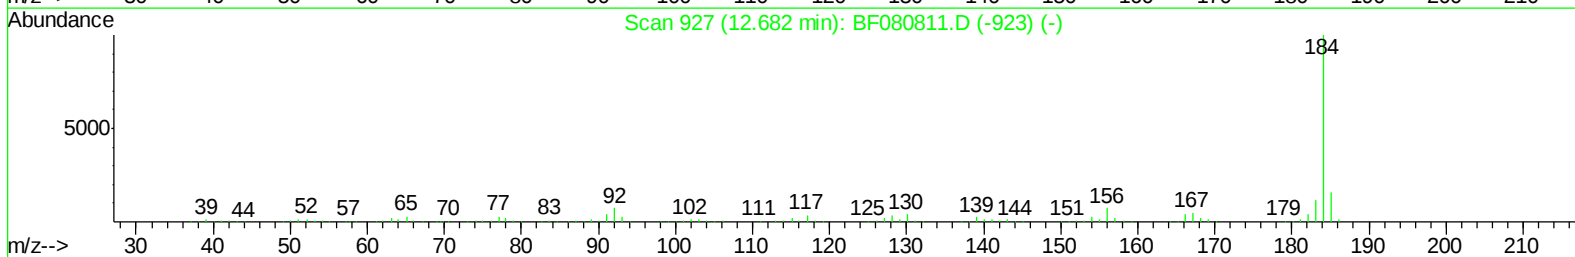
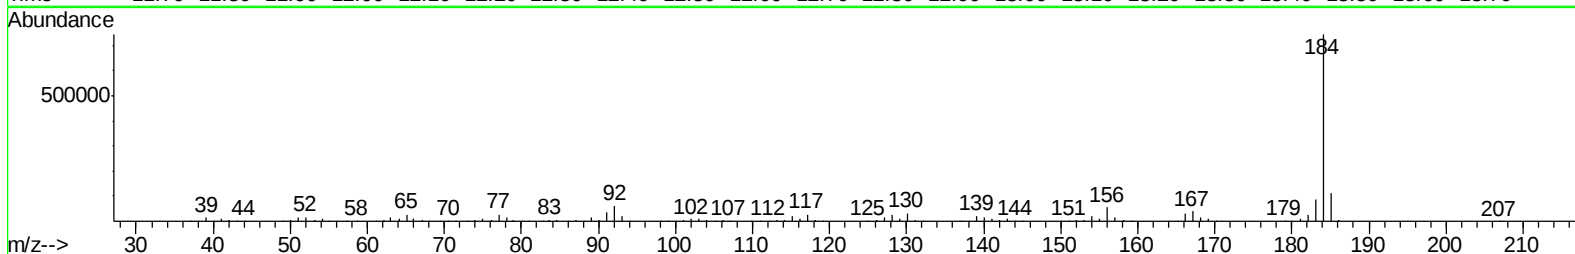


Data Path : Z:\HPCHEM1\BNA_F\Data\BF080315\
Data File : BF080806.D
Acq On : 3 Aug 2015 17:48
Operator : TP
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Aug 28 06:31:03 2015
Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF080315.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Aug 04 14:50:50 2015
Response via : Initial Calibration

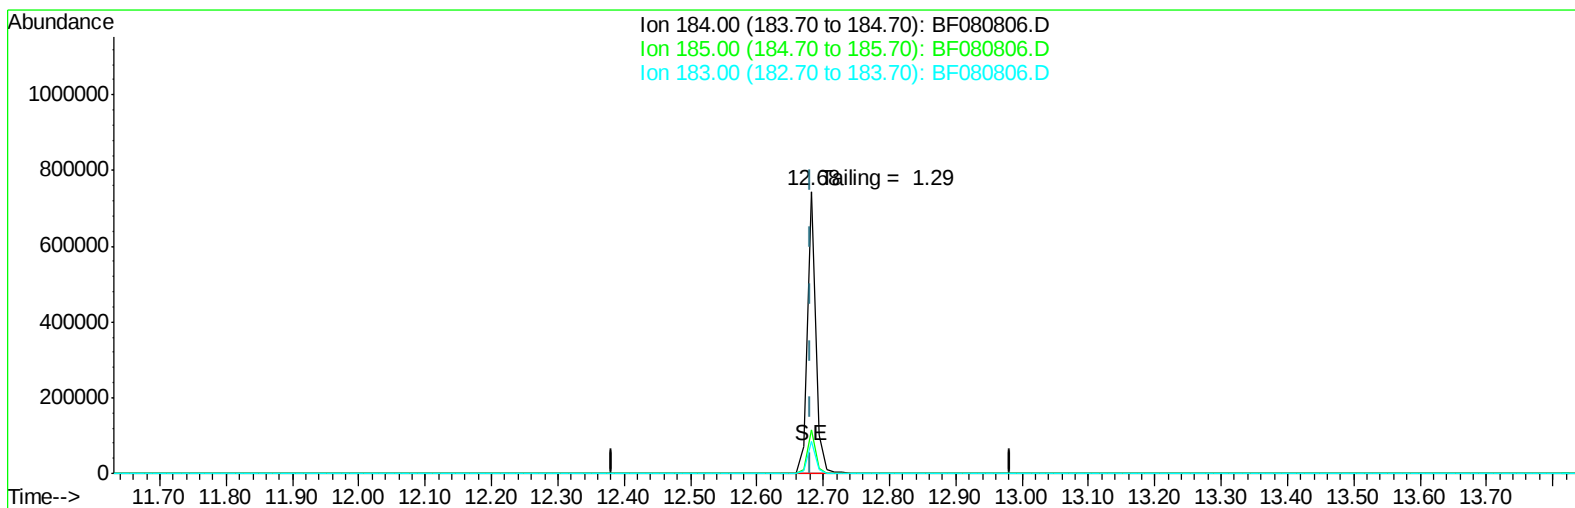

TIC: BF080806.D

(76) Benzidine




12.682min (+0.000) 0.00ng

response 643368

Ion	Exp%	Act%
184.00	100	100
185.00	15.70	15.35
183.00	11.60	11.57
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA_F\Data\BF080315\
Data File : BF080806.D
Acq On : 3 Aug 2015 17:48
Operator : TP
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Aug 28 06:31:03 2015
Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF080315.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Aug 04 14:50:50 2015
Response via : Initial Calibration

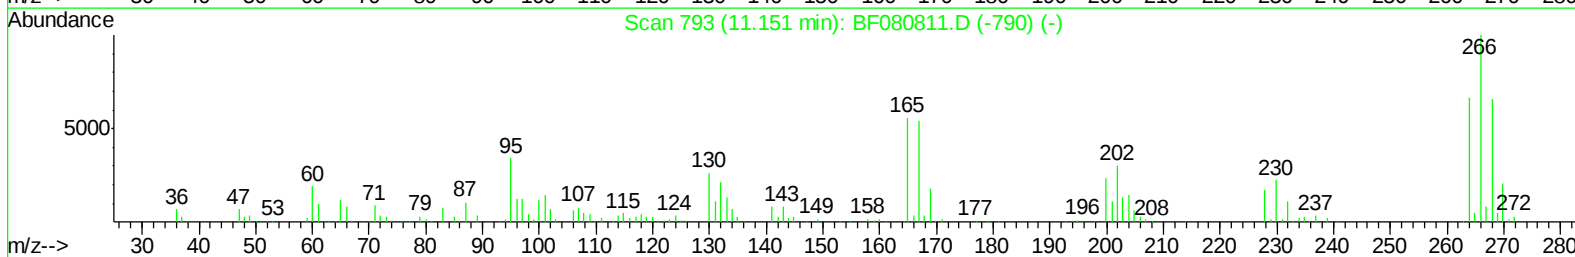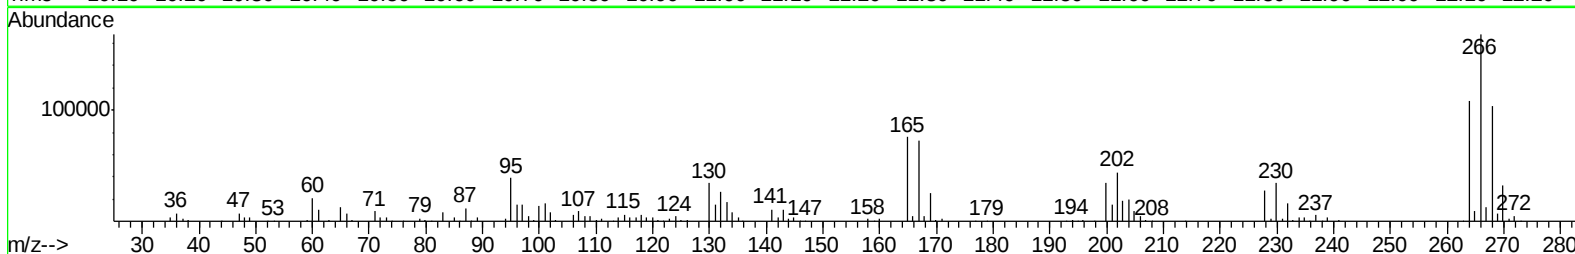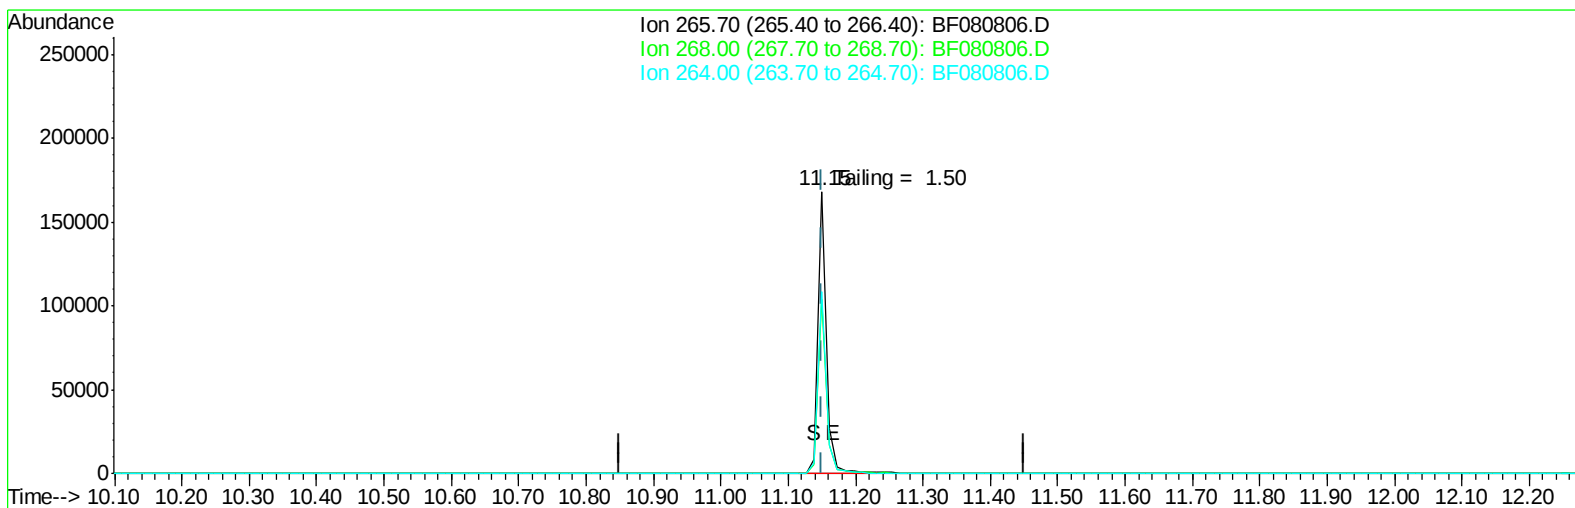

TIC: BF080806.D

(69) Pentachlorophenol (C)

11.150min (-0.000) 93633.20ng

response 146526

Ion	Exp%	Act%
265.70	100	100
268.00	65.90	62.04
264.00	66.70	64.39
0.00	0.00	0.00