


Data Path : Z:\HPCHEM1\BNA_F\Data\BF080315\
Data File : BF080826.D
Acq On : 4 Aug 2015 5:45
Operator : TP
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF080315.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Tue Aug 04 14:50:50 2015

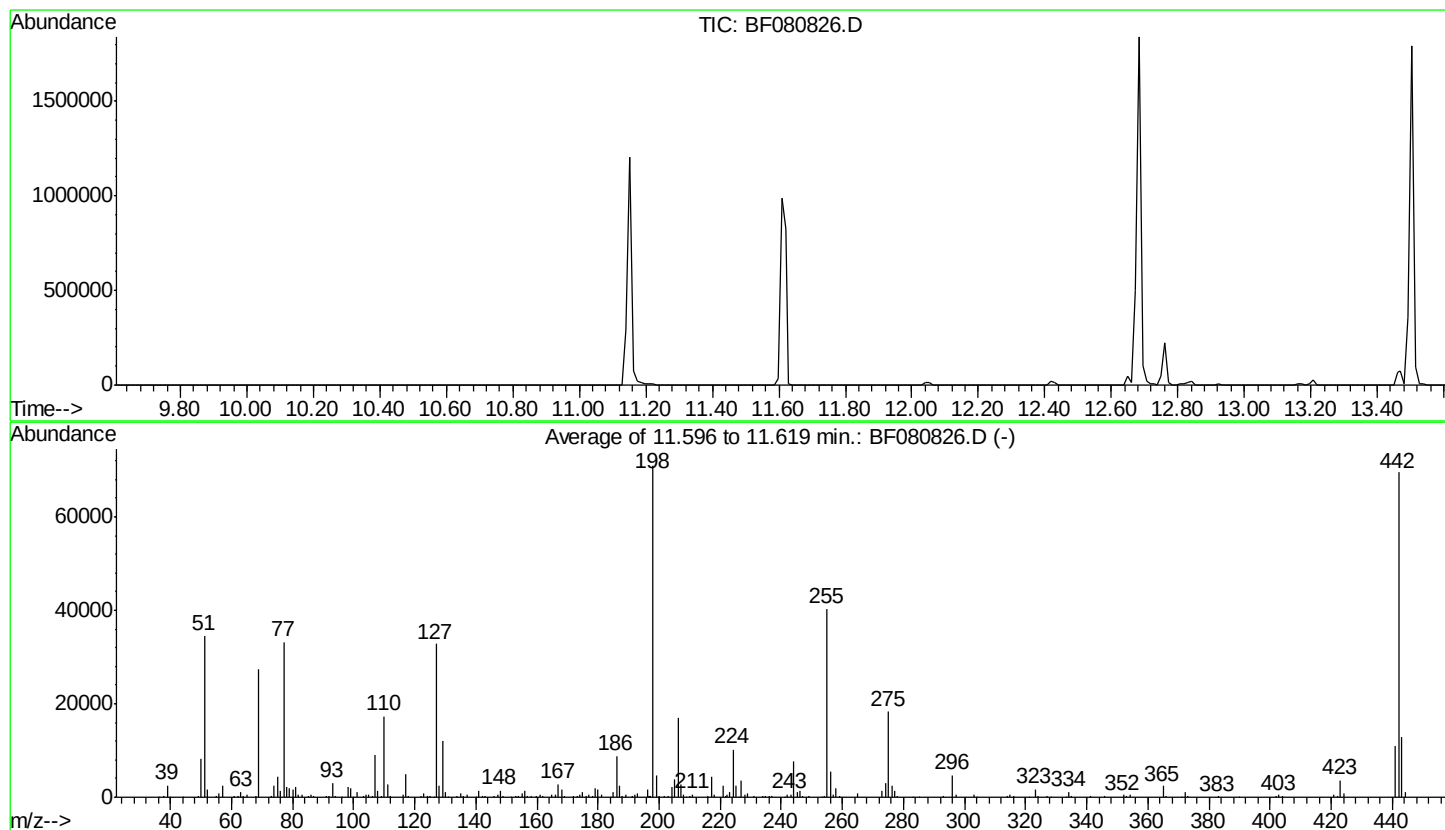

AutoFind: Scans 832, 833, 834; Background Corrected with Scan 829

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	48.8	34621	PASS
68	69	0.00	2	1.1	314	PASS
69	198	0.00	100	38.7	27445	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	46.3	32871	PASS
197	198	0.00	2	0.4	252	PASS
198	198	100	100	100.0	70980	PASS
199	198	5	9	6.7	4754	PASS
275	198	10	60	25.8	18312	PASS
365	198	1	100	3.4	2419	PASS
441	442	0.01	24	15.8	11019	PASS
442	198	50	100	98.1	69656	PASS
443	442	15	24	18.3	12766	PASS