

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF080316\
 Data File : BF089578.D
 Acq On : 4 Aug 2016 4:24
 Operator : UM/SJ
 Sample : H4328-03 5X
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 PLSA-003(WATERY-SHEEN)

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF080316.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.404	331	334	347	rBV3	3574	21304	5.26%	0.964%
2	7.039	474	477	483	rBV	6523	24776	6.12%	1.121%
3	7.130	483	485	501	rVB	24508	64008	15.80%	2.895%
4	7.462	512	514	533	rBV	138513	233521	57.64%	10.563%
5	7.702	533	535	551	rVB	26558	50688	12.51%	2.293%
6	8.410	594	597	616	rBV	3458	21636	5.34%	0.979%
7	9.485	689	691	712	rBV	206649	353248	87.20%	15.978%
8	11.268	845	847	859	rBB	59032	76442	18.87%	3.458%
9	12.308	936	938	949	rBB	258866	405111	100.00%	18.324%
10	13.611	1050	1052	1057	rBB	11463	21054	5.20%	0.952%
11	14.708	1146	1148	1162	rBV	247465	364052	89.86%	16.467%
12	17.063	1352	1354	1359	rVB	44015	56290	13.89%	2.546%
13	18.400	1469	1471	1477	rBV	170475	234243	57.82%	10.595%
14	20.069	1614	1617	1623	rBV	144721	244103	60.26%	11.041%
15	20.343	1639	1641	1646	rVB3	14026	23218	5.73%	1.050%
16	21.143	1709	1711	1715	rVB2	11577	17116	4.23%	0.774%


Sum of corrected areas: 2210810

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF080316\
Data File : BF089578.D
Acq On : 4 Aug 2016 4:24
Operator : UM/SJ
Sample : H4328-03 5X
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PLSA-003(WATERY-SHEEN)

Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF080316.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST11.L
TIC Integration Parameters: LSCINT.P

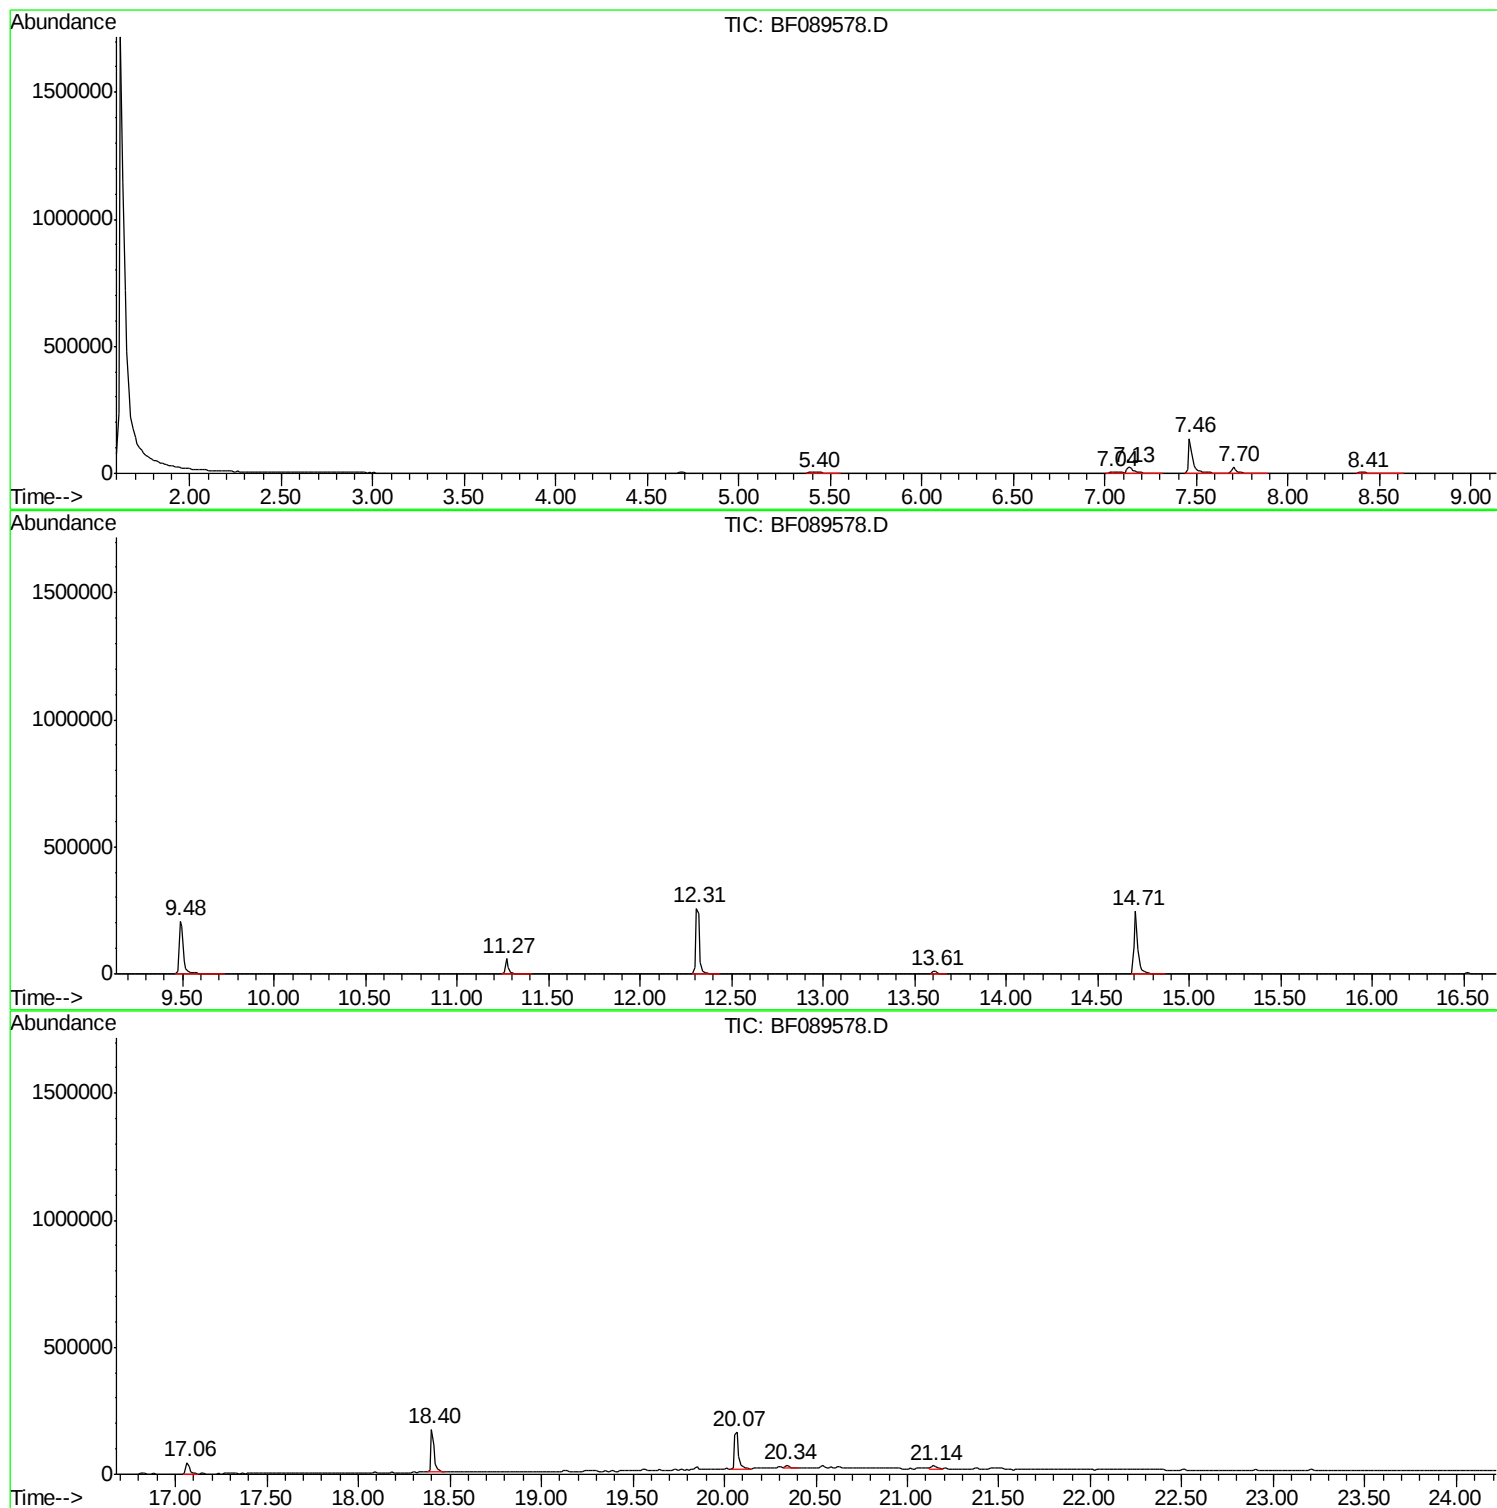

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF080316\
Data File : BF089578.D
Acq On : 4 Aug 2016 4:24
Operator : UM/SJ
Sample : H4328-03 5X
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PLSA-003(WATERY-SHEEN)










Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF080316.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST11.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 unknown7.13 Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
7.13	5.48 ng	64008	1,4-Dichlorobenzene-d4	7.46

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Benzene, 1-methyl-4-(1-methyleth...	132	C10H12	001195-32-0	12
2			1H-Benzimidazole, 2-methyl-	132	C8H8N2	000615-15-6	12
3			3-Chloro-6-fluoro-pyrazine	132	C4H2ClFN2	1000146-10-7	9
4			4-Chloro-2-fluoro-pyrimidine	132	C4H2ClFN2	051422-00-5	9
5			(E)-3-Chloro-2-methyl-2-pentenal	132	C6H9ClO	031357-76-3	9

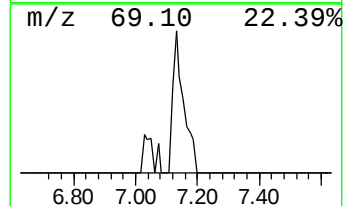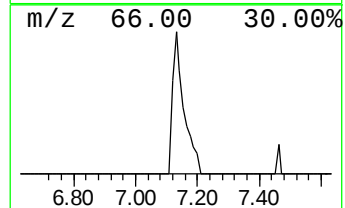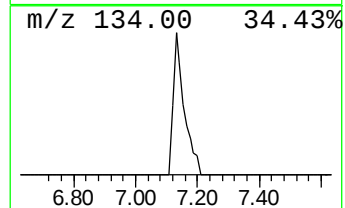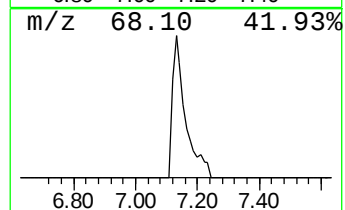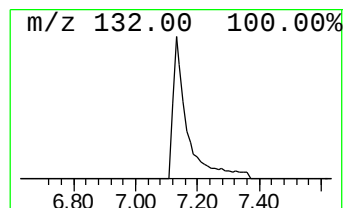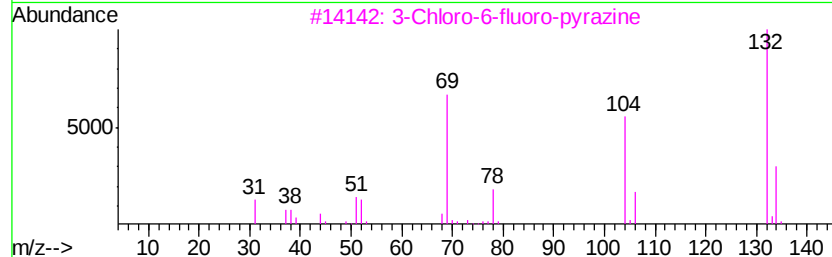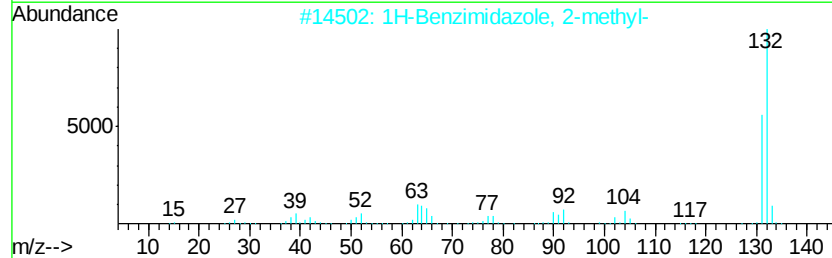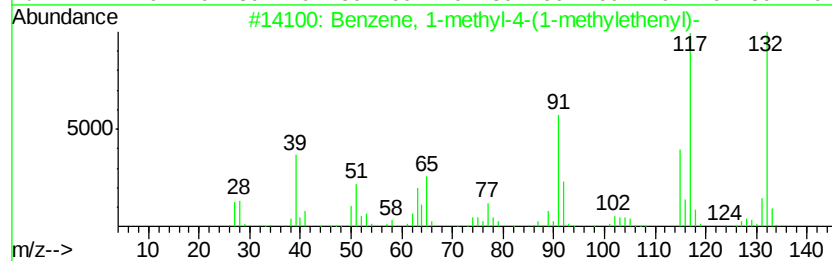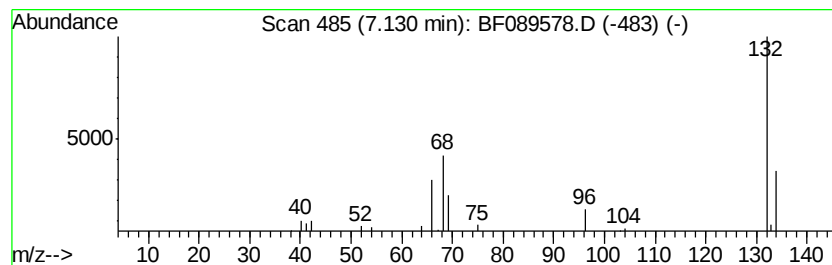

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF080316\
Data File : BF089578.D
Acq On : 4 Aug 2016 4:24
Operator : UM/SJ
Sample : H4328-03 5X
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PLSA-003(WATERY-SHEEN)

Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF080316.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
unknown7.13	7.13	5.5	ng	64008	1	7.46	233521	20.0