


Data Path : Z:\HPCHEM1\BNA\_F\DATA\BF080316\  
Data File : BF089564.D  
Acq On : 3 Aug 2016 17:15  
Operator : UM/SJ  
Sample : DFTPP  
Misc :  
ALS Vial : 1 Sample Multiplier: 1

Instrument :  
BNA\_F  
ClientSampleId :  
DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA\_F\METHODS\8270-BF080316.M  
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
Last Update : Thu Aug 04 08:40:24 2016

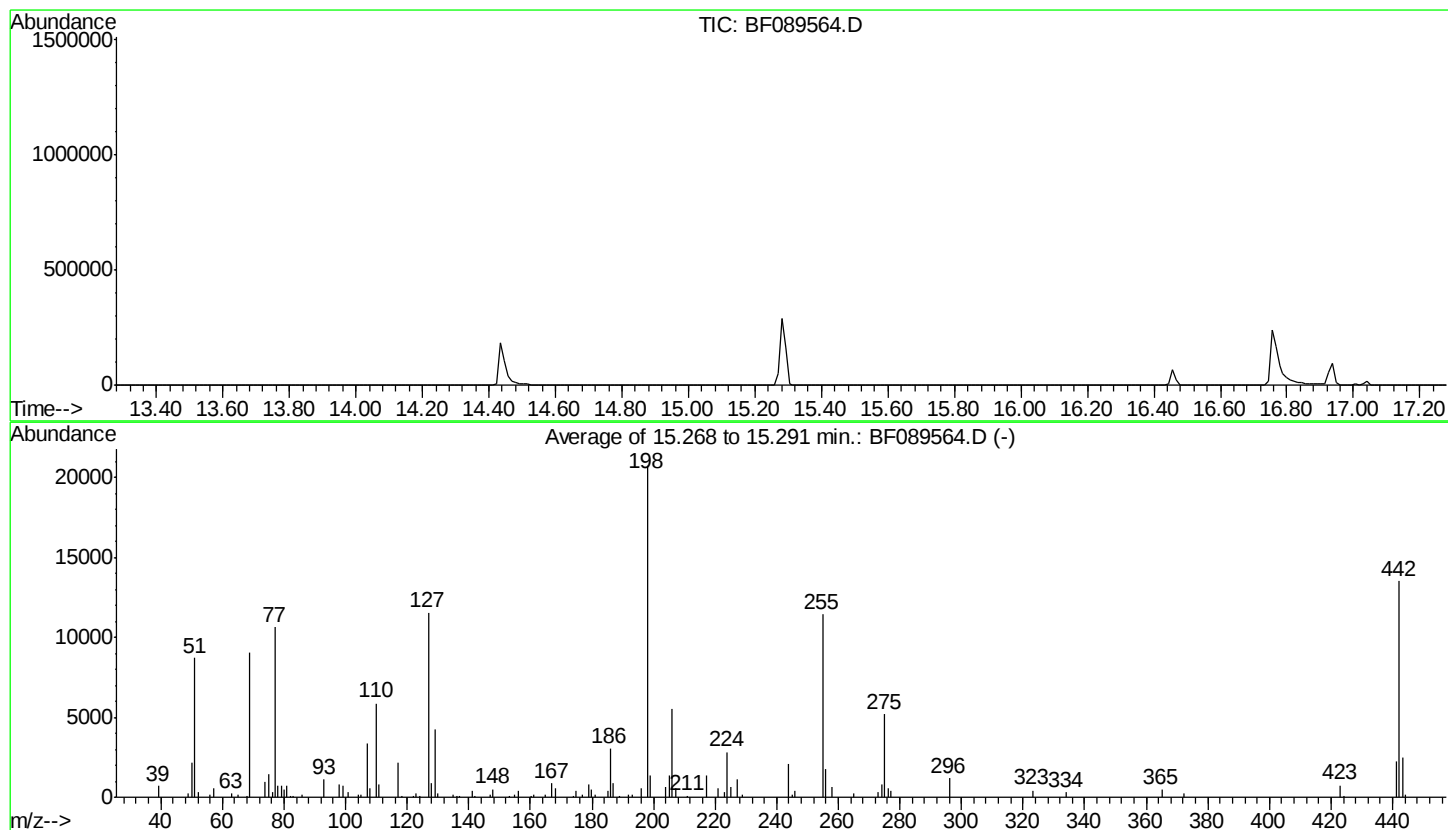

AutoFind: Scans 1197, 1198, 1199; Background Corrected with Scan 1194

| Target Mass | Rel. to Mass | Lower Limit% | Upper Limit% | Rel. Abn% | Raw Abn | Result Pass/Fail |
|-------------|--------------|--------------|--------------|-----------|---------|------------------|
| 51          | 198          | 10           | 80           | 41.9      | 8696    | PASS             |
| 68          | 69           | 0.00         | 2            | 1.3       | 118     | PASS             |
| 69          | 198          | 0.00         | 100          | 43.5      | 9024    | PASS             |
| 70          | 69           | 0.00         | 2            | 0.0       | 0       | PASS             |
| 127         | 198          | 10           | 80           | 55.7      | 11548   | PASS             |
| 197         | 198          | 0.00         | 2            | 0.0       | 0       | PASS             |
| 198         | 198          | 100          | 100          | 100.0     | 20739   | PASS             |
| 199         | 198          | 5            | 9            | 6.7       | 1396    | PASS             |
| 275         | 198          | 10           | 60           | 25.0      | 5195    | PASS             |
| 365         | 198          | 1            | 100          | 2.2       | 452     | PASS             |
| 441         | 442          | 0.01         | 24           | 16.4      | 2215    | PASS             |
| 442         | 198          | 50           | 100          | 65.1      | 13501   | PASS             |
| 443         | 442          | 15           | 24           | 18.3      | 2464    | PASS             |