


Data Path : Z:\HPCHEM1\BNA_F\DATA\BF080316\
 Data File : BF089574.D
 Acq On : 4 Aug 2016 2:10
 Operator : UM/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF080316.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Thu Aug 04 08:40:24 2016

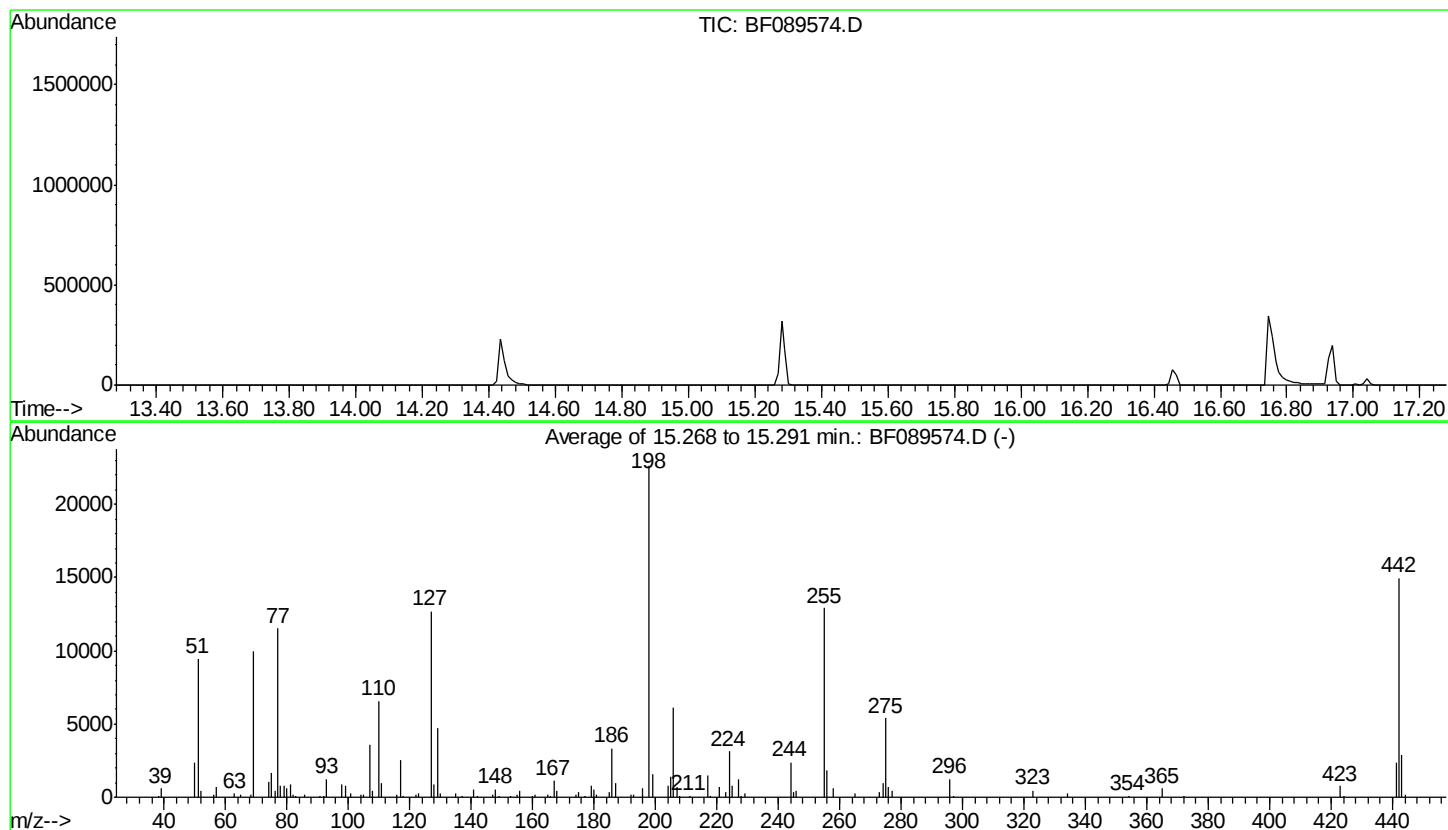

AutoFind: Scans 1197, 1198, 1199; Background Corrected with Scan 1194

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	41.7	9451	PASS
68	69	0.00	2	1.6	162	PASS
69	198	0.00	100	44.2	10002	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	56.0	12682	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	22652	PASS
199	198	5	9	7.0	1586	PASS
275	198	10	60	23.8	5398	PASS
365	198	1	100	2.7	612	PASS
441	442	0.01	24	16.0	2390	PASS
442	198	50	100	66.1	14980	PASS
443	442	15	24	19.5	2928	PASS