
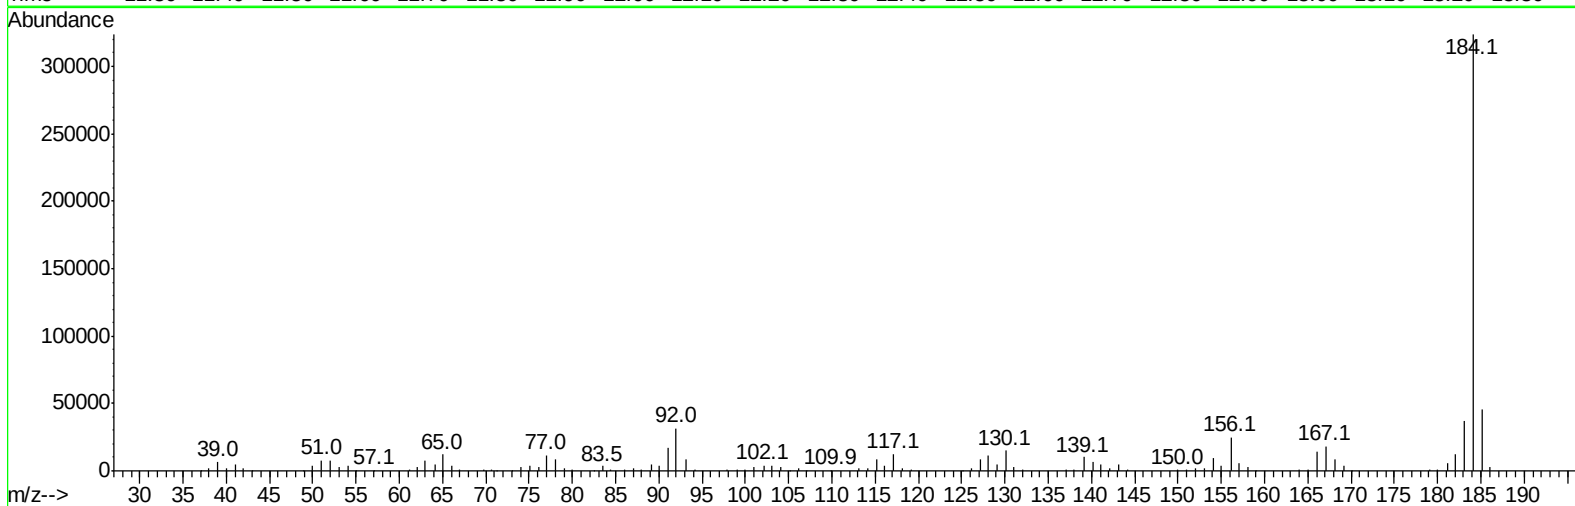


Data Path : Z:\HPCHEM1\BNA F\DATA\BF080317\  
Data File : BF097321.D  
Acq On : 3 Aug 2017 17:19  
Operator : SJ/JU  
Sample : DFTPP  
Misc :  
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Aug 04 08:12:48 2017  
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF072517.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Fri Aug 04 01:17:22 2017  
Response via : Initial Calibration

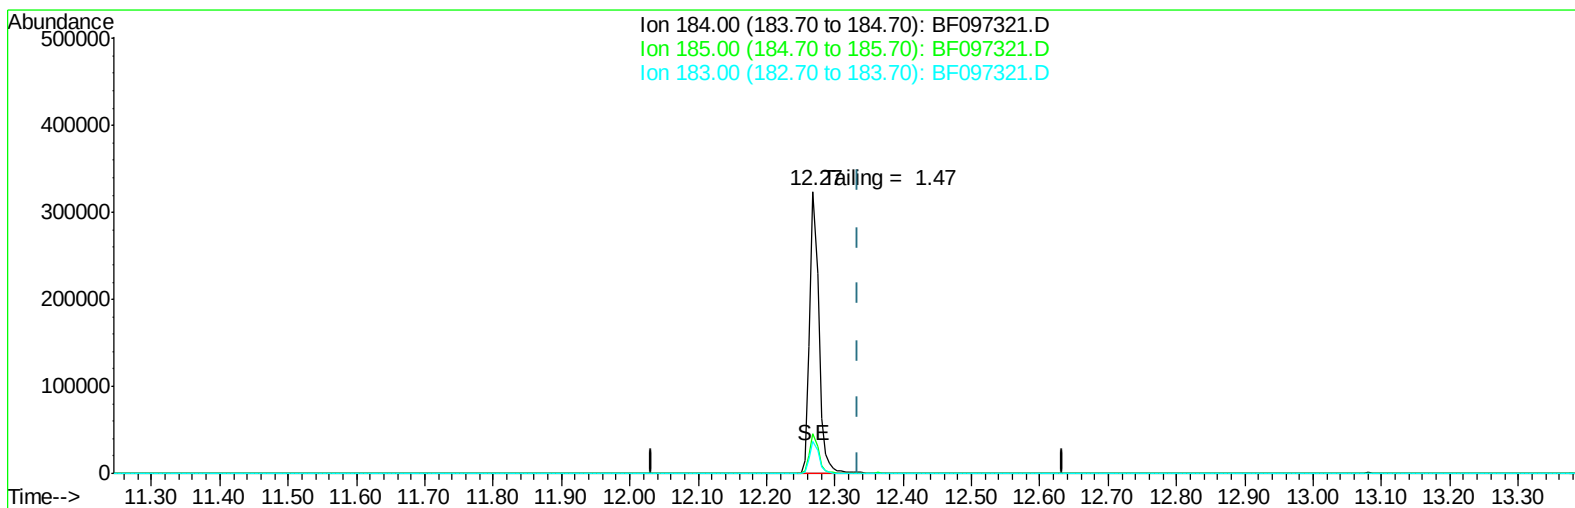

TIC: BF097321.D

(76) Benzidine



12.268min (-0.065) 0.00ng

response 293172

| Ion    | Exp%  | Act%   |
|--------|-------|--------|
| 184.00 | 100   | 100    |
| 185.00 | 19.40 | 14.18# |
| 183.00 | 12.20 | 11.45  |
| 0.00   | 0.00  | 0.00   |

Data Path : Z:\HPCHEM1\BNA F\DATA\BF080317\  
Data File : BF097321.D  
Acq On : 3 Aug 2017 17:19  
Operator : SJ/JU  
Sample : DFTPP  
Misc :  
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Aug 04 08:12:48 2017  
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF072517.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Fri Aug 04 01:17:22 2017  
Response via : Initial Calibration

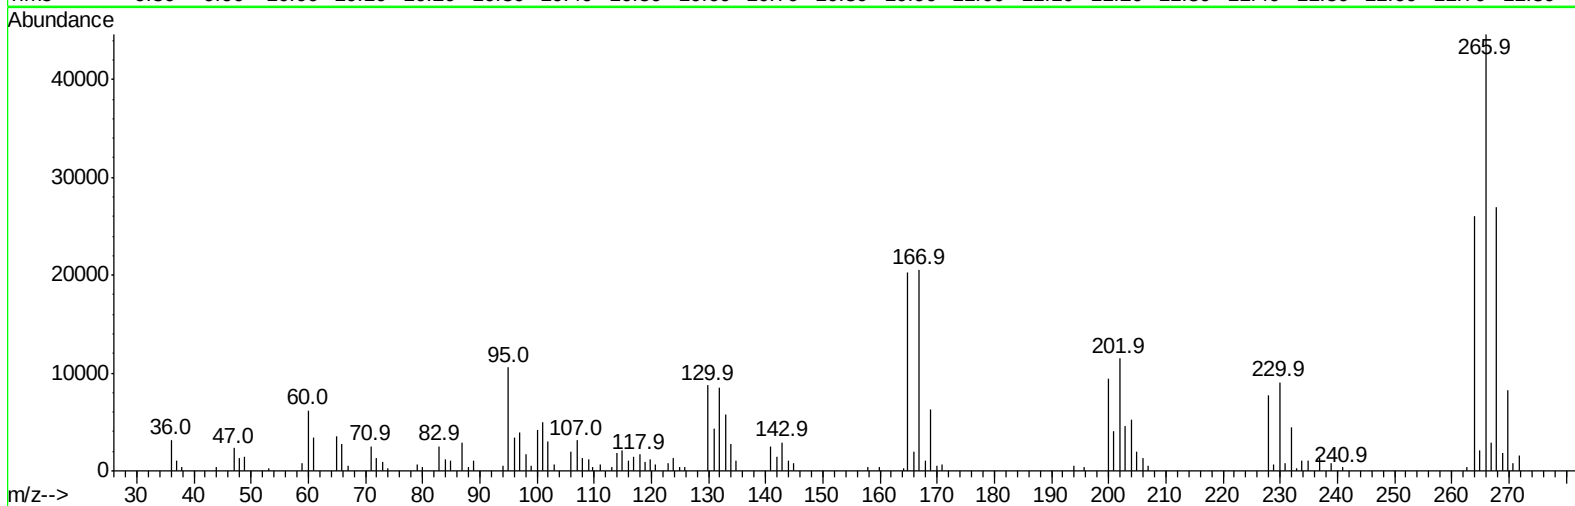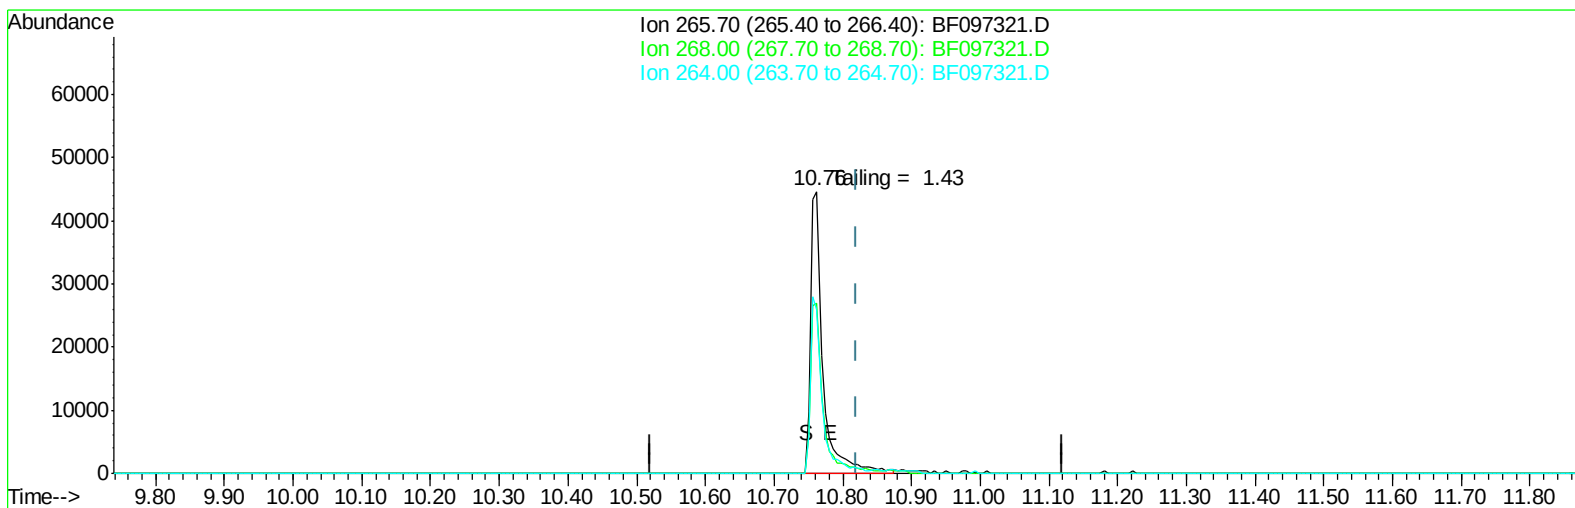

TIC: BF097321.D

(69) Pentachlorophenol (C)

10.762min (-0.059) 99125.05ng

response 53702

| Ion    | Exp%  | Act%  |
|--------|-------|-------|
| 265.70 | 100   | 100   |
| 268.00 | 63.90 | 60.39 |
| 264.00 | 64.60 | 58.24 |
| 0.00   | 0.00  | 0.00  |