


Data Path : Z:\HPCHEM1\BNA F\DATA\BF080317\
 Data File : BF097321.D
 Acq On : 3 Aug 2017 17:19
 Operator : SJ/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF072517.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri Aug 04 01:17:22 2017

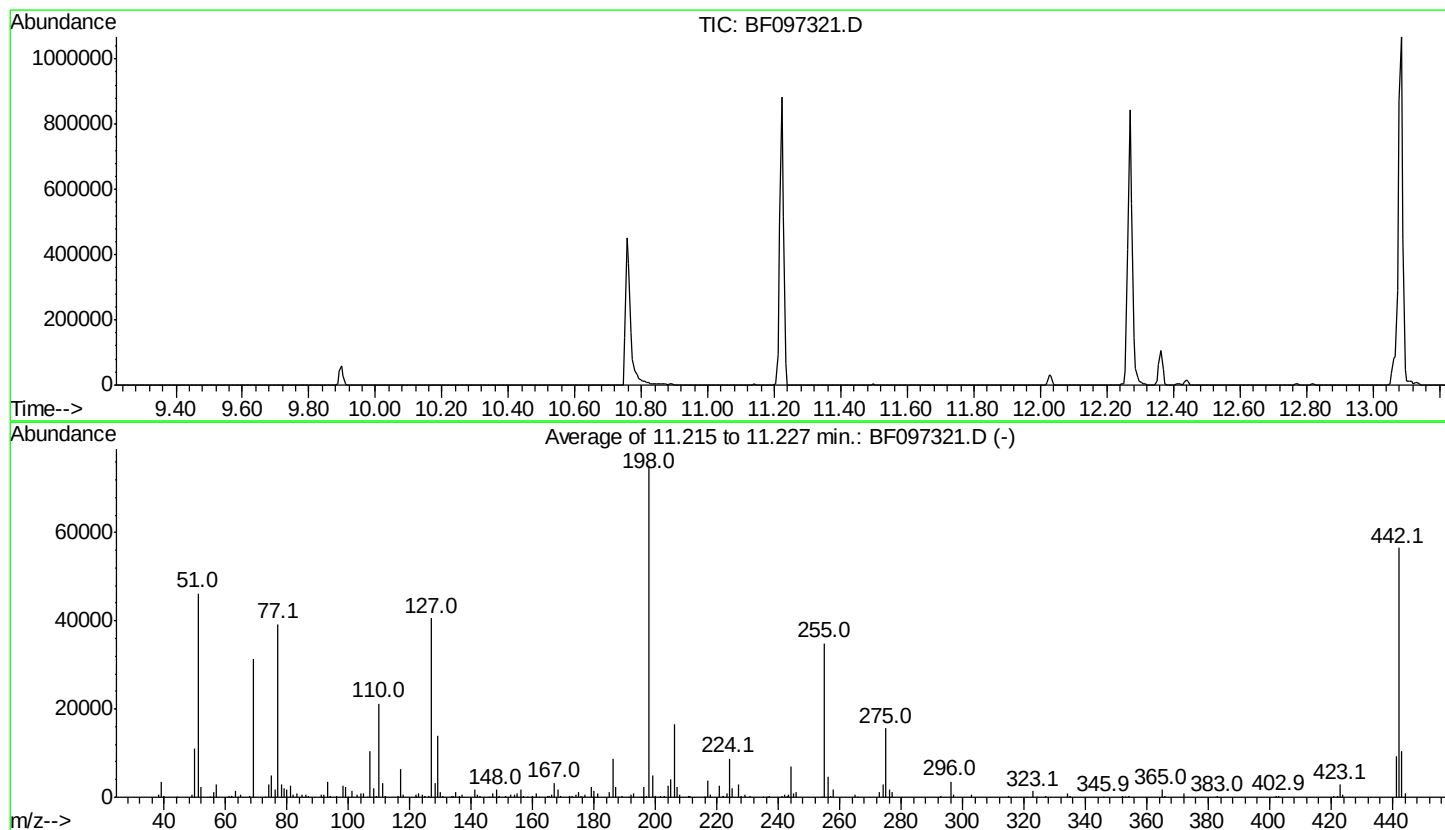

AutoFind: Scans 1586, 1587, 1588; Background Corrected with Scan 1581

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	61.5	46258	PASS
68	69	0.00	2	1.3	413	PASS
69	198	0.00	100	41.6	31266	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	54.0	40584	PASS
197	198	0.00	2	0.5	352	PASS
198	198	100	100	100.0	75192	PASS
199	198	5	9	6.4	4814	PASS
275	198	10	60	20.7	15594	PASS
365	198	1	100	2.2	1627	PASS
441	442	0.01	24	16.5	9332	PASS
442	198	50	100	75.1	56498	PASS
443	442	15	24	18.4	10414	PASS