


Data Path : Z:\HPCHEM1\BNA F\DATA\BF080317\
Data File : BF097347.D
Acq On : 4 Aug 2017 8:08
Operator : SJ/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF072517.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Fri Aug 04 01:17:22 2017

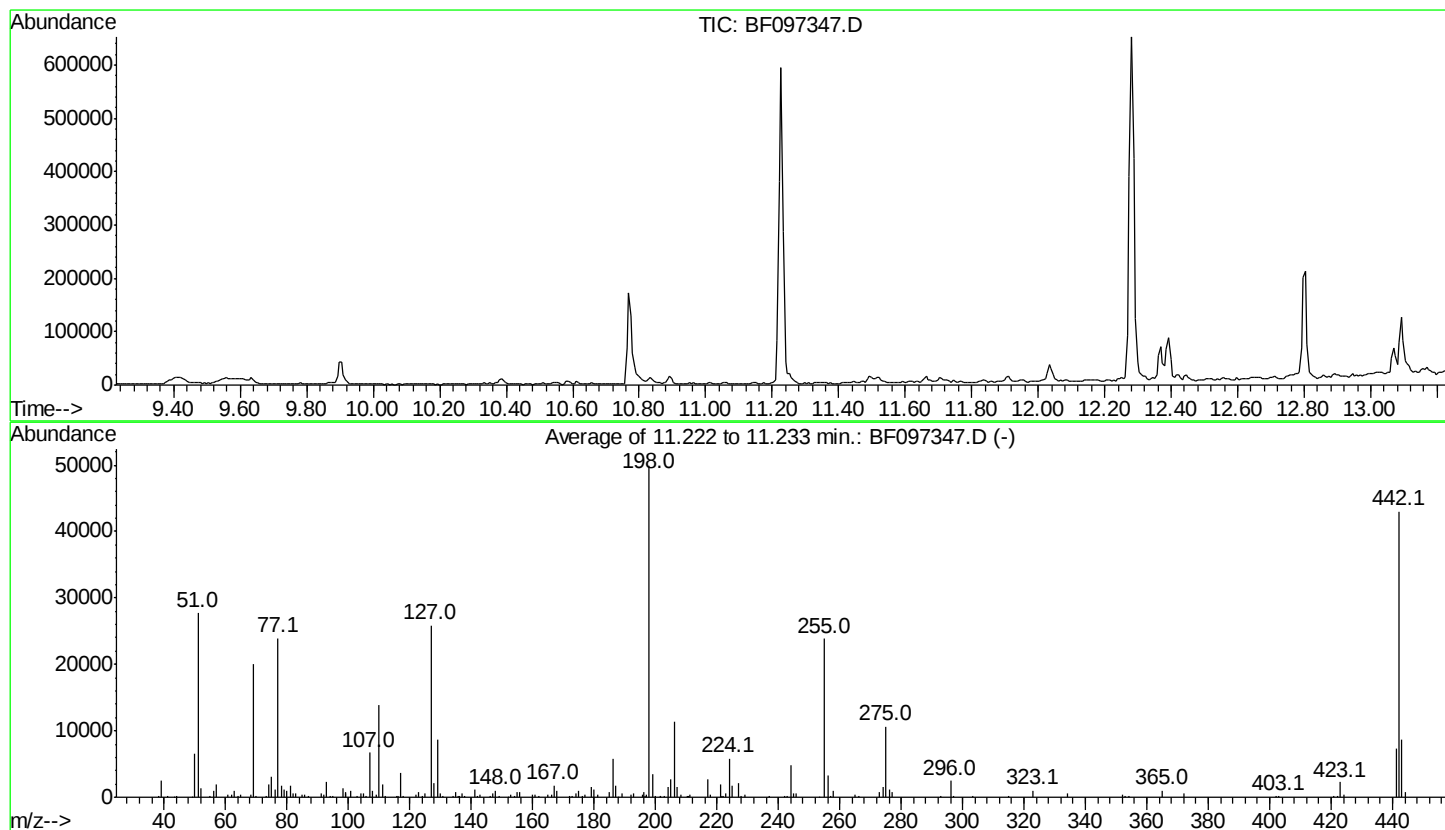

AutoFind: Scans 1587, 1588, 1589; Background Corrected with Scan 1582

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	55.8	27845	PASS
68	69	0.00	2	1.8	367	PASS
69	198	0.00	100	40.0	19966	PASS
70	69	0.00	2	0.6	118	PASS
127	198	10	80	51.9	25912	PASS
197	198	0.00	2	0.9	427	PASS
198	198	100	100	100.0	49914	PASS
199	198	5	9	6.9	3424	PASS
275	198	10	60	21.2	10603	PASS
365	198	1	100	2.1	1036	PASS
441	442	0.01	24	17.1	7346	PASS
442	198	50	100	86.2	43010	PASS
443	442	15	24	20.0	8613	PASS