

Data Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF080318\
 Data File : BF107947.D
 Acq On : 3 Aug 2018 19:33
 Operator : JU/SJ
 Sample : J4318-01
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 BEEBEE-SITE-DEMO-1

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0
 Filtering: 5
 Min Area: 3 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF073018.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.178	480	483	488	rBV4	7347	14312	1.56%	0.242%
2	6.684	731	739	740	rBV4	9021	16964	1.85%	0.286%
3	6.772	748	754	759	rBV5	19212	49726	5.43%	0.839%
4	6.960	782	786	804	rBV	161261	510780	55.79%	8.620%
5	7.107	808	811	825	rVB2	47509	123351	13.47%	2.082%
6	7.584	885	892	893	rBV4	6523	10432	1.14%	0.176%
7	8.236	999	1003	1031	rBV	346777	841692	91.93%	14.205%
8	9.313	1182	1186	1193	rBV	70705	144398	15.77%	2.437%
9	9.989	1297	1301	1322	rBV	677341	915559	100.00%	15.452%
10	10.801	1435	1439	1448	rBV3	32112	77563	8.47%	1.309%
11	10.872	1448	1451	1459	rVB5	15184	28776	3.14%	0.486%
12	11.319	1524	1527	1530	rBV	15572	14633	1.60%	0.247%
13	11.489	1552	1556	1572	rBV	461613	866715	94.67%	14.627%
14	11.677	1586	1588	1593	rVB4	9492	12206	1.33%	0.206%
15	11.748	1597	1600	1604	rVV2	14838	14891	1.63%	0.251%
16	11.995	1638	1642	1646	rBV4	51775	85882	9.38%	1.449%
17	12.030	1646	1648	1655	rVB	40879	52139	5.69%	0.880%
18	12.154	1666	1669	1672	rVB	22791	22543	2.46%	0.380%
19	12.466	1720	1722	1725	rBV3	8527	9296	1.02%	0.157%
20	12.542	1732	1735	1738	rBV2	27378	24835	2.71%	0.419%
21	12.713	1760	1764	1770	rBV	55364	94151	10.28%	1.589%
22	12.777	1773	1775	1780	rBV6	14767	23093	2.52%	0.390%
23	12.918	1796	1799	1800	rBV2	14870	14591	1.59%	0.246%
24	12.942	1800	1803	1808	rVB	47203	66148	7.22%	1.116%
25	13.071	1821	1825	1832	rBV	139043	202094	22.07%	3.411%
26	14.142	2003	2007	2018	rBV	548148	903562	98.69%	15.249%
27	15.671	2263	2267	2281	rVB2	398704	785034	85.74%	13.249%


Sum of corrected areas: 5925366

Data Path : Z:\SVOASRV\HPCHEM1\BNA F\DATA\BF080318\
Data File : BF107947.D
Acq On : 3 Aug 2018 19:33
Operator : JU/SJ
Sample : J4318-01
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
BEEBEE-SITE-DEMO-1

Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF073018.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

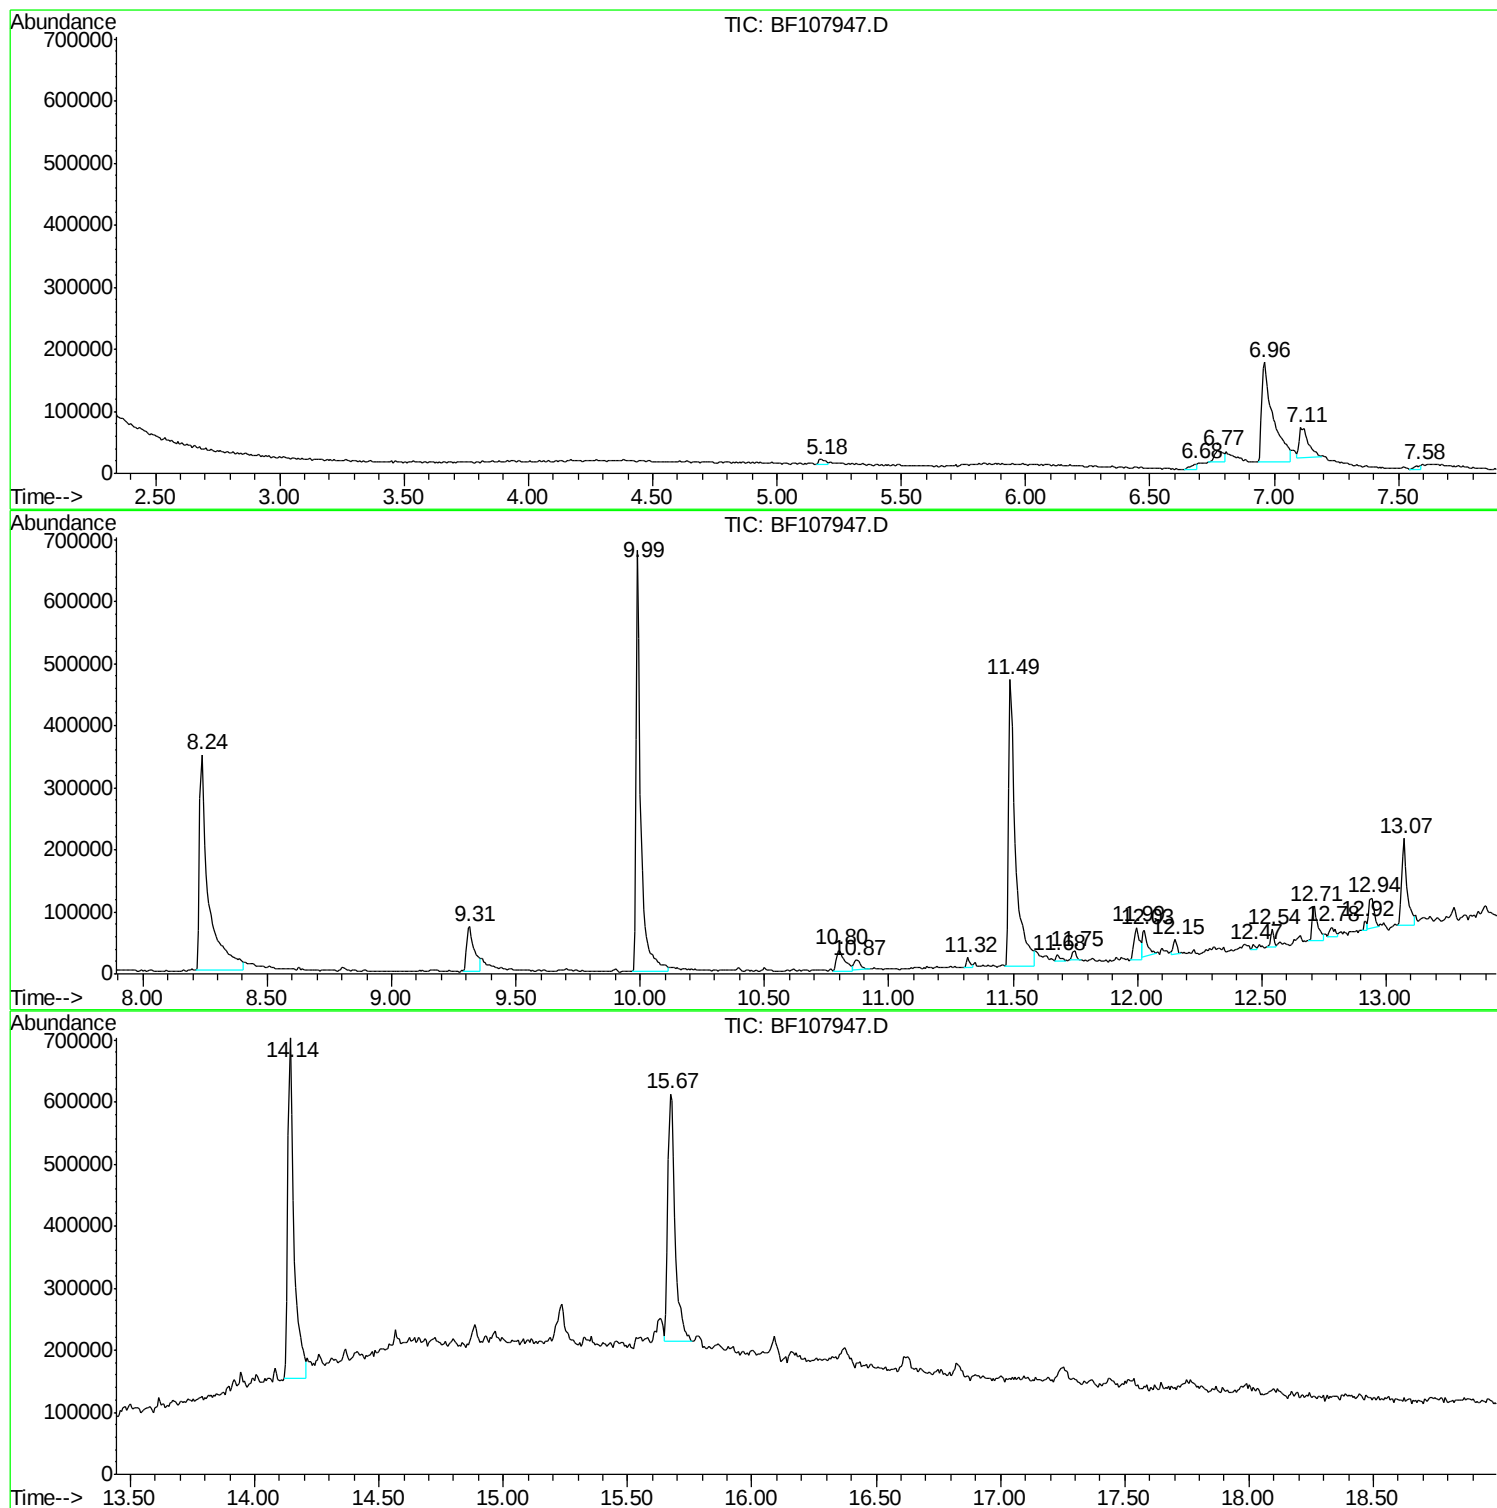

Data_Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF080318\
Data_File : BF107947.D
Acq_On : 3_Aug_2018_ 19:333
Operator : JU/SJJ
Sample : J4318-011
Misc :
ALS_Vial : 14 Sample_Multiplier: 11

Instrument :
BNA_F
ClientSampleId :
BEEBEE-SITE-DEMO-1

Quant_Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF073018.MM
Quant_Title : ASP. BNA. STANDARDS. FOR. 5. POINT. CALIBRATIONN

TIC_Library : C:\DATABASE\NIST11.LL
TIC_Integration Parameters: LSCINT.PP

TIC Top Hit name	RT	EstConc	Units	Response	Internal Standard
				#	RT Resp Conc

No Library Search Compounds Detected
