
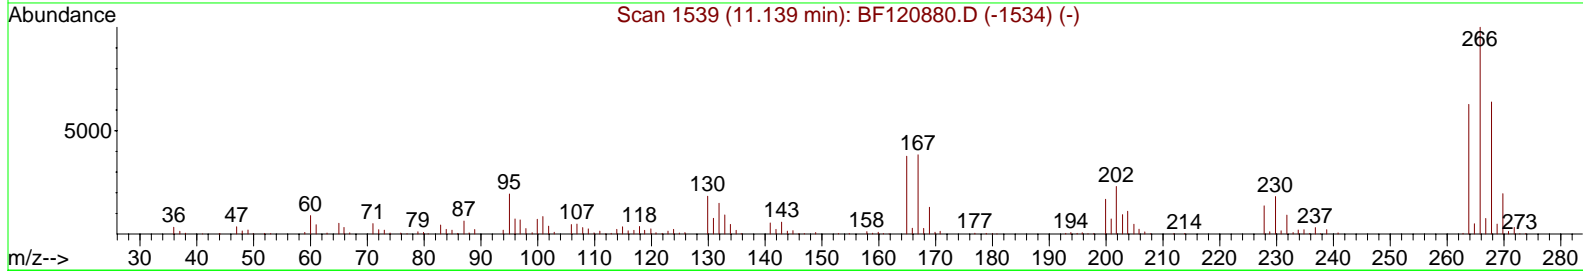
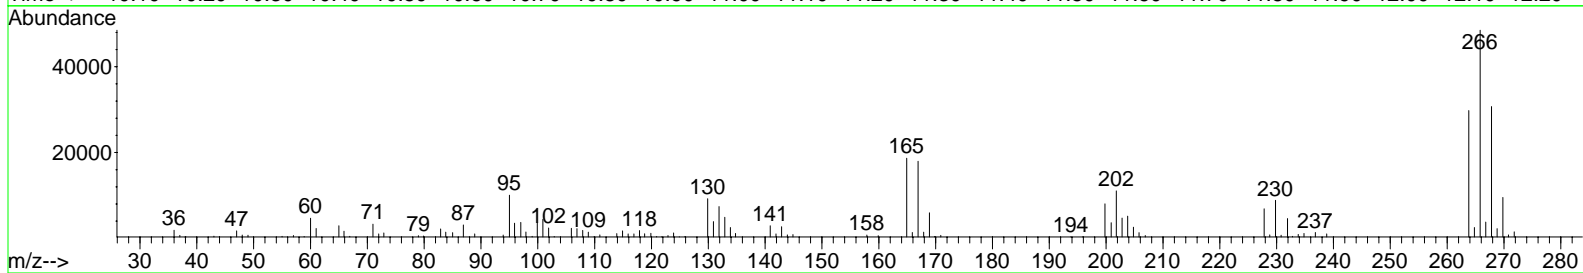


Data Path : Z:\SVOASRV\HPCHEM1\BNA F\DATA\BF080320\
 Data File : BF121171.D
 Acq On : 3 Aug 2020 9:23
 Operator : JU/CG
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Aug 03 18:34:57 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF071620.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Jul 29 14:55:43 2020
 Response via : Initial Calibration

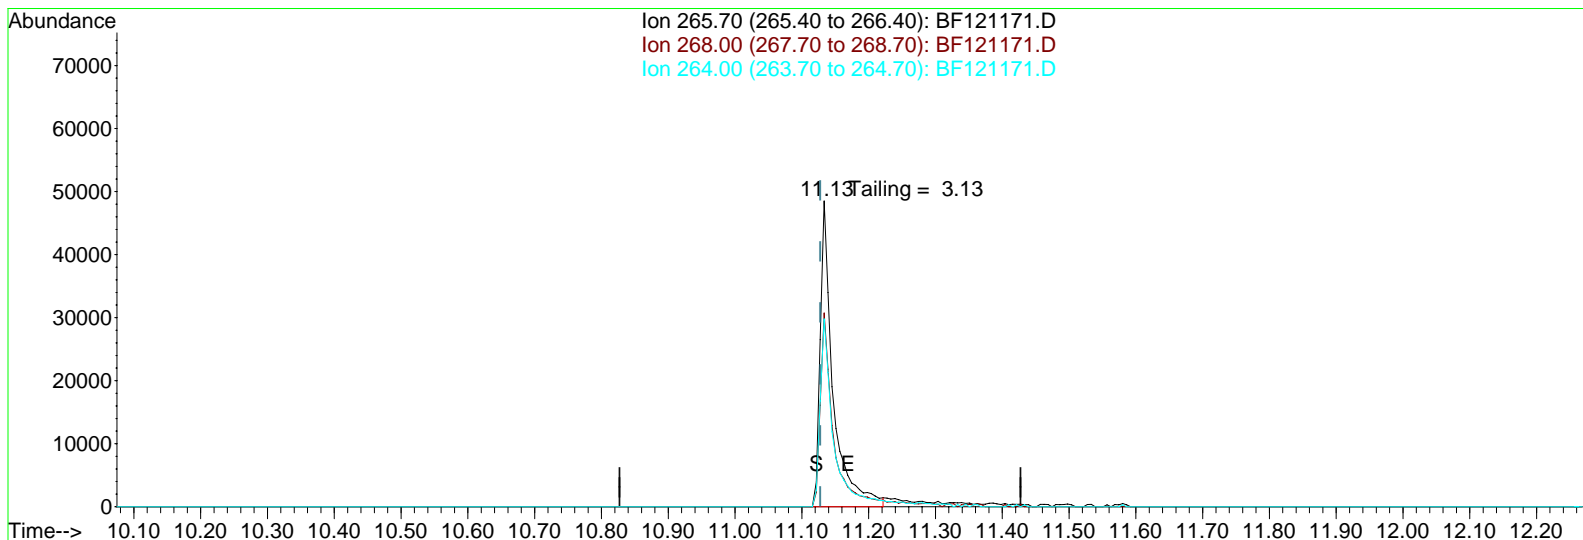

(70) Pentachlorophenol (C)




11.133min (+0.006) 30297.20ng

response 68661

Ion	Exp%	Act%
265.70	100	100
268.00	62.10	63.36
264.00	63.00	61.43
0.00	0.00	0.00

Data Path : Z:\SVOASRV\HPCHEM1\BNA F\DATA\BF080320\
 Data File : BF121171.D
 Acq On : 3 Aug 2020 9:23
 Operator : JU/CG
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Aug 03 18:34:57 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF071620.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Jul 29 14:55:43 2020
 Response via : Initial Calibration

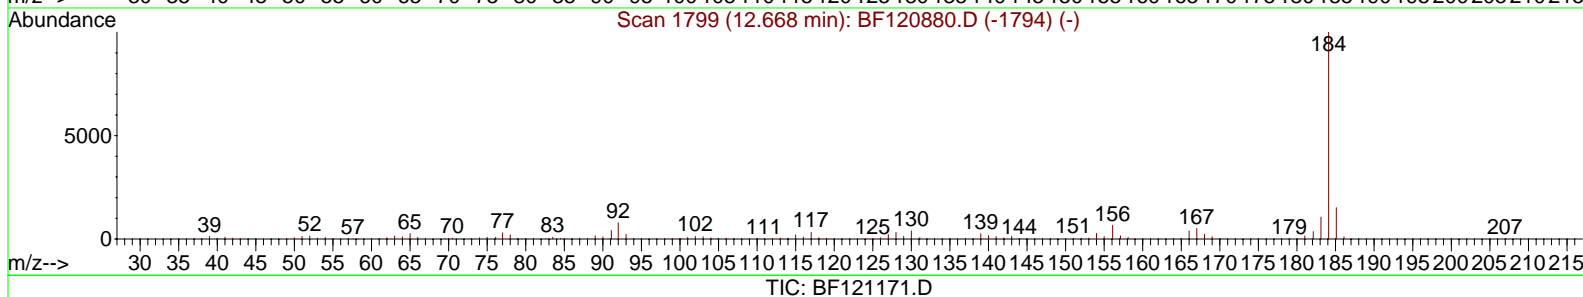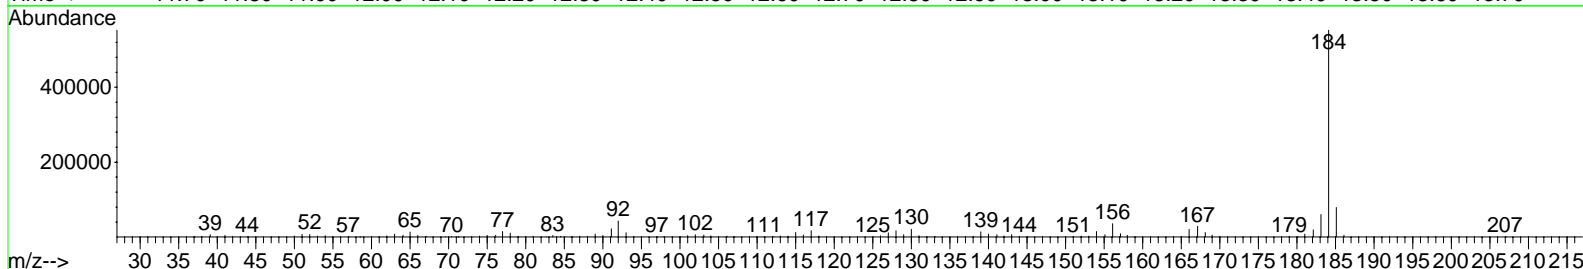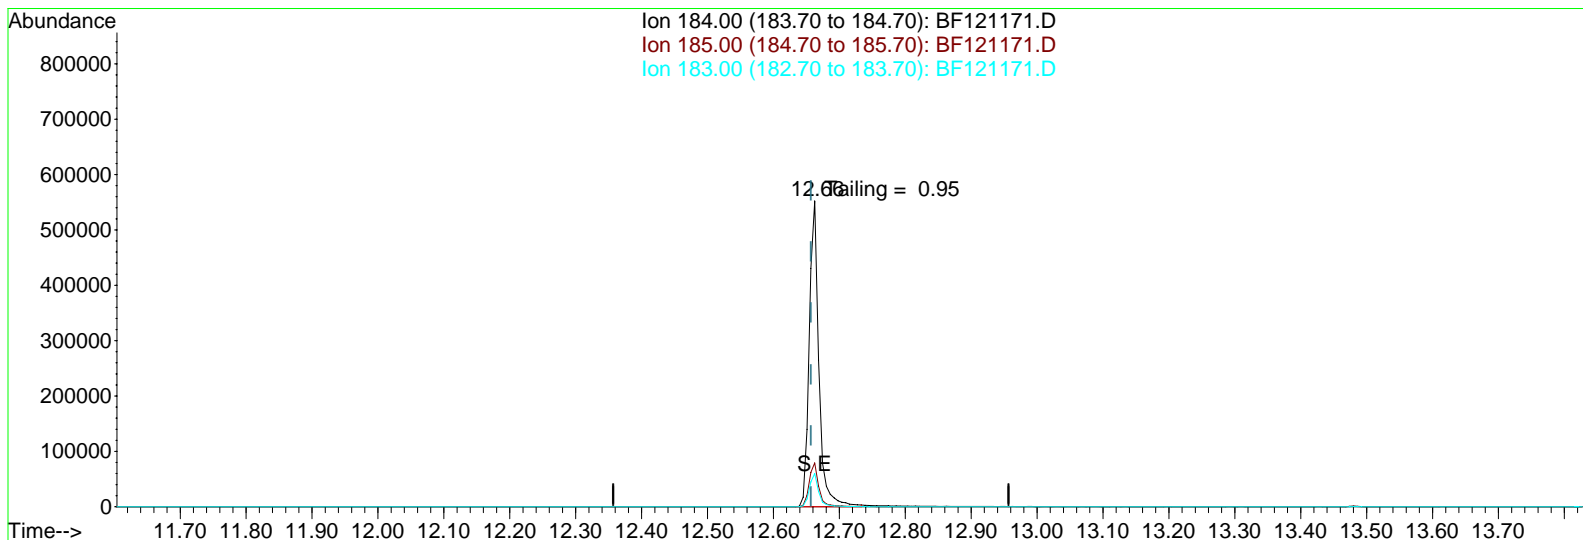

(77) Benzidine

12.663min (+0.006) 0.00ng

response 573077

Ion	Exp%	Act%
184.00	100	100
185.00	15.10	14.33
183.00	11.20	10.89
0.00	0.00	0.00