


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF080320\
 Data File : BF121171.D
 Acq On : 3 Aug 2020 9:23
 Operator : JU/CG
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF071620.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed Jul 29 14:55:43 2020

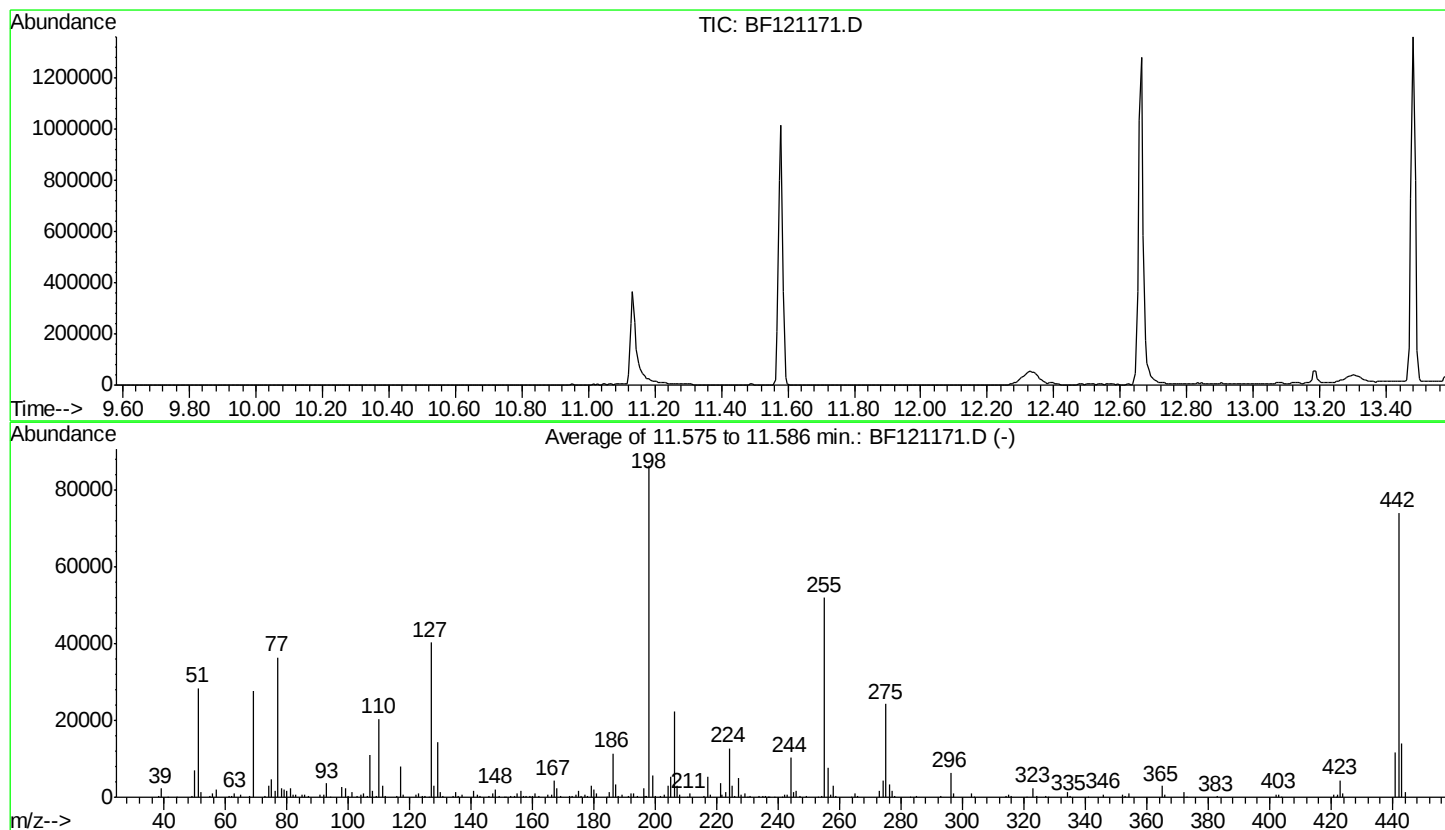

AutoFind: Scans 1613, 1614, 1615; Background Corrected with Scan 1608

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	33.0	28466	PASS
68	69	0.00	2	1.4	377	PASS
69	198	0.00	100	31.9	27591	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	46.6	40236	PASS
197	198	0.00	2	0.5	435	PASS
198	198	100	100	100.0	86373	PASS
199	198	5	9	6.6	5736	PASS
275	198	10	60	28.1	24304	PASS
365	198	1	100	3.4	2960	PASS
441	198	0.01	100	13.5	11643	PASS
442	198	50	100	85.7	74053	PASS
443	442	15	24	18.9	13975	PASS