
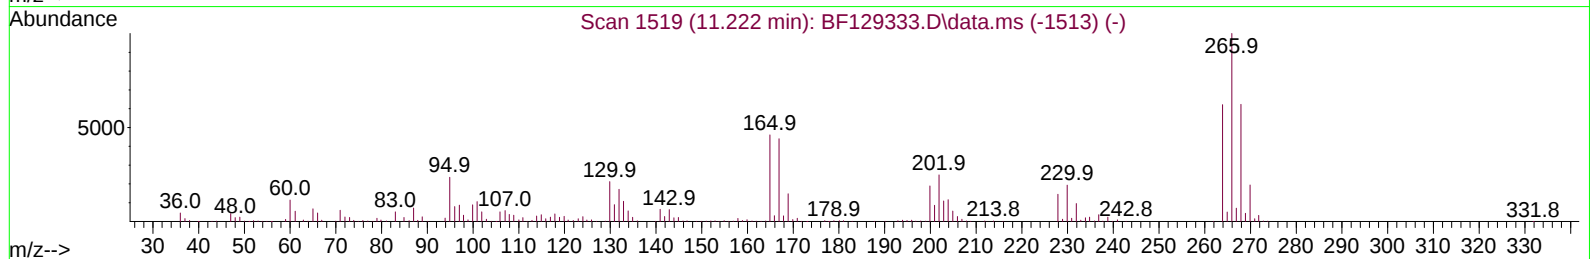
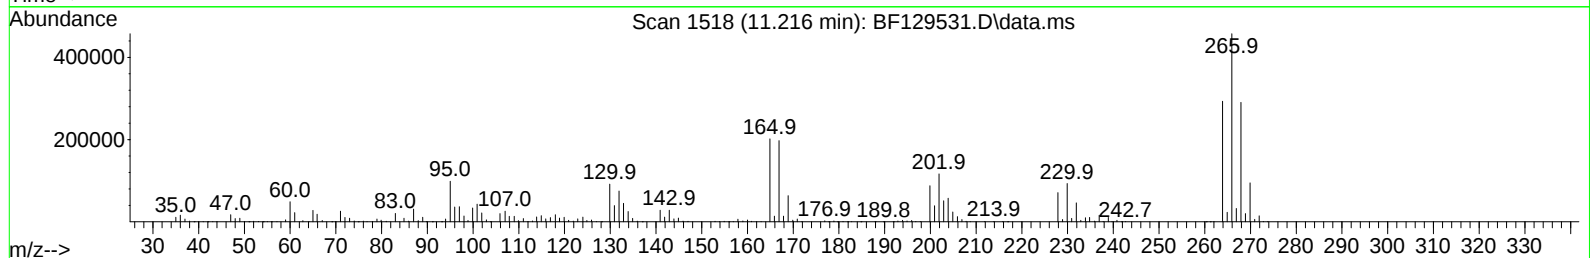


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF080322\
Data File : BF129531.D
Acq On : 03 Aug 2022 09:57
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Aug 03 16:44:02 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF072522.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Aug 02 01:11:25 2022
Response via : Initial Calibration

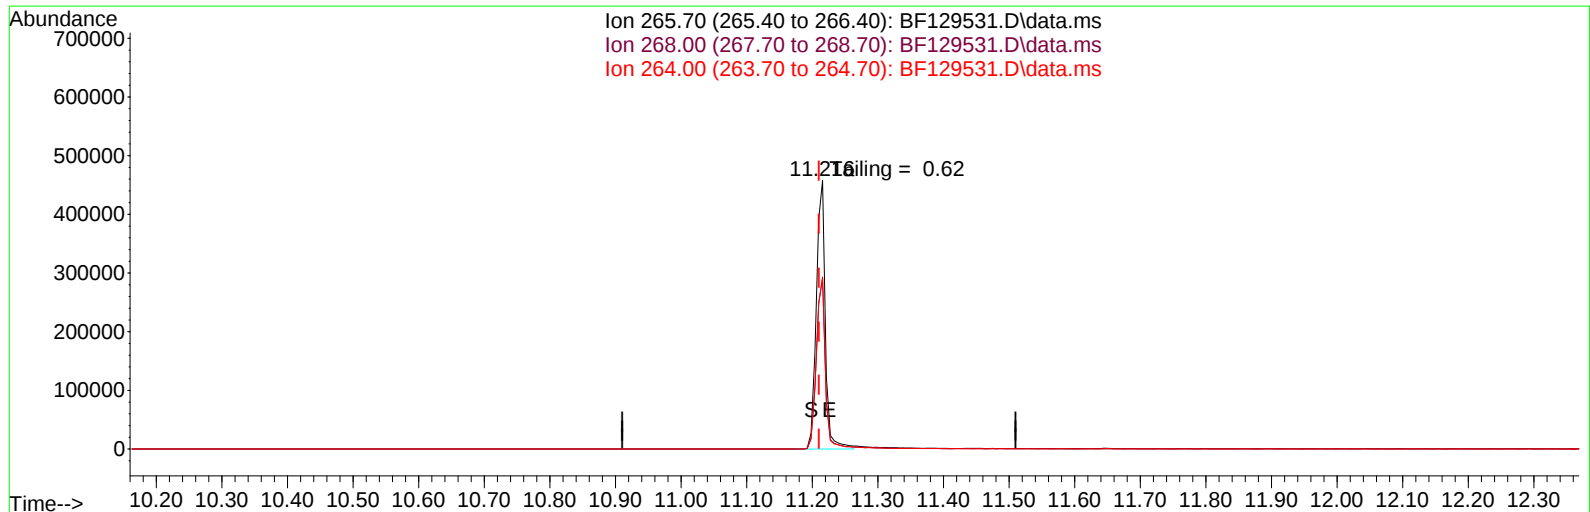

TIC: BF129531.D\data.ms

(70) Pentachlorophenol (C)




11.216min (+ 0.006) 531006.32 ng

response 452111

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.70	63.54
264.00	61.80	64.10
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF080322\
 Data File : BF129531.D
 Acq On : 03 Aug 2022 09:57
 Operator : CG\JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Aug 03 16:44:02 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF072522.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Aug 02 01:11:25 2022
 Response via : Initial Calibration

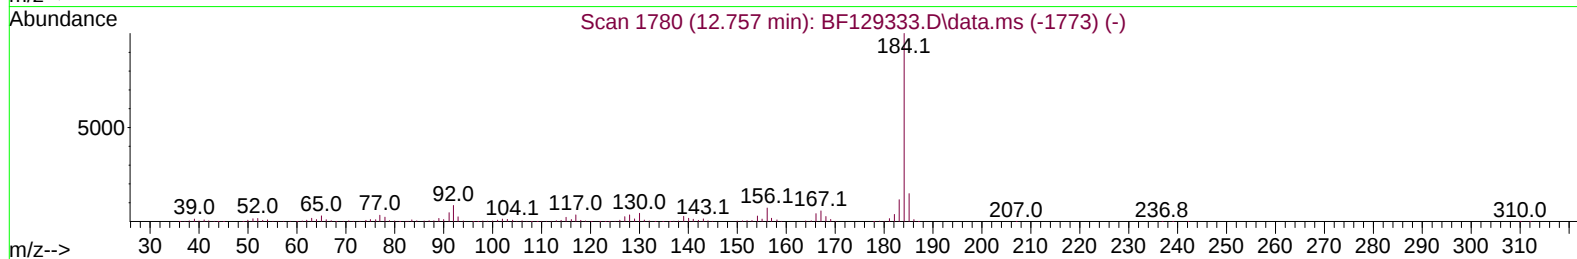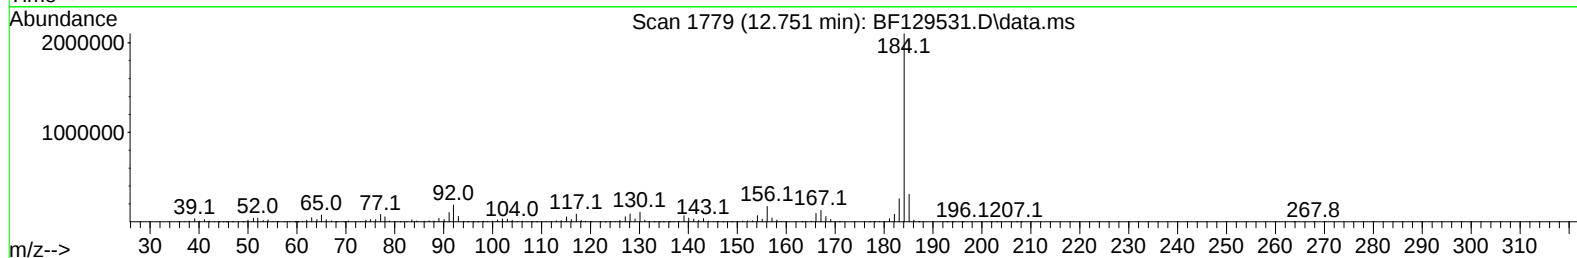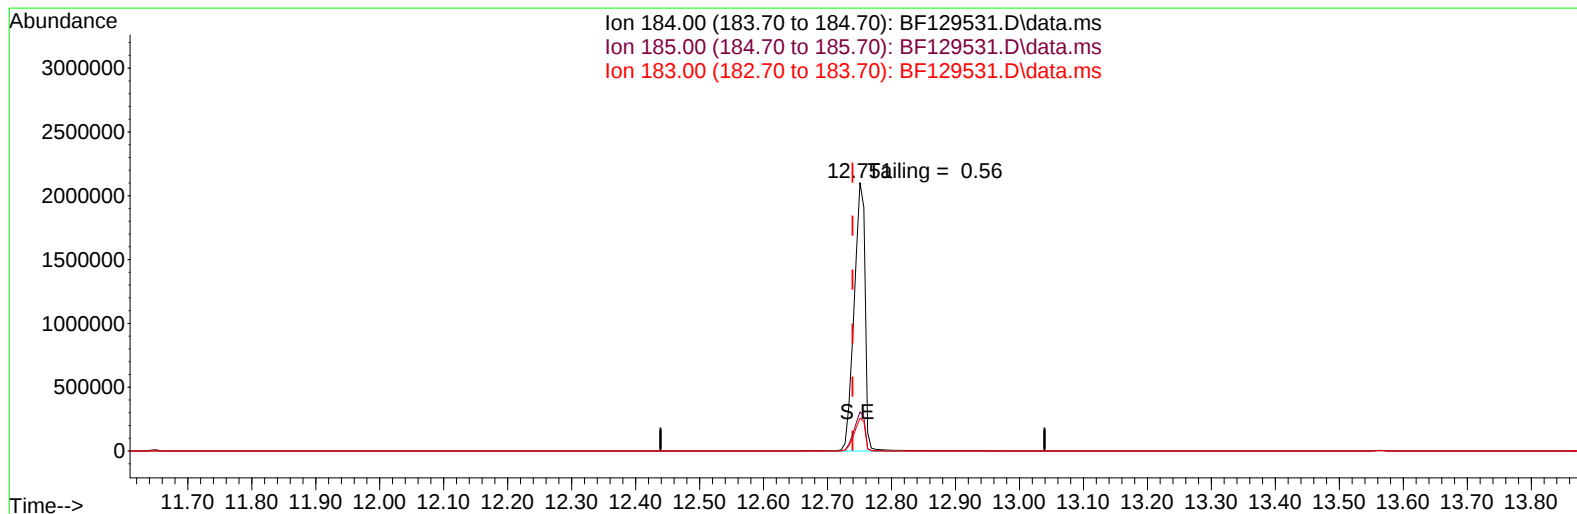

TIC: BF129531.D\data.ms

(77) Benzidine

12.751min (+ 0.012) 25800.02 ng

response 2516515

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.90	14.62
183.00	11.60	12.23
0.00	0.00	0.00