
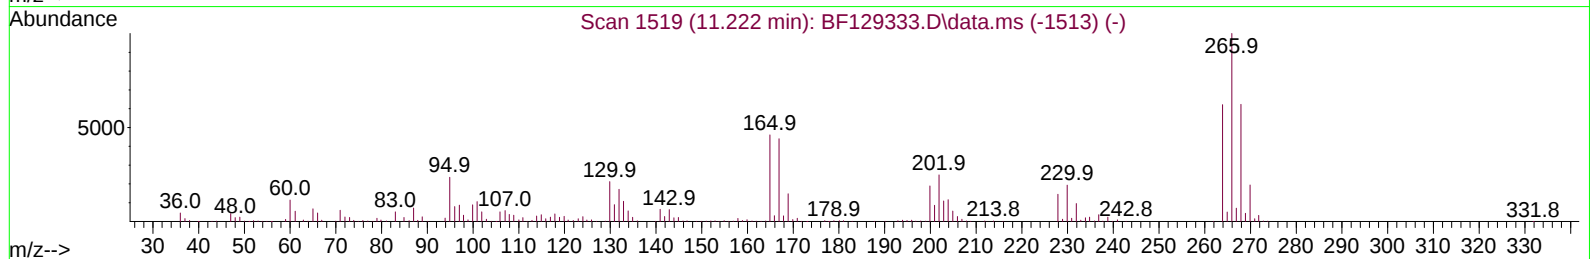
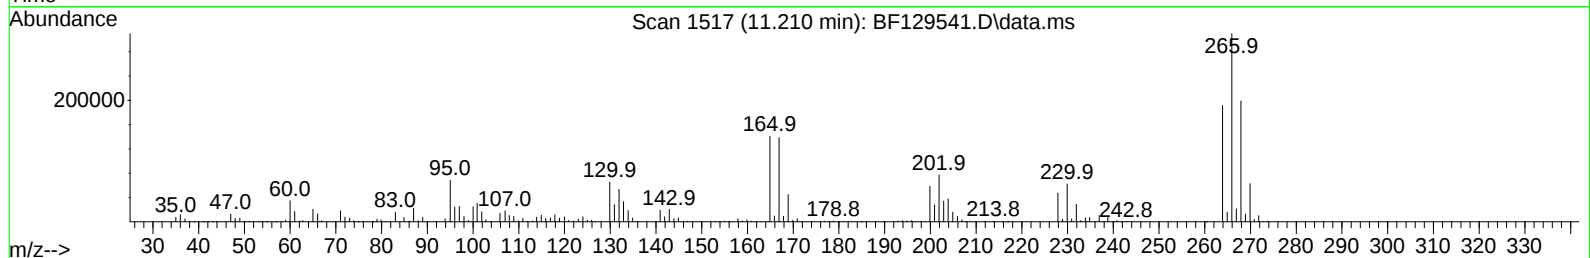


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF080322\
Data File : BF129541.D
Acq On : 03 Aug 2022 15:31
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Aug 03 17:44:49 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF072522.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Aug 02 01:11:25 2022
Response via : Initial Calibration

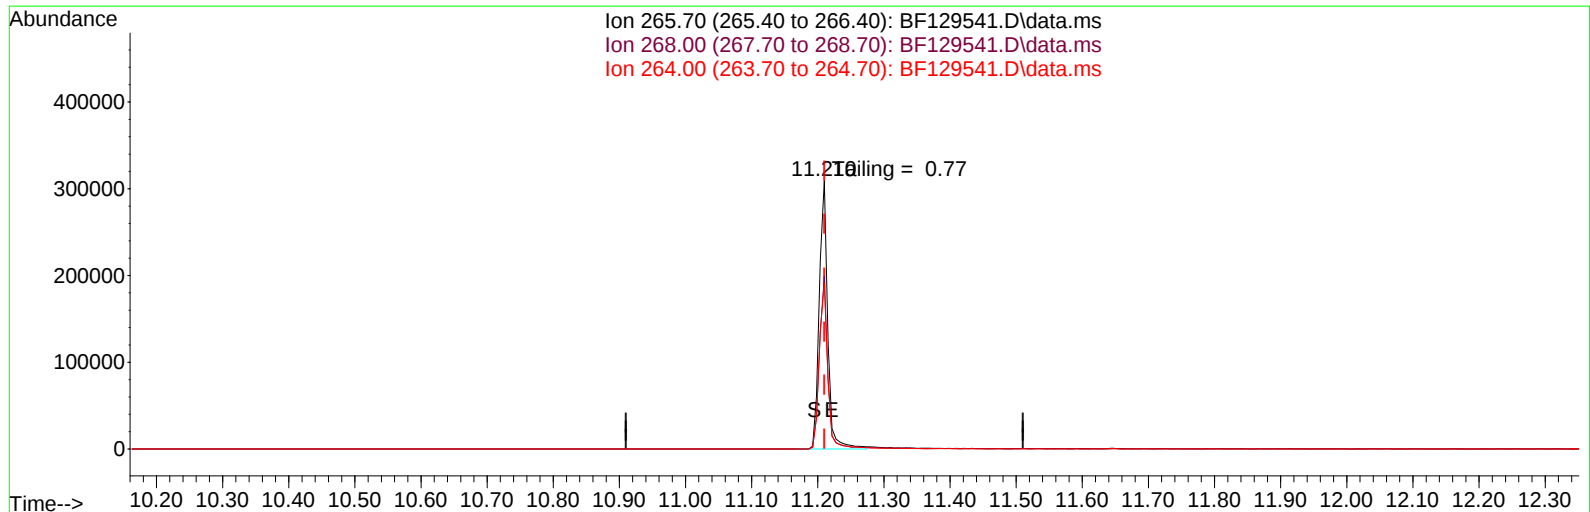

TIC: BF129541.D\data.ms

(70) Pentachlorophenol (C)




11.210min (-0.000) 114985.32 ng

response 283320

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.70	64.32
264.00	61.80	61.85
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF080322\
Data File : BF129541.D
Acq On : 03 Aug 2022 15:31
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Aug 03 17:44:49 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF072522.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Aug 02 01:11:25 2022
Response via : Initial Calibration

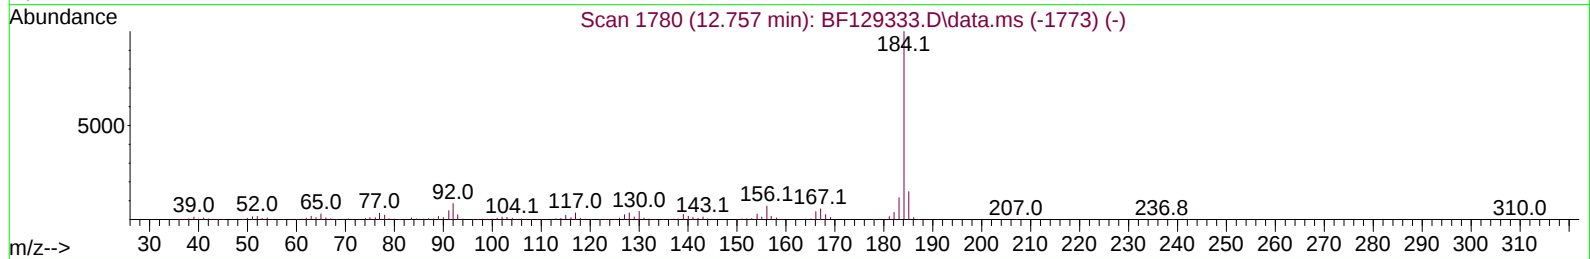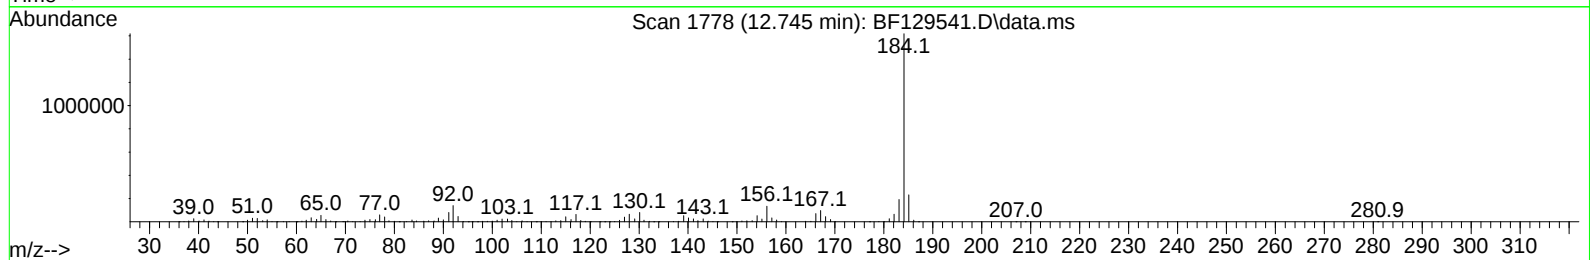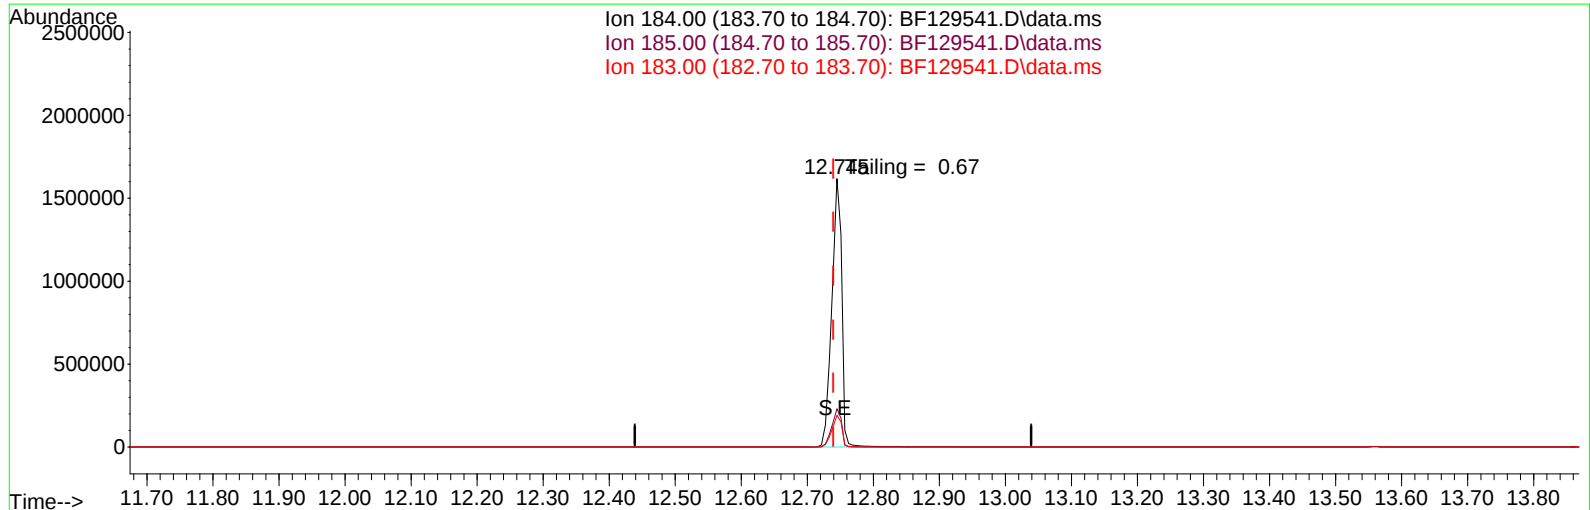

TIC: BF129541.D\data.ms

(77) Benzidine

12.745min (+ 0.006) 119110.70 ng

response 1691570

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.90	14.29
183.00	11.60	11.82
0.00	0.00	0.00