
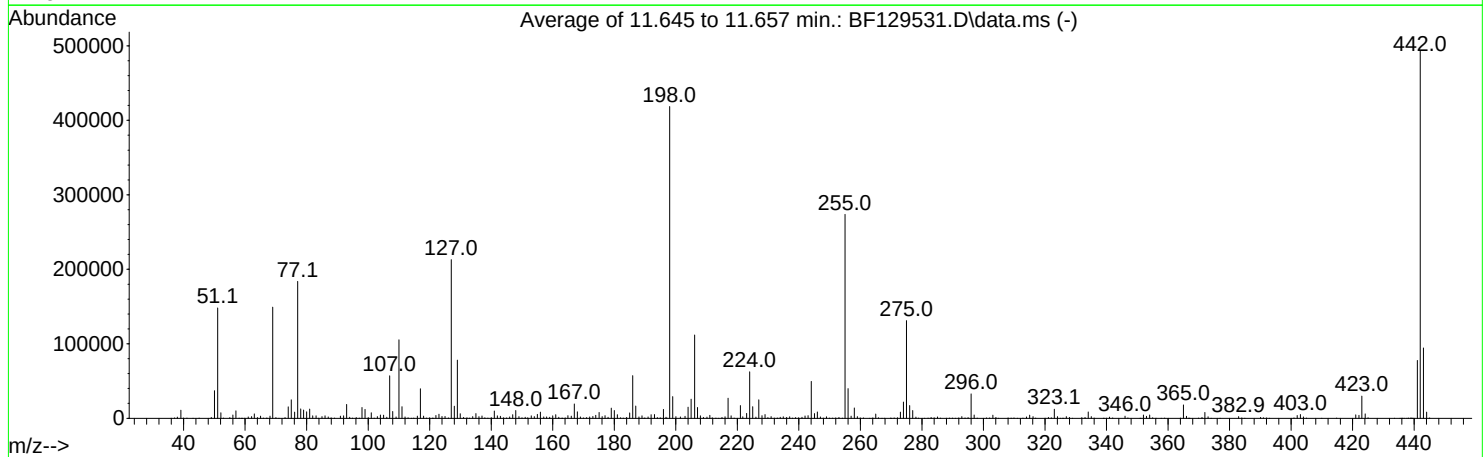


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF080322\
 Data File : BF129531.D
 Acq On : 03 Aug 2022 09:57
 Operator : CG\JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF072522.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Tue Aug 02 01:11:25 2022

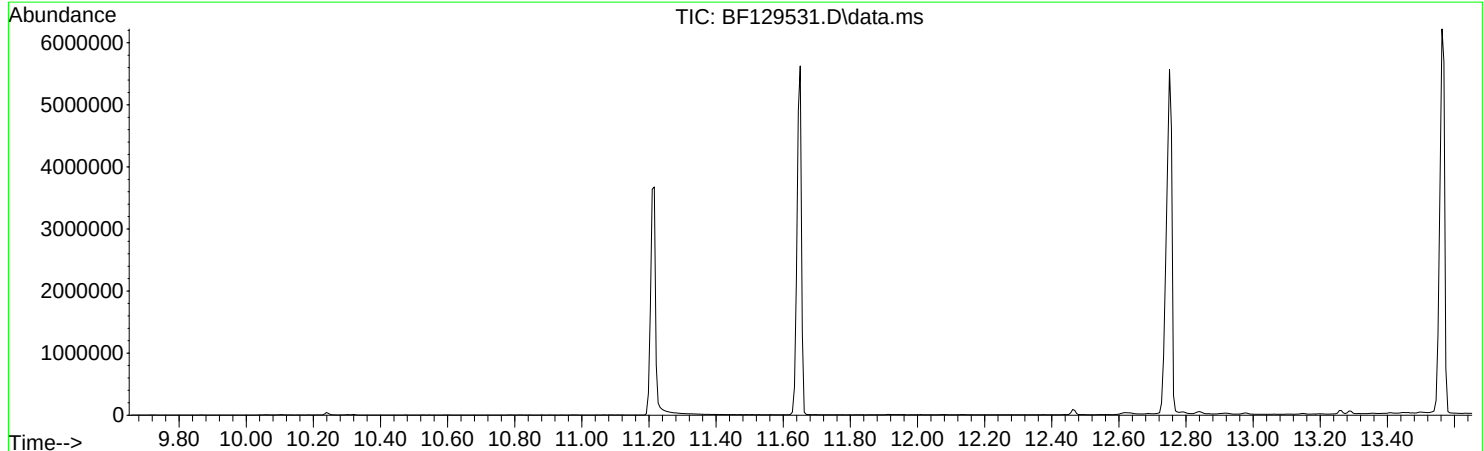




AutoFind: Scans 1591, 1592, 1593; Background Corrected with Scan 1584

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	35.4	148141	PASS
68	69	0.00	2	1.9	2878	PASS
69	198	0.00	100	35.6	149222	PASS
70	69	0.00	2	0.6	895	PASS
127	198	10	80	50.9	212936	PASS
197	198	0.00	2	0.3	1378	PASS
198	198	100	100	100.0	418651	PASS
199	198	5	9	7.0	29204	PASS
275	198	10	60	31.3	131219	PASS
365	198	1	100	4.3	17900	PASS
441	198	0.01	100	18.5	77568	PASS
442	442	50	100	100.0	493845	PASS
443	442	15	24	19.1	94397	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF080322\
Data File : BF129531.D
Acq On : 03 Aug 2022 09:57
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Aug 03 16:44:02 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF072522.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Aug 02 01:11:25 2022
Response via : Initial Calibration

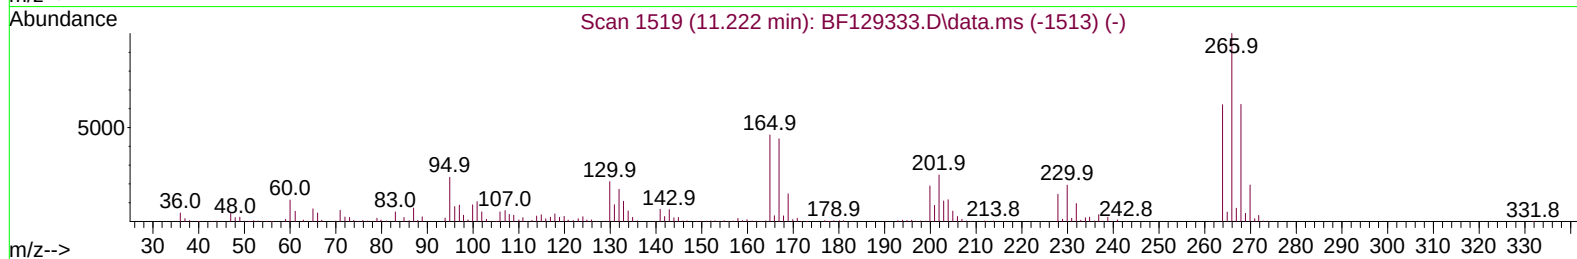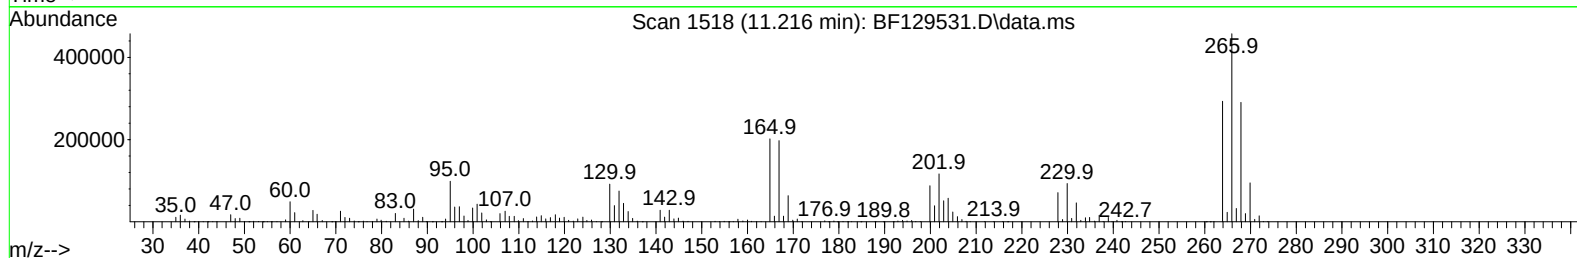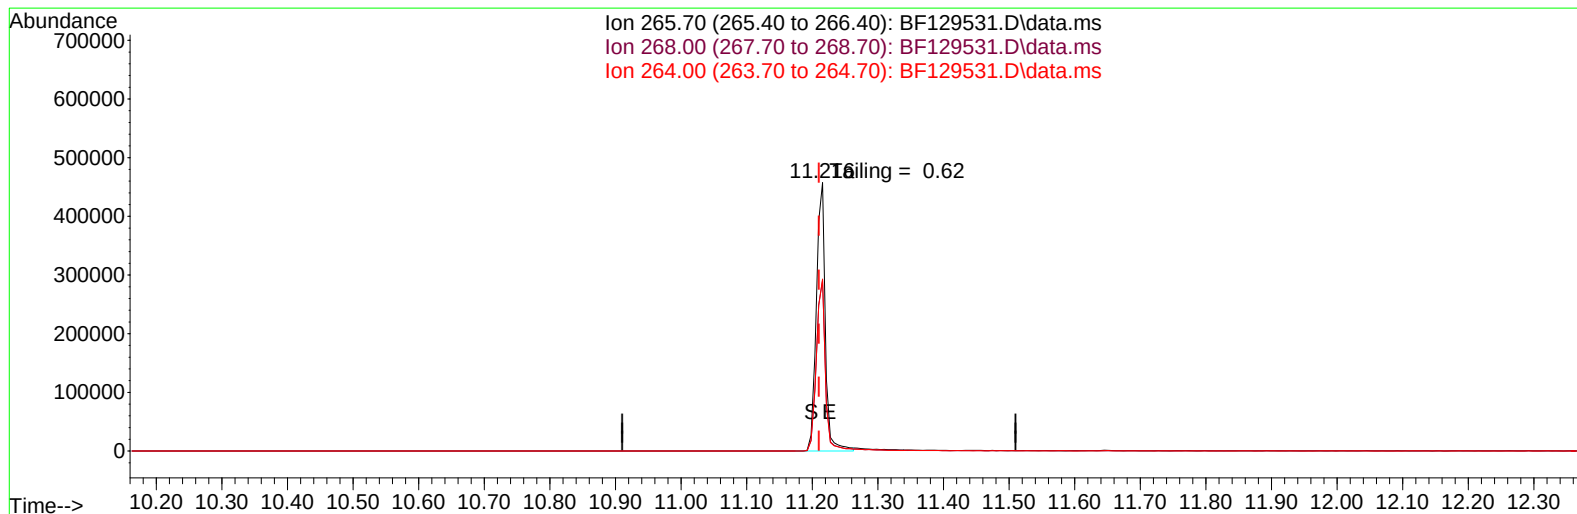

TIC: BF129531.D\data.ms

(70) Pentachlorophenol (C)

11.216min (+ 0.006) 531006.32 ng




response 452111

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.70	63.54
264.00	61.80	64.10
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF080322\
 Data File : BF129531.D
 Acq On : 03 Aug 2022 09:57
 Operator : CG\JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Quant Time: Aug 03 16:44:02 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF072522.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Aug 02 01:11:25 2022
 Response via : Initial Calibration

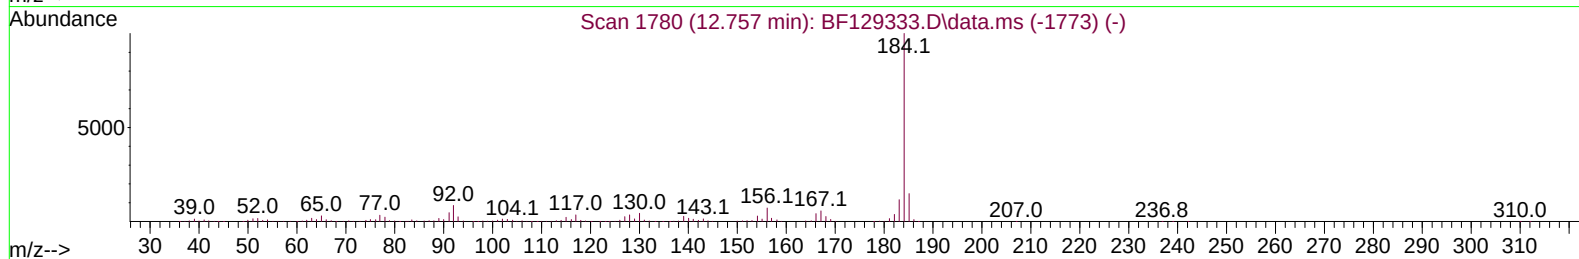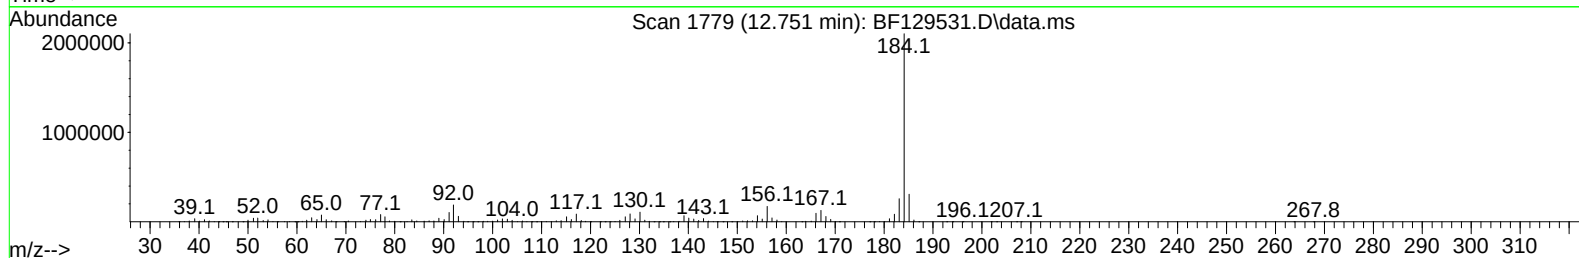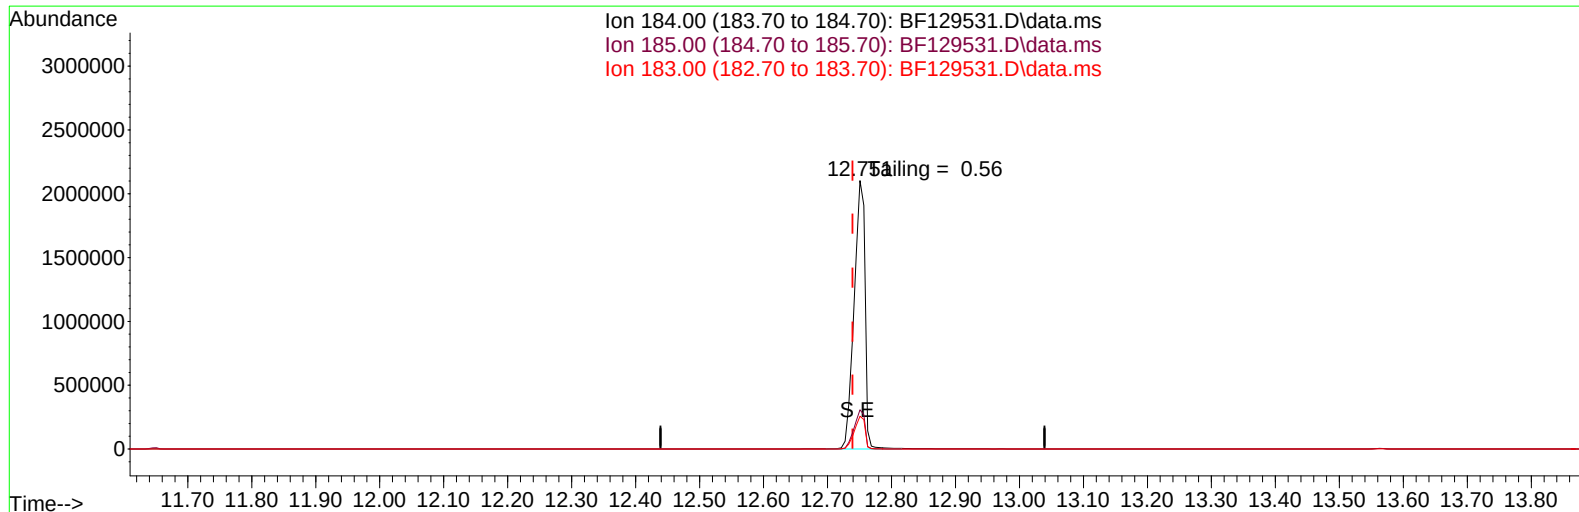

TIC: BF129531.D\data.ms

(77) Benzidine

12.751min (+ 0.012) 25800.02 ng

response 2516515

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.90	14.62
183.00	11.60	12.23
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
8/3/2022	BNA_F	<u>BF129531.D</u>
Compound Name	Response	Retention Time
DDT	1194813	13.56
DDD	10307	13.26
DDE	2358	12.92
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
12665	1207478	1.05

Instrument :
BNA_F
ClientSampleId :
DFTPP