


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF080322\
 Data File : BF129541.D
 Acq On : 03 Aug 2022 15:31
 Operator : CG\JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF072522.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Tue Aug 02 01:11:25 2022

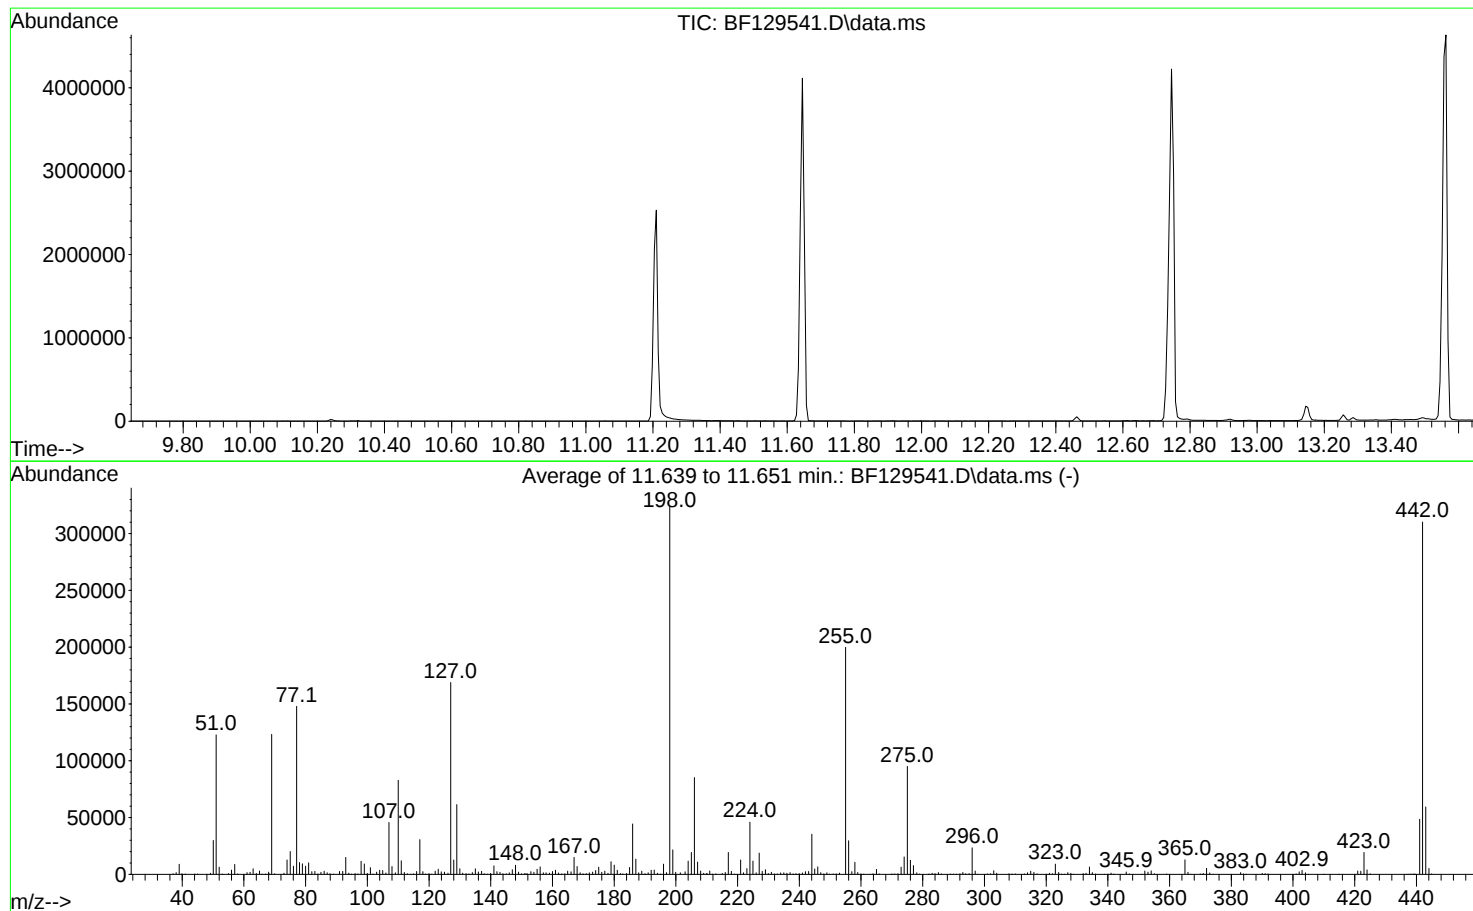




AutoFind: Scans 1590, 1591, 1592; Background Corrected with Scan 1584

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	37.9	122784	PASS
68	69	0.00	2	1.6	1929	PASS
69	198	0.00	100	38.0	123112	PASS
70	69	0.00	2	0.4	504	PASS
127	198	10	80	52.1	168763	PASS
197	198	0.00	2	0.4	1447	PASS
198	198	100	100	100.0	323819	PASS
199	198	5	9	6.6	21432	PASS
275	198	10	60	29.3	94968	PASS
365	198	1	100	3.9	12735	PASS
441	198	0.01	100	14.9	48331	PASS
442	442	50	100	100.0	310101	PASS
443	442	15	24	19.1	59205	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF080322\
 Data File : BF129541.D
 Acq On : 03 Aug 2022 15:31
 Operator : CG\JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Quant Time: Aug 03 17:44:49 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF072522.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Aug 02 01:11:25 2022
 Response via : Initial Calibration

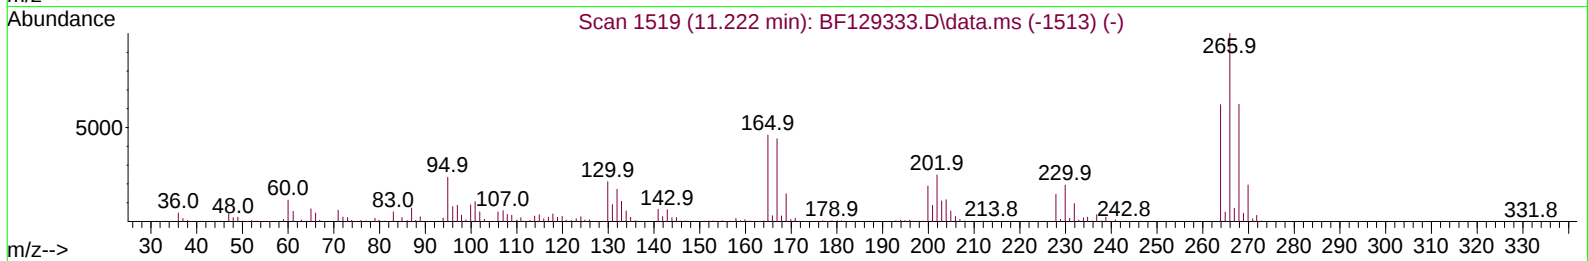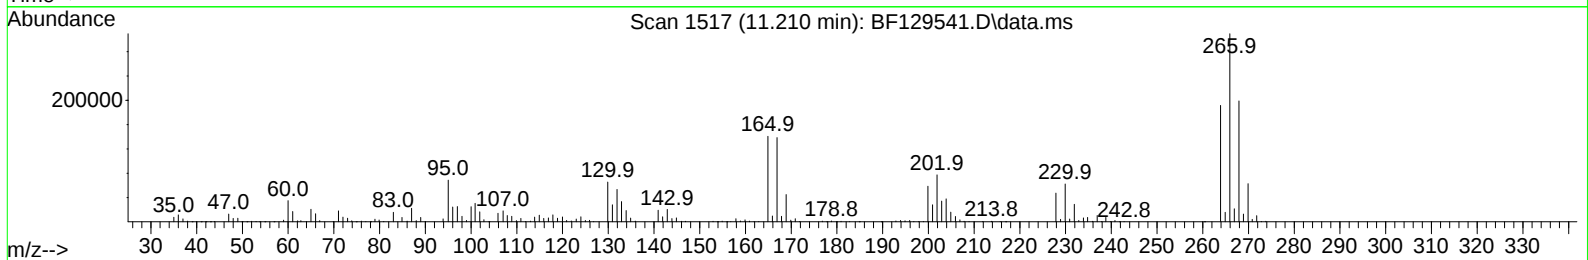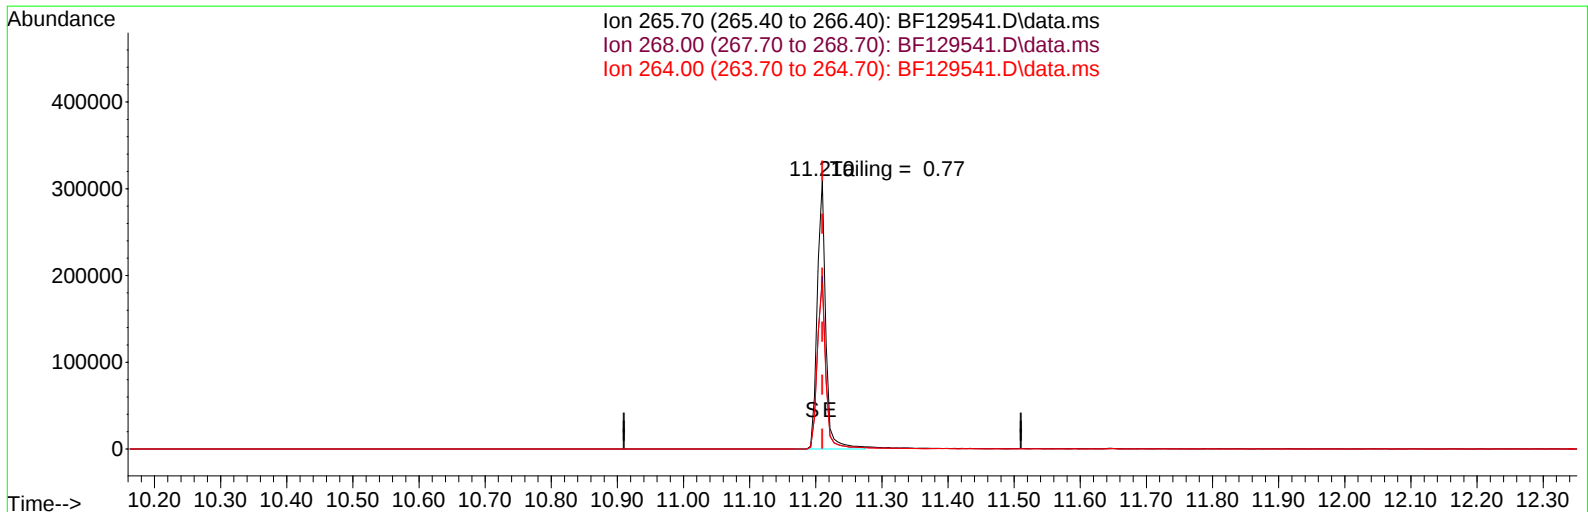

TIC: BF129541.D\data.ms

(70) Pentachlorophenol (C)

11.210min (-0.000) 114985.32 ng




response 283320

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.70	64.32
264.00	61.80	61.85
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF080322\
Data File : BF129541.D
Acq On : 03 Aug 2022 15:31
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Aug 03 17:44:49 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF072522.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Aug 02 01:11:25 2022
Response via : Initial Calibration

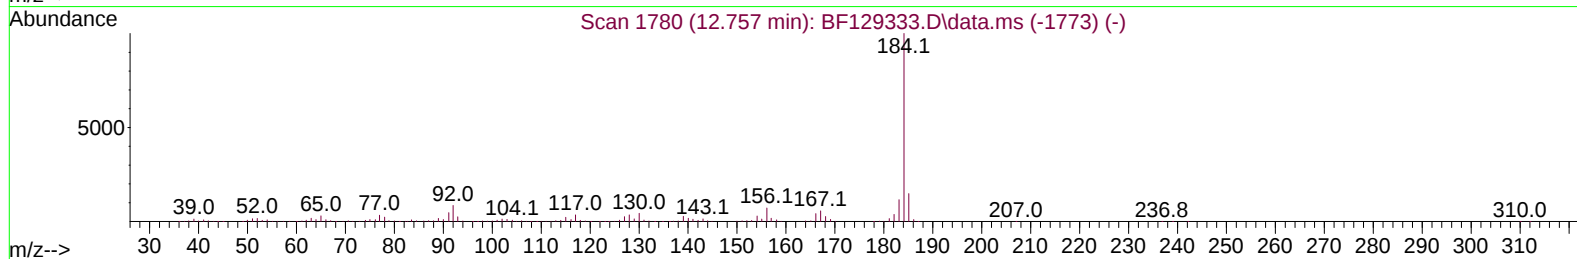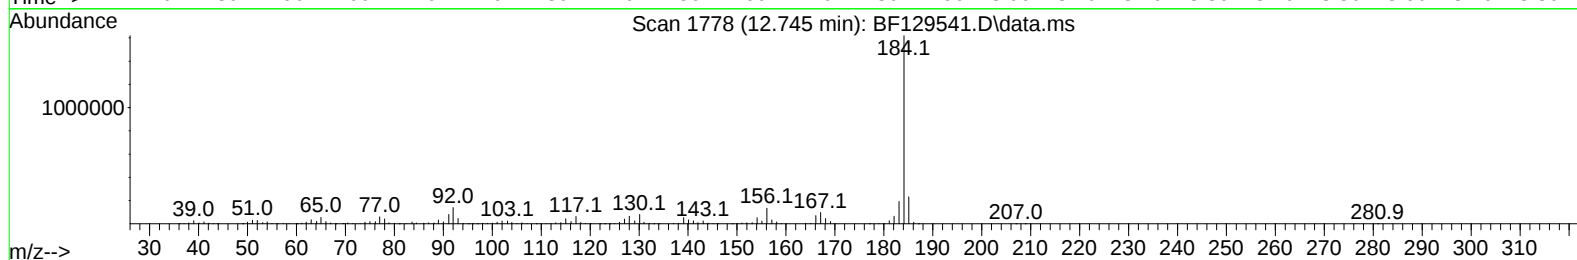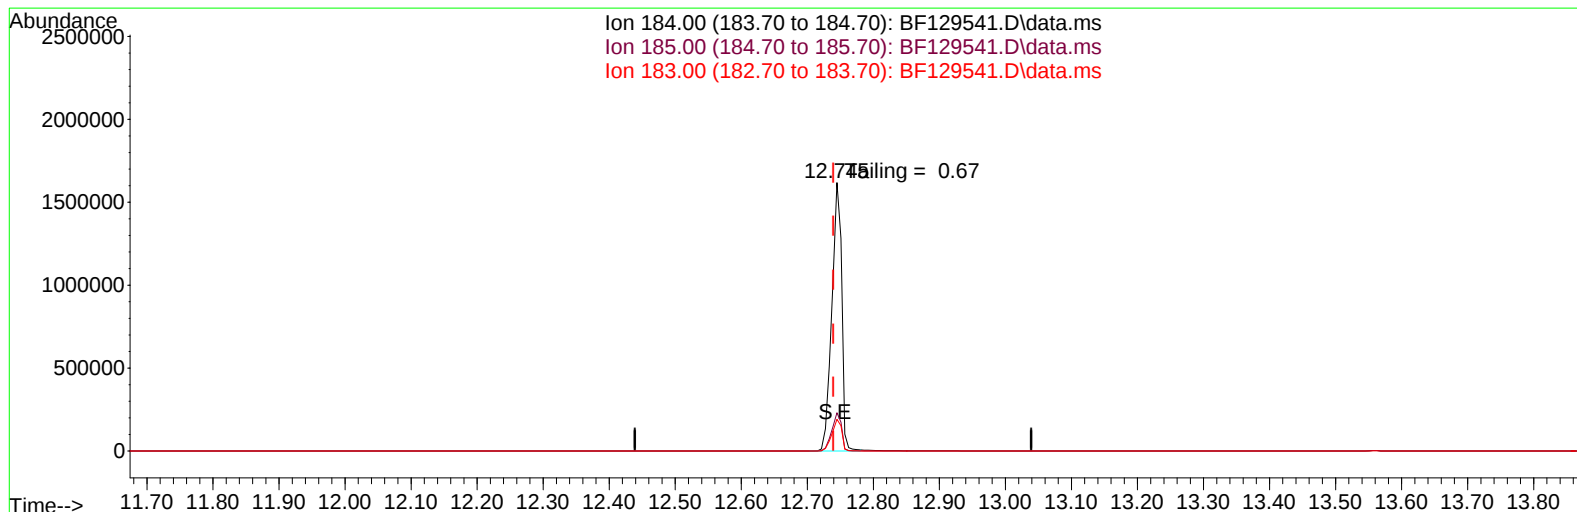

TIC: BF129541.D\data.ms

(77) Benzidine

12.745min (+ 0.006) 119110.70 ng

response 1691570

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.90	14.29
183.00	11.60	11.82
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
8/3/2022	BNA_F	<u>BF129541.D</u>
Compound Name	Response	Retention Time
DDT	840684	13.56
DDD	10400	13.26
DDE	2129	12.92
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
12529	853213	1.47

Instrument :
BNA_F
ClientSampleId :
DFTPP