
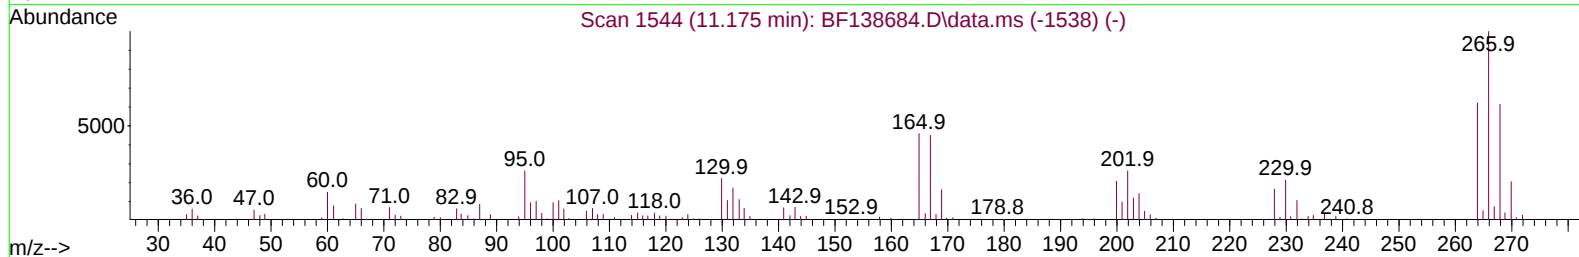
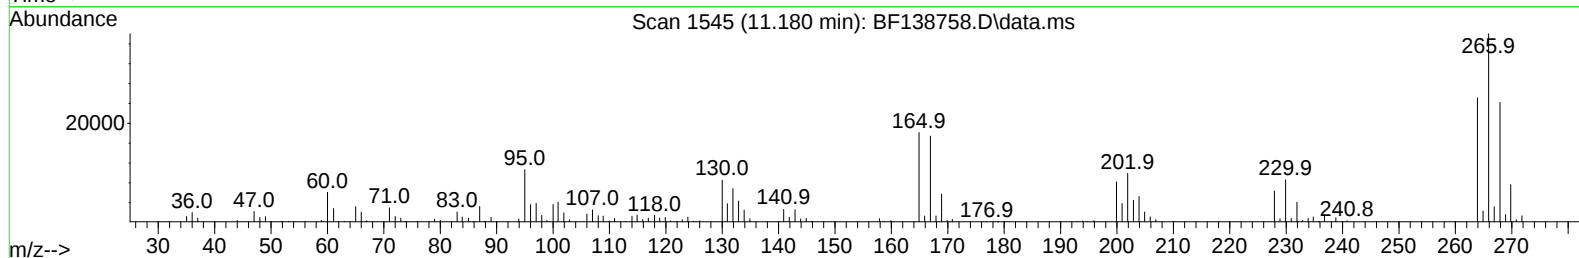


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF080324\
Data File : BF138758.D
Acq On : 03 Aug 2024 08:58
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Aug 05 00:35:51 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF073024.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Jul 30 17:50:01 2024
Response via : Initial Calibration

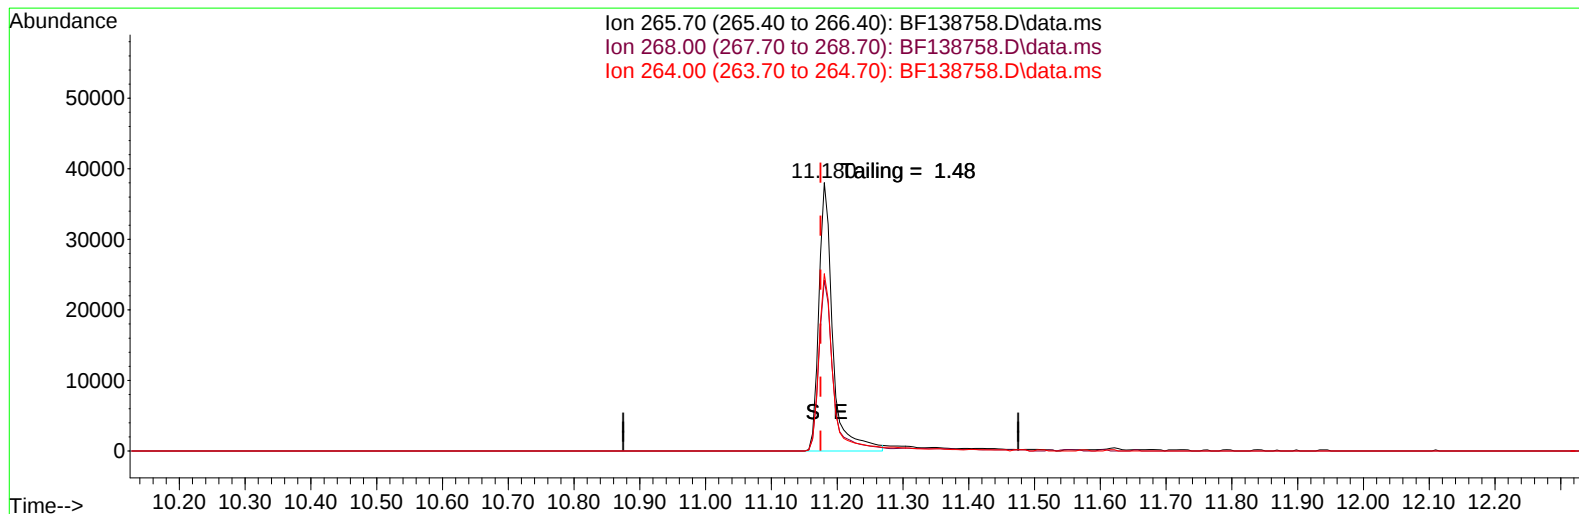

TIC: BF138758.D\data.ms

(70) Pentachlorophenol (C)




11.180min (+ 0.005) 28524.59 ng

response 58354

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	61.50	63.68
264.00	62.20	66.08
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF080324\
Data File : BF138758.D
Acq On : 03 Aug 2024 08:58
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Aug 05 00:35:51 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF073024.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Jul 30 17:50:01 2024
Response via : Initial Calibration

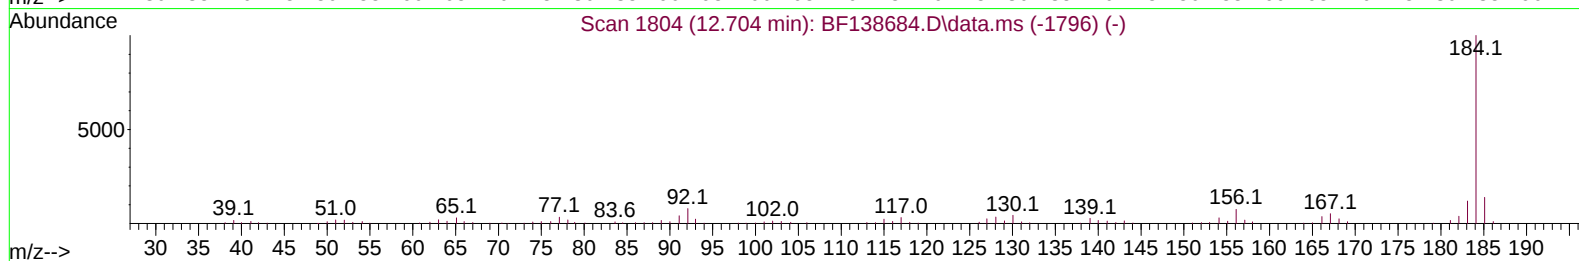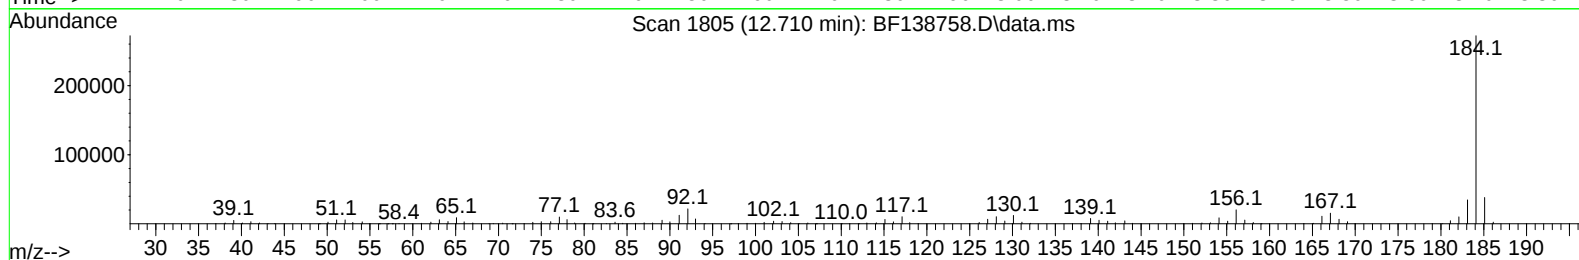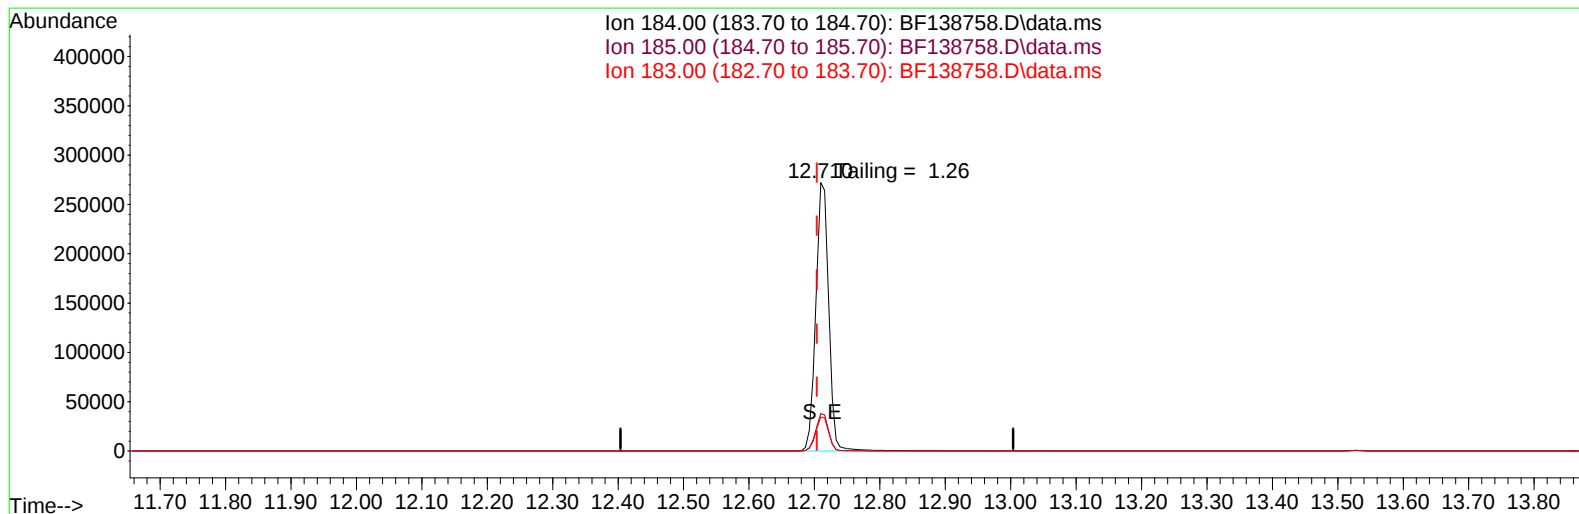

TIC: BF138758.D\data.ms

(77) Benzidine

12.710min (+ 0.006) 0.00 ng

response 375269

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	13.90	13.98
183.00	12.00	12.74
0.00	0.00	0.00