

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF080324\
 Data File : BF138762.D
 Acq On : 03 Aug 2024 11:02
 Operator : RC/JU
 Sample : P3379-03RX
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 OU4-PCS-02-072324RX

Quant Time: Aug 05 00:49:01 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF073024.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Jul 30 17:50:01 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	6.845	152	53746	20.000	ng	0.00
21) Naphthalene-d8	8.128	136	242226	20.000	ng	0.00
39) Acenaphthene-d10	9.880	164	143809	20.000	ng	0.00
64) Phenanthrene-d10	11.369	188	209060	20.000	ng	0.00
76) Chrysene-d12	14.010	240	126686	20.000	ng	0.00
86) Perylene-d12	15.480	264	130904	20.000	ng	0.01
System Monitoring Compounds						
5) 2-Fluorophenol	5.487	112	431008	123.791	ng	0.02
7) Phenol-d6	6.492	99	603774	129.161	ng	0.00
23) Nitrobenzene-d5	7.410	82	418614	84.494	ng	0.00
42) 2,4,6-Tribromophenol	10.674	330	167014	141.779	ng	0.00
45) 2-Fluorobiphenyl	9.204	172	788398	82.371	ng	0.00
79) Terphenyl-d14	12.957	244	727767	96.181	ng	0.01


Target Compounds	Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF080324\
Data File : BF138762.D
Acq On : 03 Aug 2024 11:02
Operator : RC/JU
Sample : P3379-03RX
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
OU4-PCS-02-072324RX


Quant Time: Aug 05 00:49:01 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF073024.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Jul 30 17:50:01 2024
Response via : Initial Calibration

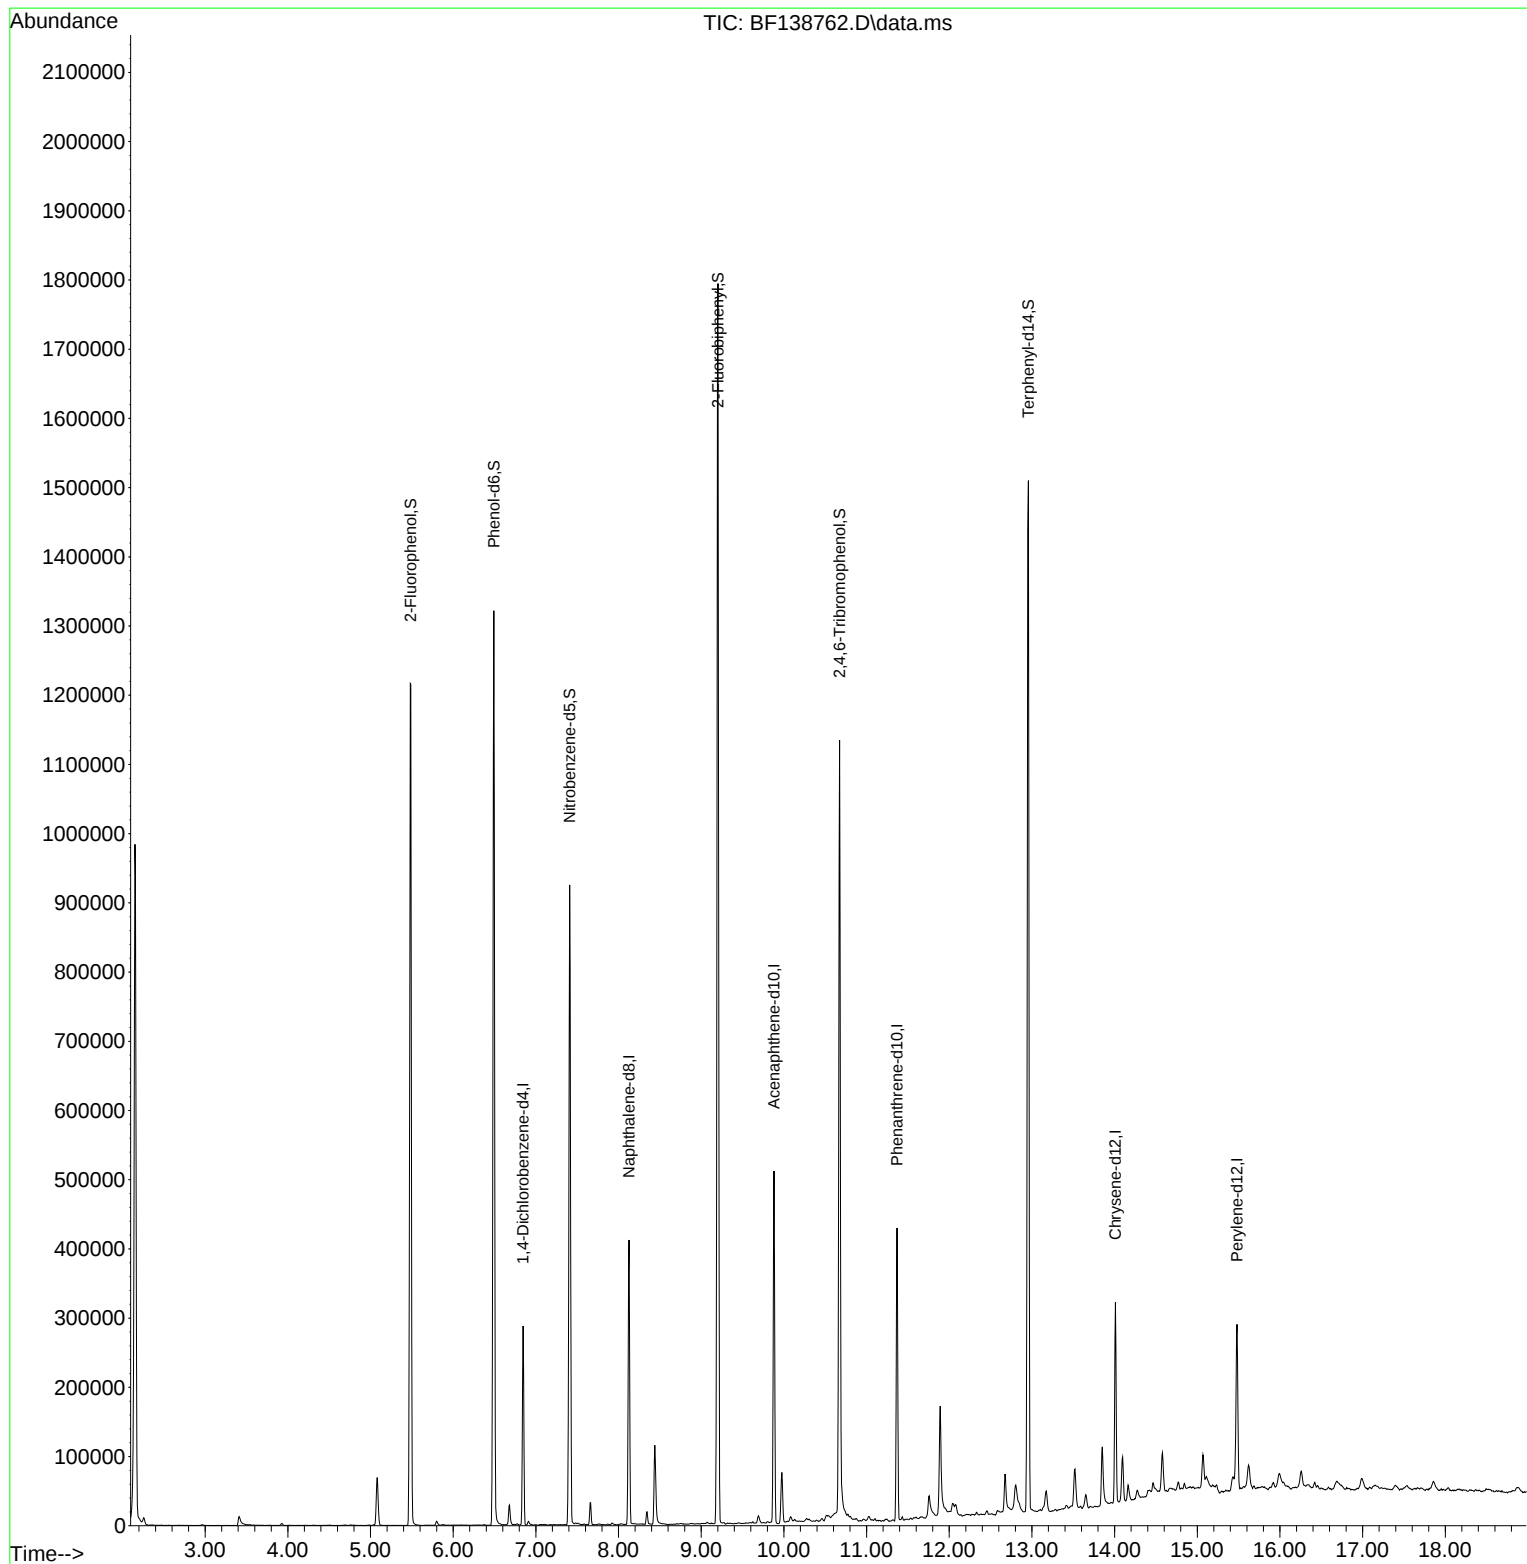



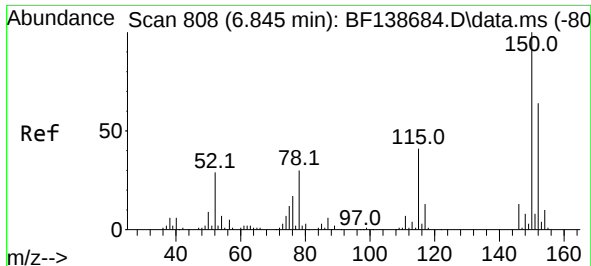


#1
1,4-Dichlorobenzene-d4
Concen: 20.000 ng
RT: 6.845 min Scan# 808
Delta R.T. 0.000 min
Lab File: BF138762.D
Acq: 03 Aug 2024 11:02


Instrument :
BNA_F
ClientSampleId :
OU4-PCS-02-072324RX

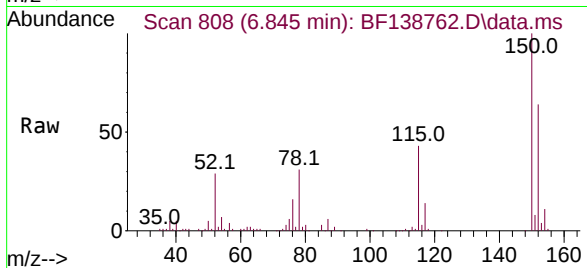



Tgt Ion:152 Resp: 53746
Ion Ratio Lower Upper
152 100
150 157.5 126.0 189.0
115 68.2 51.7 77.5

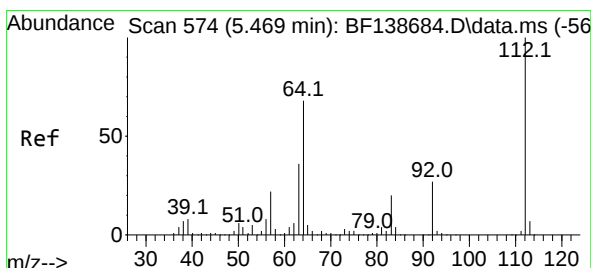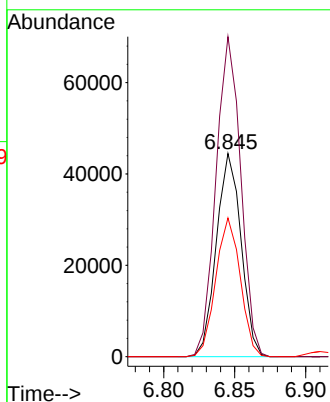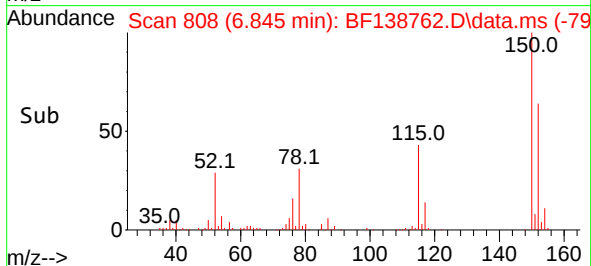

#5
2-Fluorophenol
Concen: 123.791 ng
RT: 5.487 min Scan# 577
Delta R.T. 0.018 min
Lab File: BF138762.D
Acq: 03 Aug 2024 11:02

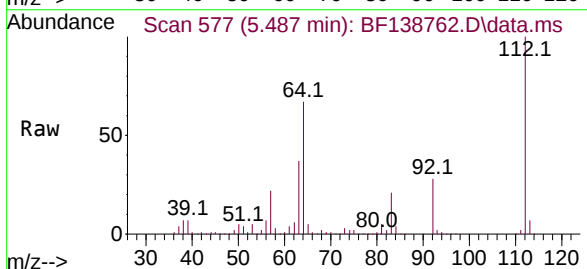

Tgt Ion:112 Resp: 431008
Ion Ratio Lower Upper
112 100
64 66.9 54.2 81.4
63 36.6 28.7 43.1



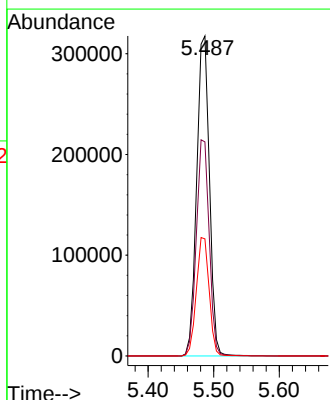
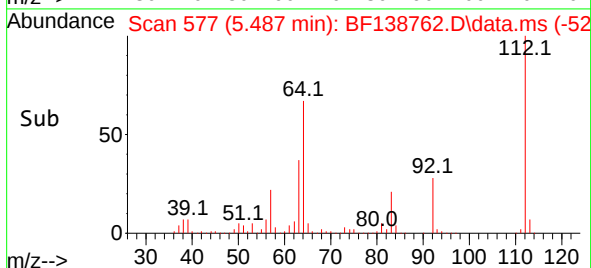




#7
Phenol-d6
Concen: 129.161 ng
RT: 6.492 min Scan# 74
Delta R.T. 0.006 min
Lab File: BF138762.D
Acq: 03 Aug 2024 11:02




Instrument :
BNA_F
ClientSampleId :
OU4-PCS-02-072324RX


Tgt Ion: 99 Resp: 603774
Ion Ratio Lower Upper
99 100
42 21.9 17.4 26.0
71 36.9 28.1 42.1

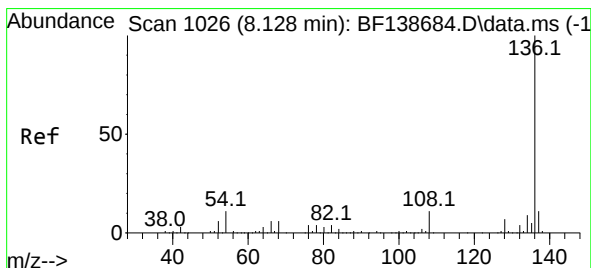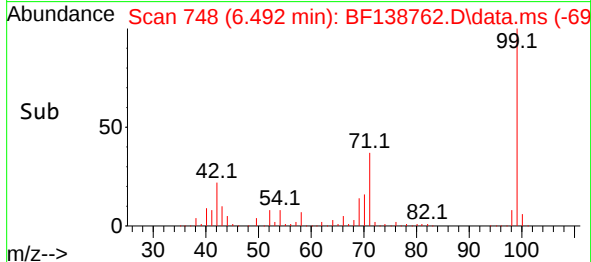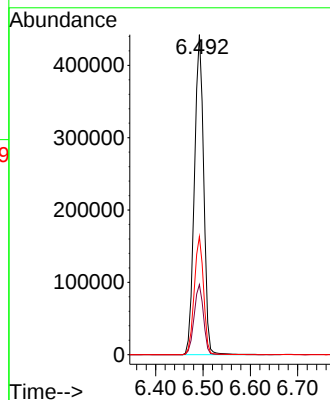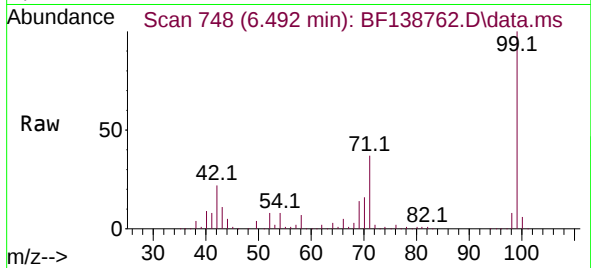

#21
Naphthalene-d8
Concen: 20.000 ng
RT: 8.128 min Scan# 1026
Delta R.T. -0.000 min
Lab File: BF138762.D
Acq: 03 Aug 2024 11:02

Tgt Ion: 136 Resp: 242226
Ion Ratio Lower Upper
136 100
137 10.8 8.9 13.3
54 9.5 8.6 12.8
68 5.6 4.8 7.2


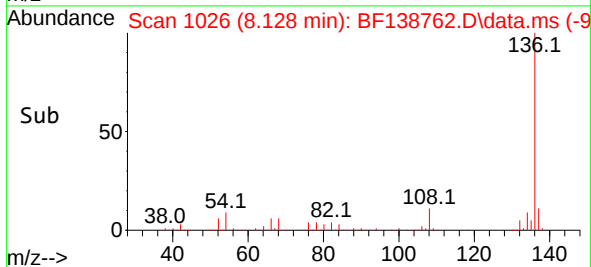
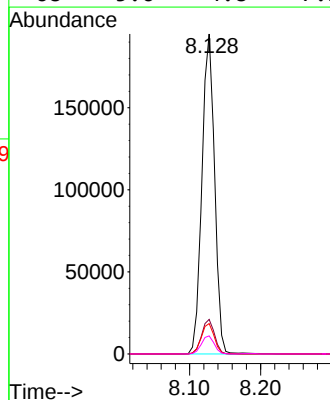
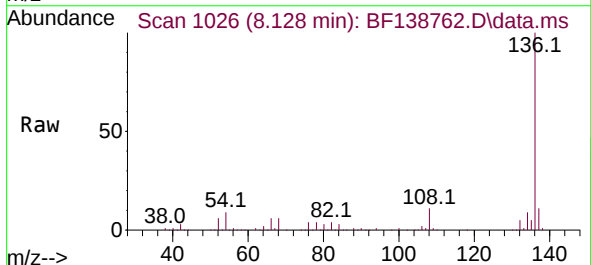


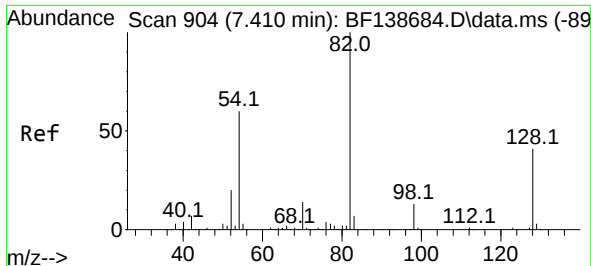

#23
Nitrobenzene-d5
Concen: 84.494 ng
RT: 7.410 min Scan# 904
Delta R.T. -0.000 min
Lab File: BF138762.D
Acq: 03 Aug 2024 11:02




Instrument :
BNA_F
ClientSampleId :
OU4-PCS-02-072324RX


Tgt Ion: 82 Resp: 418614
Ion Ratio Lower Upper
82 100
128 41.4 32.8 49.2
54 58.6 48.3 72.5

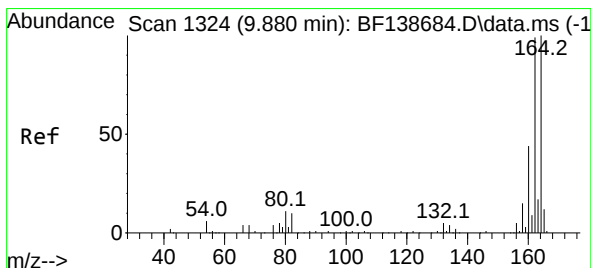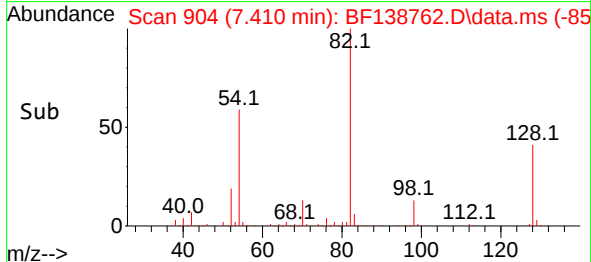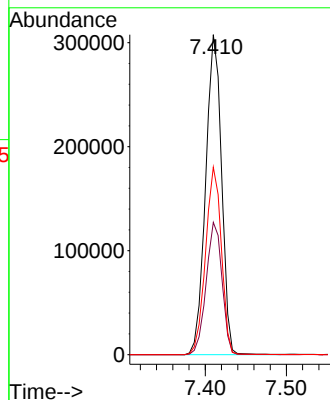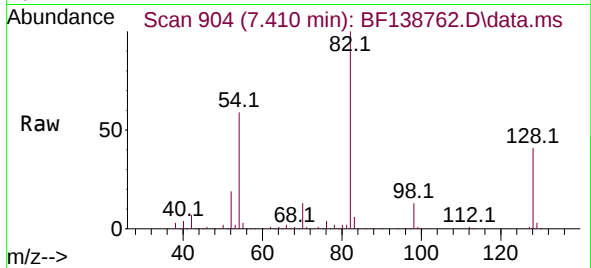

#39
Acenaphthene-d10
Concen: 20.000 ng
RT: 9.880 min Scan# 1324
Delta R.T. 0.000 min
Lab File: BF138762.D
Acq: 03 Aug 2024 11:02

Tgt Ion:164 Resp: 143809
Ion Ratio Lower Upper
164 100
162 101.8 79.4 119.0
160 44.0 35.1 52.7

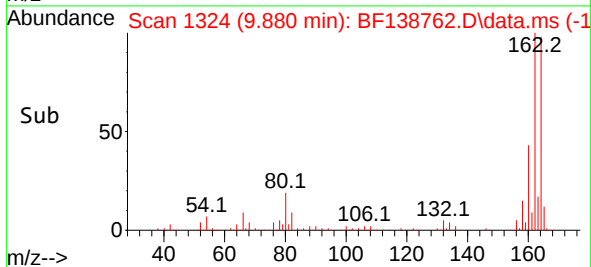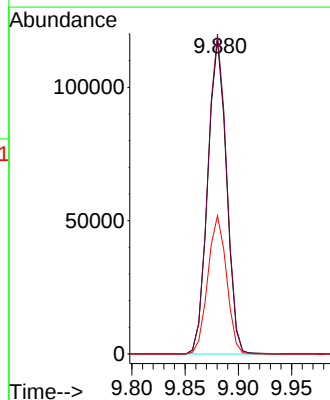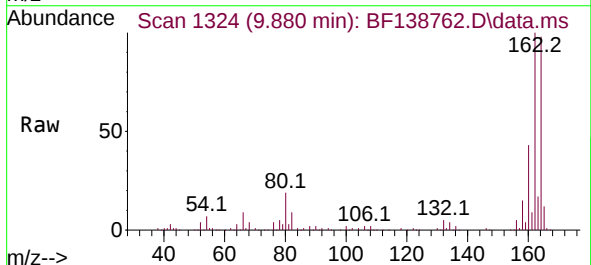

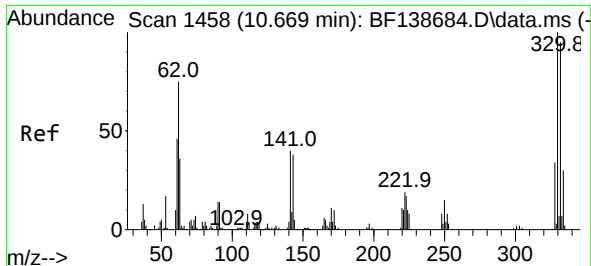

#42

2,4,6-Tribromophenol

Concen: 141.779 ng

RT: 10.674 min Scan# 1458

Delta R.T. 0.006 min

Lab File: BF138762.D


Acq: 03 Aug 2024 11:02

Instrument :

BNA_F

ClientSampleId :

OU4-PCS-02-072324RX

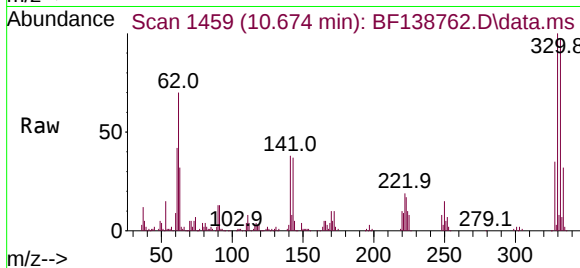




Tgt Ion:330 Resp: 167014

Ion Ratio Lower Upper

330 100

332 96.5 76.4 114.6

141 38.6 31.1 46.7

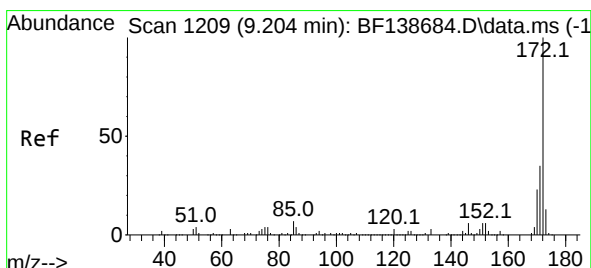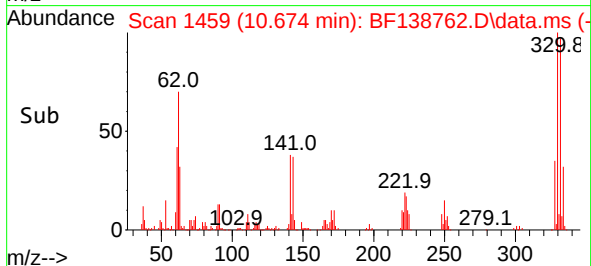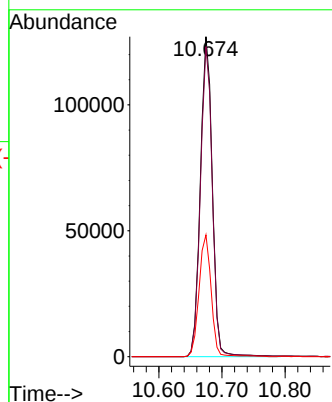

#45

2-Fluorobiphenyl

Concen: 82.371 ng

RT: 9.204 min Scan# 1209

Delta R.T. -0.000 min

Lab File: BF138762.D

Acq: 03 Aug 2024 11:02




Tgt Ion:172 Resp: 788398


Ion Ratio Lower Upper

172 100

171 36.0 28.3 42.5

170 23.5 18.8 28.2

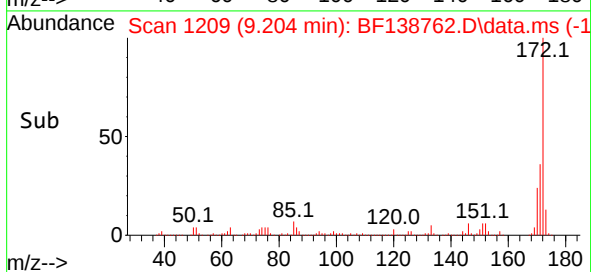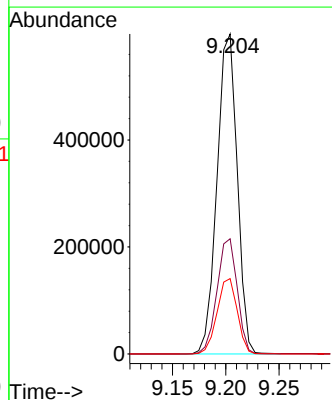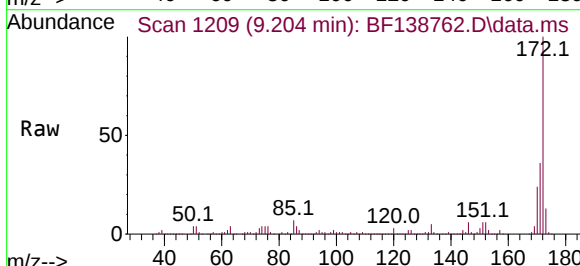

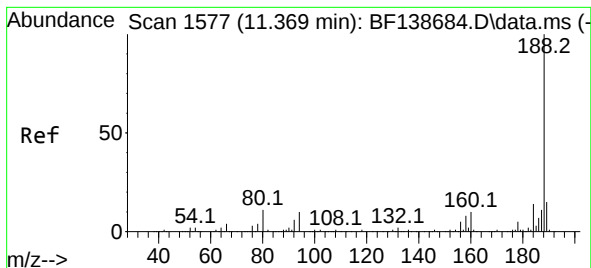

#64

Phenanthrene-d10

Concen: 20.000 ng

RT: 11.369 min Scan# 1

Delta R.T. -0.000 min

Lab File: BF138762.D

Acq: 03 Aug 2024 11:02

Instrument :

BNA_F

ClientSampleId :

OU4-PCS-02-072324RX





Tgt Ion:188 Resp: 209060

Ion Ratio Lower Upper

188 100

94 9.4 7.6 11.4

80 9.9 8.6 12.8

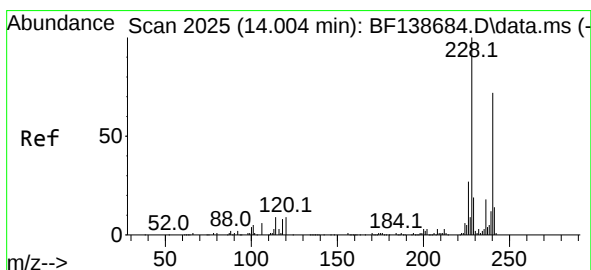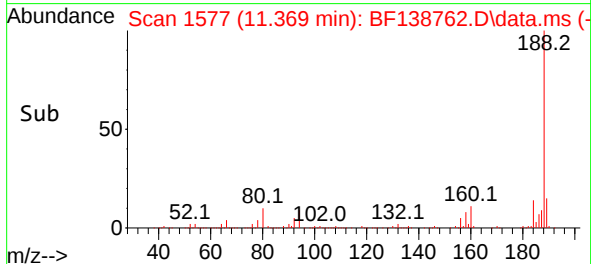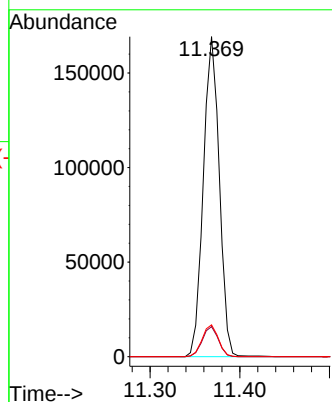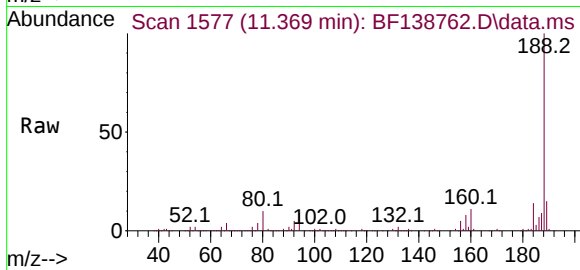

#76

Chrysene-d12

Concen: 20.000 ng

RT: 14.010 min Scan# 2026

Delta R.T. 0.006 min

Lab File: BF138762.D

Acq: 03 Aug 2024 11:02




Tgt Ion:240 Resp: 126686


Ion Ratio Lower Upper

240 100

120 11.8 10.2 15.4


236 25.6 19.8 29.8

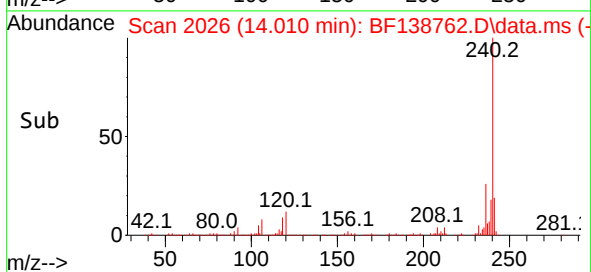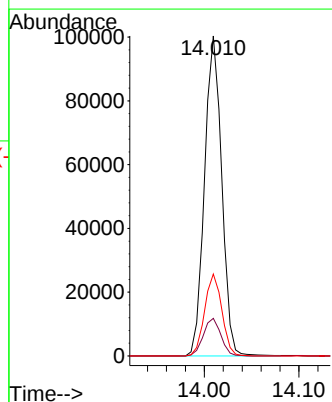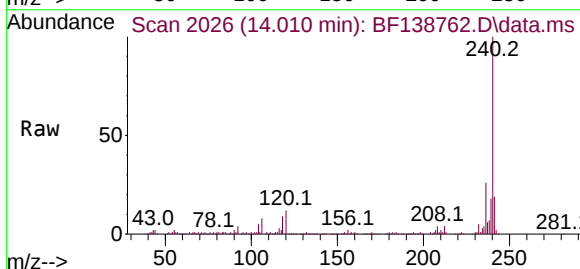



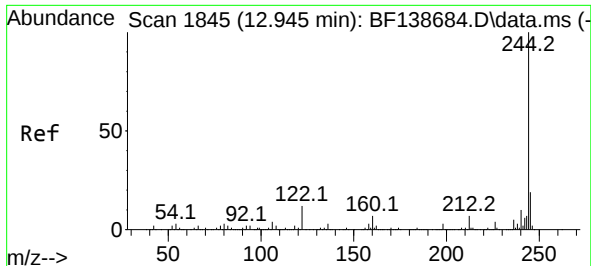


#79
Terphenyl-d14
Concen: 96.181 ng
RT: 12.957 min Scan# 11
Delta R.T. 0.012 min
Lab File: BF138762.D
Acq: 03 Aug 2024 11:02

Instrument :
BNA_F
ClientSampleId :
OU4-PCS-02-072324RX

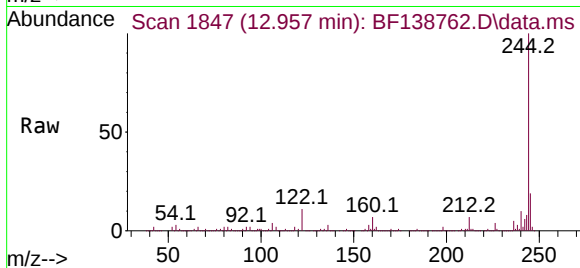

Tgt Ion:244 Resp: 727767
Ion Ratio Lower Upper
244 100
212 6.6 5.4 8.2
122 11.1 9.6 14.4

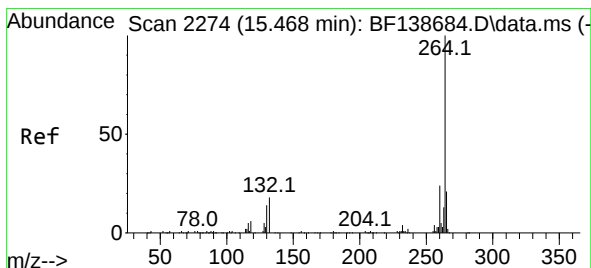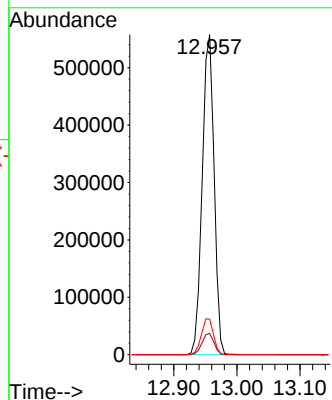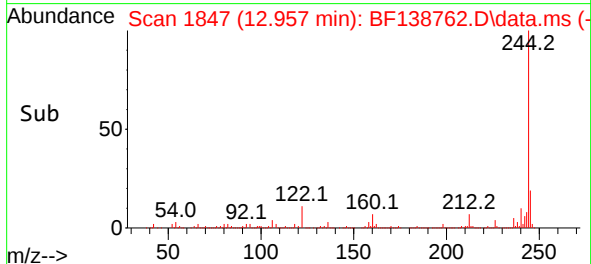

#86
Perylene-d12
Concen: 20.000 ng
RT: 15.480 min Scan# 2276
Delta R.T. 0.012 min
Lab File: BF138762.D
Acq: 03 Aug 2024 11:02

Tgt Ion:264 Resp: 130904
Ion Ratio Lower Upper
264 100
260 23.0 19.0 28.6
265 21.1 17.0 25.6

