


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF080324\
Data File : BF138758.D
Acq On : 03 Aug 2024 08:58
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF073024.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Tue Jul 30 17:50:01 2024

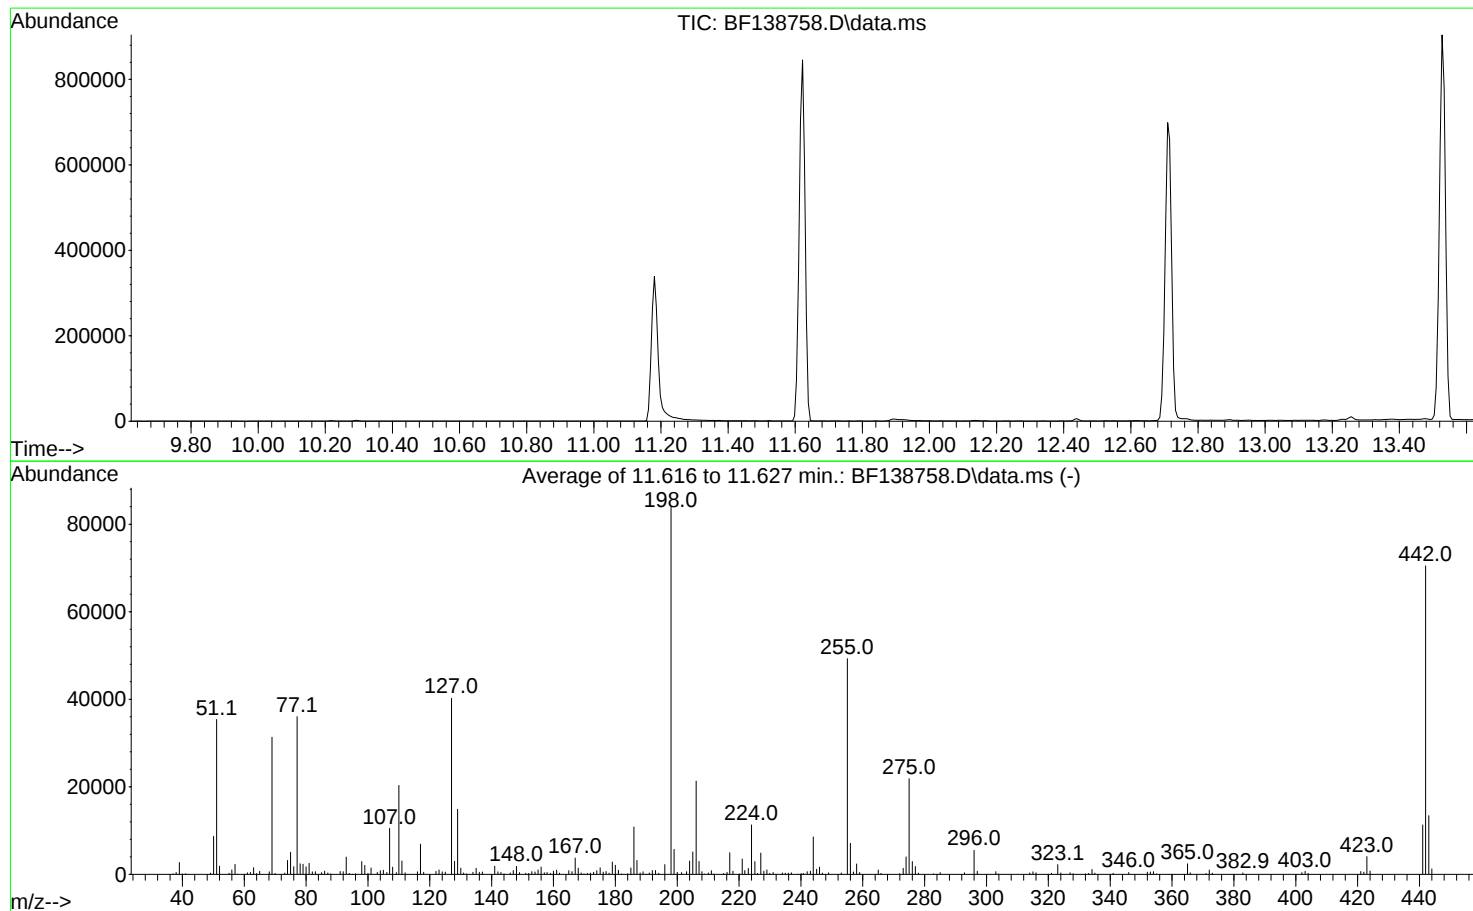

AutoFind: Scans 1619, 1620, 1621; Background Corrected with Scan 1613

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	42.1	35387	PASS
68	69	0.00	2	1.9	589	PASS
69	198	0.00	100	37.3	31320	PASS
70	69	0.00	2	0.7	213	PASS
127	198	10	80	47.9	40224	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	84043	PASS
199	198	5	9	6.8	5696	PASS
275	198	10	60	26.0	21875	PASS
365	198	1	100	2.9	2396	PASS
441	198	0.01	100	13.4	11285	PASS
442	442	50	100	100.0	70499	PASS
443	442	15	24	19.0	13421	PASS

DDT Breakdown




Date	Instrument Name	DFTPP Data File
8/3/2024	BNA_F	<u>BF138758.D</u>
Compound Name	Response	Retention Time
DDT	219603	13.527
DDD	4051	13.257
DDE	796	12.892
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
4847	224450	2.16

Instrument :
BNA_F
ClientSampleId :
DFTPP

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF080324\
Data File : BF138758.D
Acq On : 03 Aug 2024 08:58
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Aug 05 00:35:51 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF073024.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Jul 30 17:50:01 2024
Response via : Initial Calibration

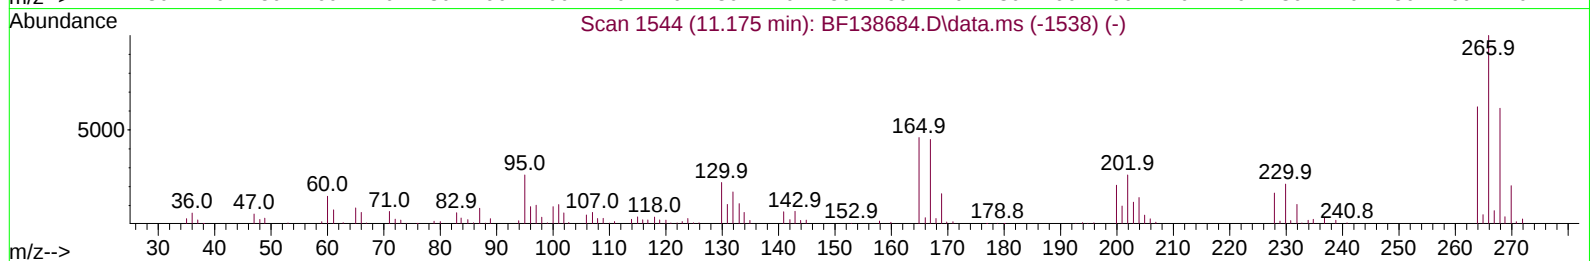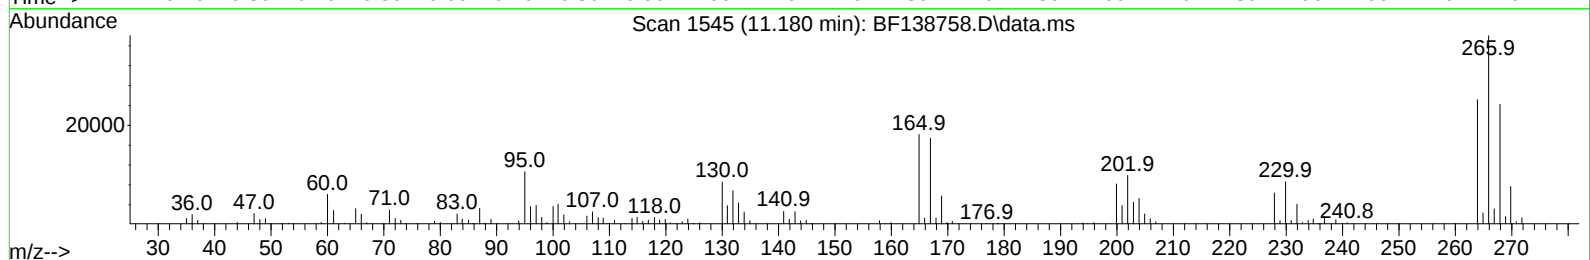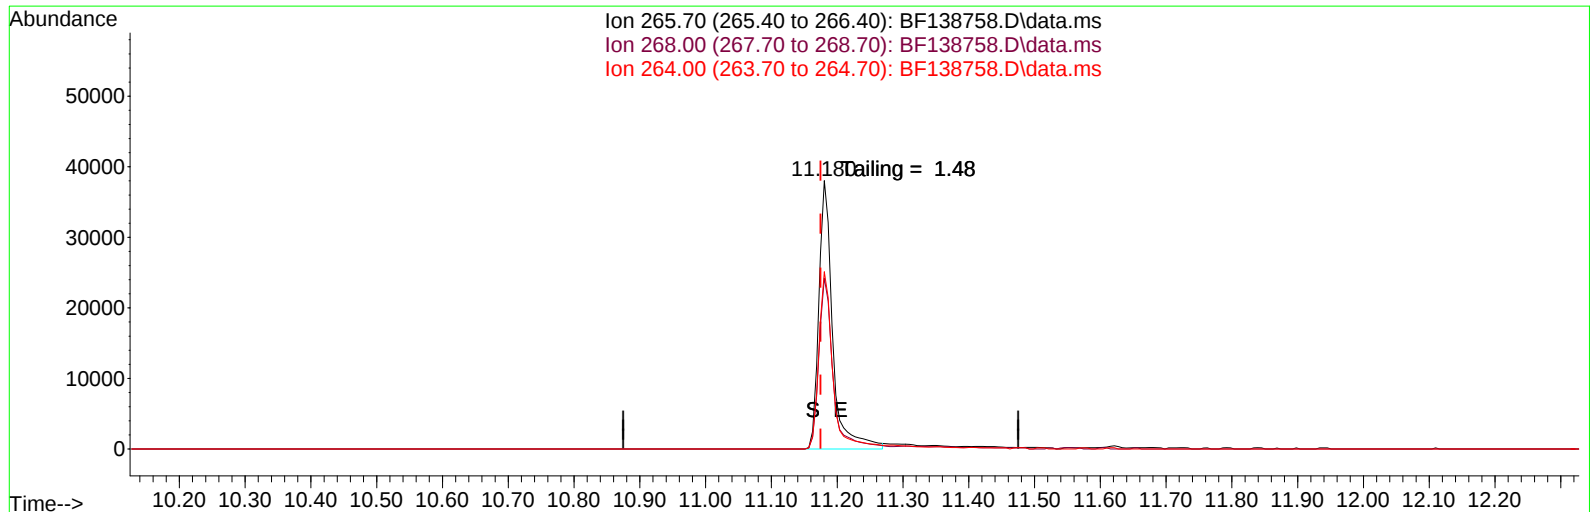

TIC: BF138758.D\data.ms

(70) Pentachlorophenol (C)

11.180min (+ 0.005) 28524.59 ng




response 58354

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	61.50	63.68
264.00	62.20	66.08
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF080324\
Data File : BF138758.D
Acq On : 03 Aug 2024 08:58
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Aug 05 00:35:51 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF073024.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Jul 30 17:50:01 2024
Response via : Initial Calibration

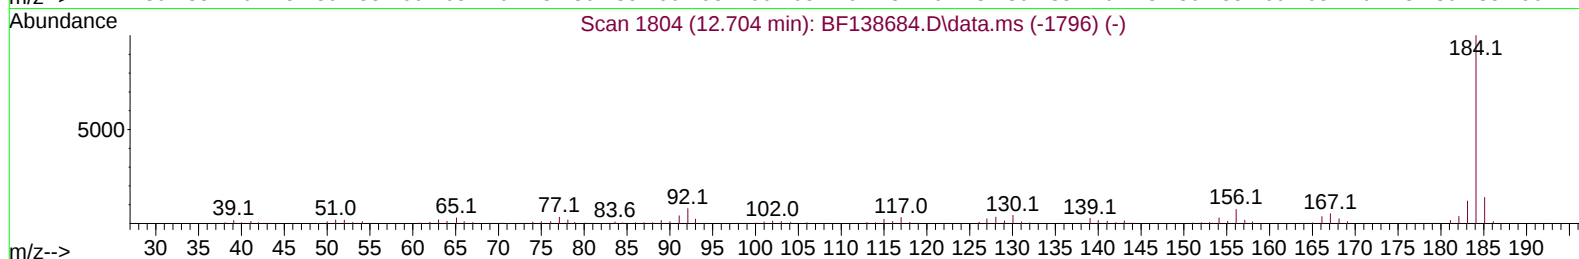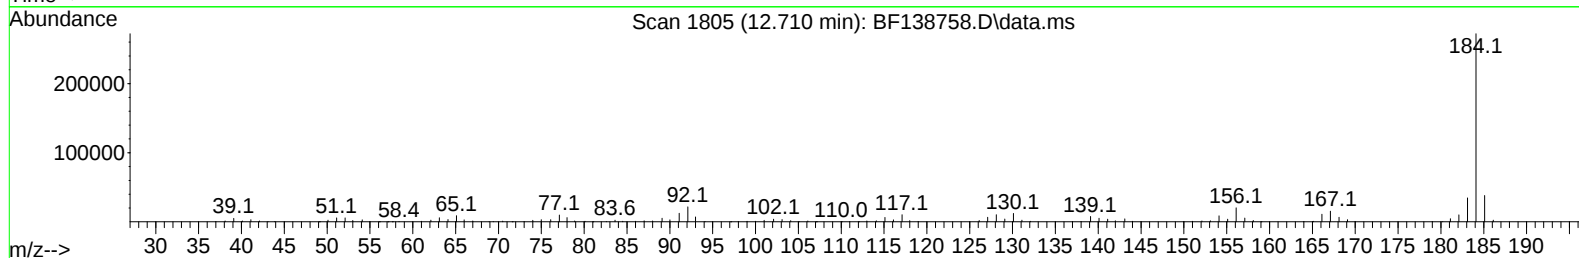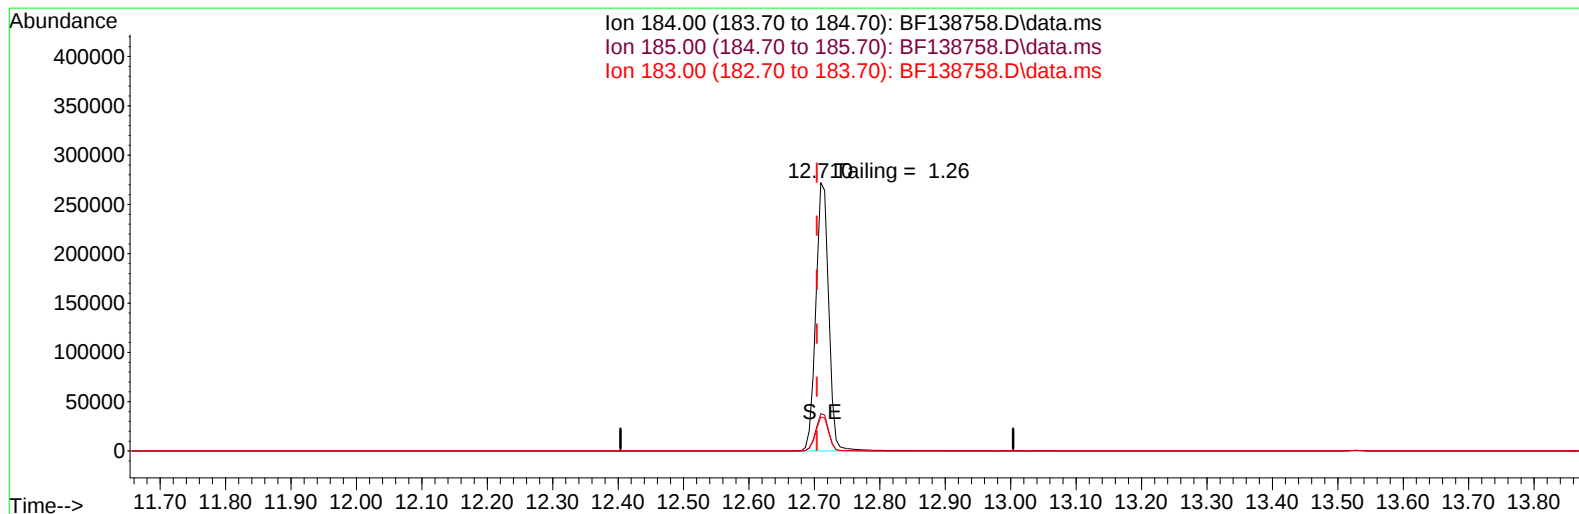

TIC: BF138758.D\data.ms

(77) Benzidine

12.710min (+ 0.006) 0.00 ng

response 375269

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	13.90	13.98
183.00	12.00	12.74
0.00	0.00	0.00