

Data Path : C:\DOCUMENTS AND SETTINGS\AYUL\DESKTOP\BF051415\
 Data File : BF079236.D
 Acq On : 14 May 2015 16:17
 Operator : TP/IZ
 Sample : SSTDCCC040
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 SSTDCCC040

Quant Time: Aug 05 04:07:33 2015
 Quant Method : C:\DOCUMENTS AND SETTINGS\AYUL\DESKTOP\BF051415\8270-BF043015.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed May 20 05:08:22 2015
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	0.00	152	0	0.00	ng	-7.13
21) Naphthalene-d8	0.00	136	0	0.00	ng	-8.71
38) Acenaphthene-d10	0.00	164	0	0.00	ng	-10.88
63) Phenanthrene-d10	0.00	188	0	0.00	ng	-12.72
75) Chrysene-d12	0.00	240	0	0.00	ng	-16.02
86) Perylene-d12	0.00	264	0	0.00	ng	-17.82
System Monitoring Compounds						
5) 2-Fluorophenol	0.00	112	0	0.00	ng	
7) Phenol-d6	0.00	99	0	0.00	ng	
23) Nitrobenzene-d5	7.84	82	14038	0.00	ng	0.01
41) 2,4,6-Tribromophenol	0.00	330	0	0.00	ng	
44) 2-Fluorobiphenyl	0.00	172	0	0.00	ng	
78) Terphenyl-d14	0.00	244	0	0.00	ng	


Target Compounds Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : C:\DOCUMENTS AND SETTINGS\AYUL\DESKTOP\BF051415\
Data File : BF079236.D
Acq On : 14 May 2015 16:17
Operator : TP/IZ
Sample : SSTDCCC040
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
SSTDCCC040

Quant Time: Aug 05 04:07:33 2015
Quant Method : C:\DOCUMENTS AND SETTINGS\AYUL\DESKTOP\BF051415\8270-BF043015.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed May 20 05:08:22 2015
Response via : Initial Calibration


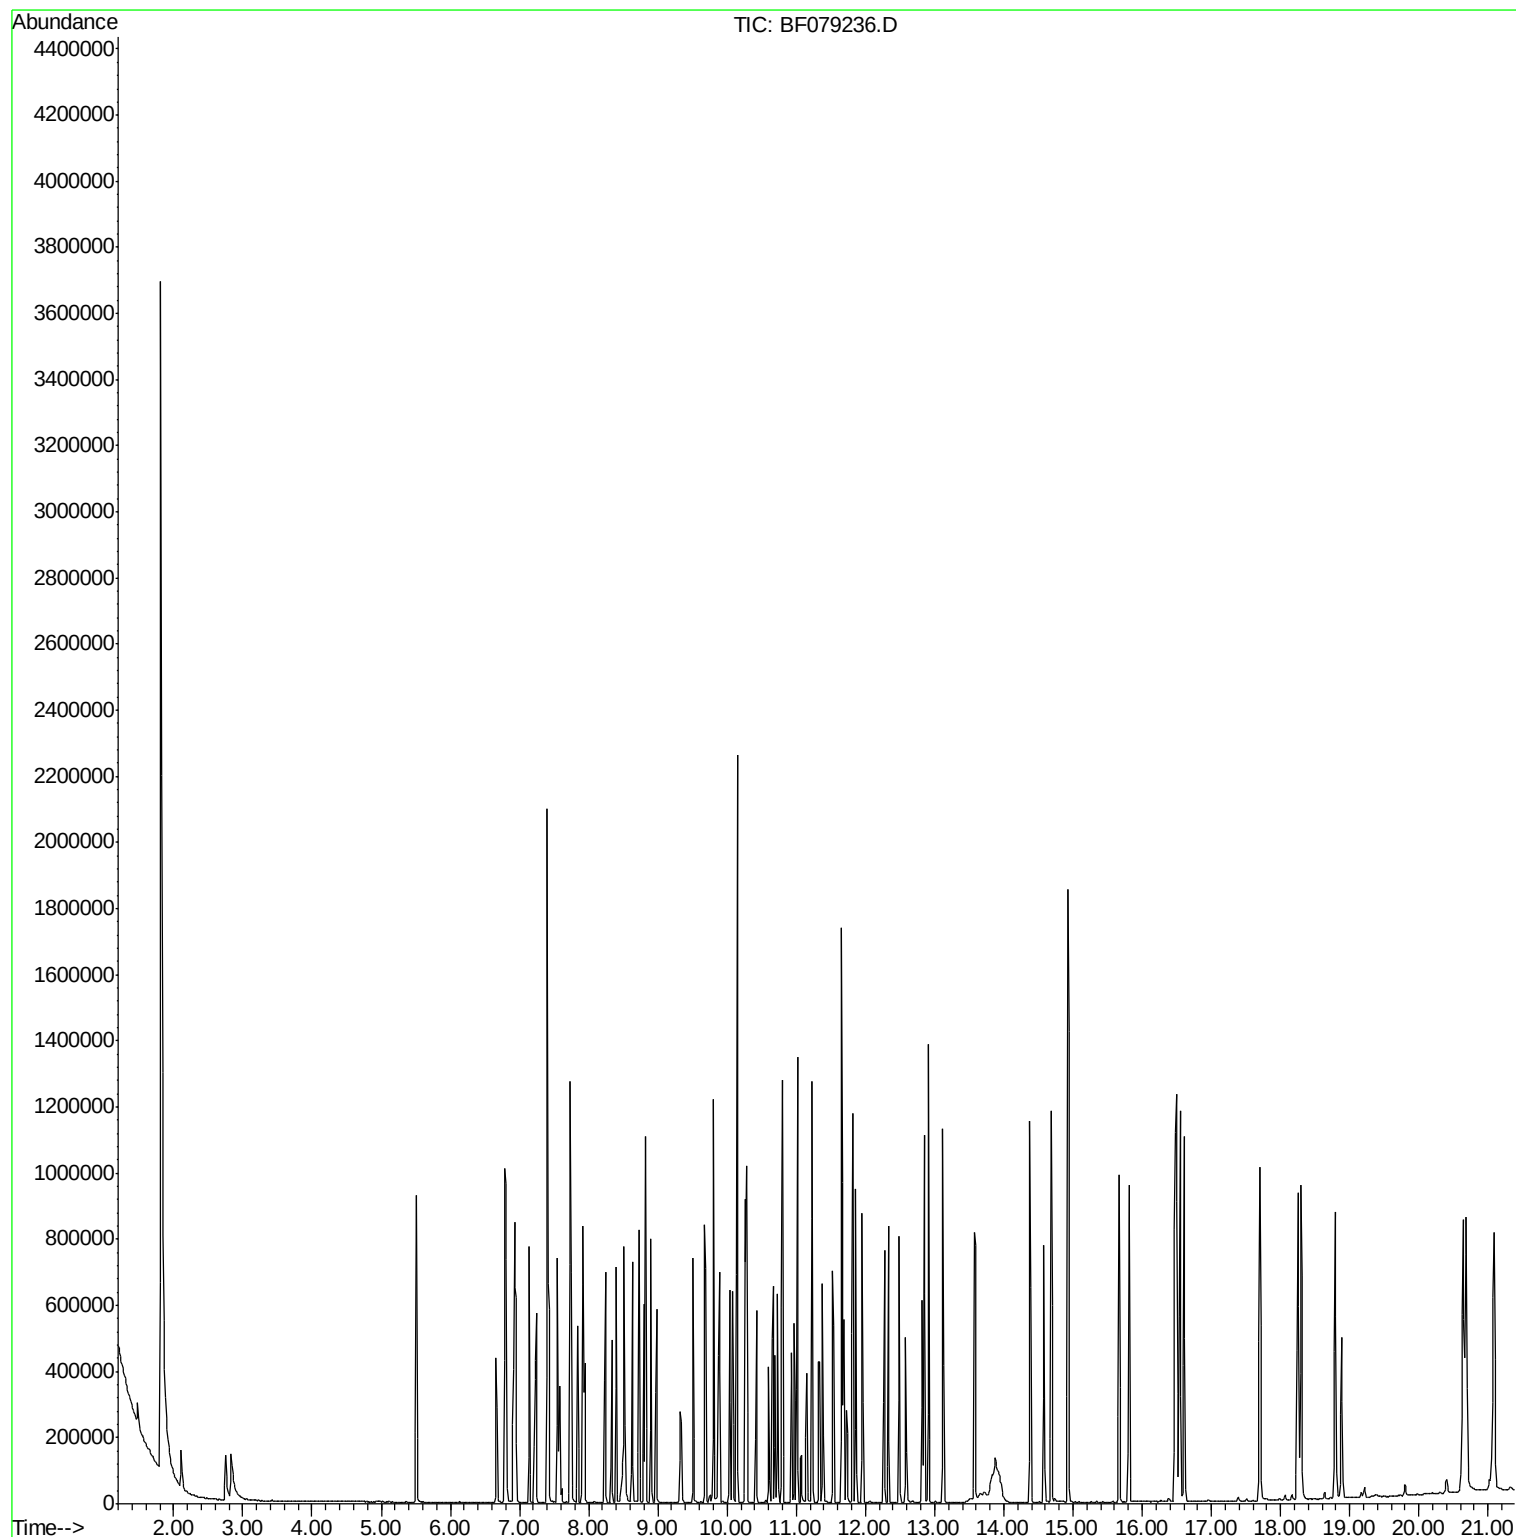


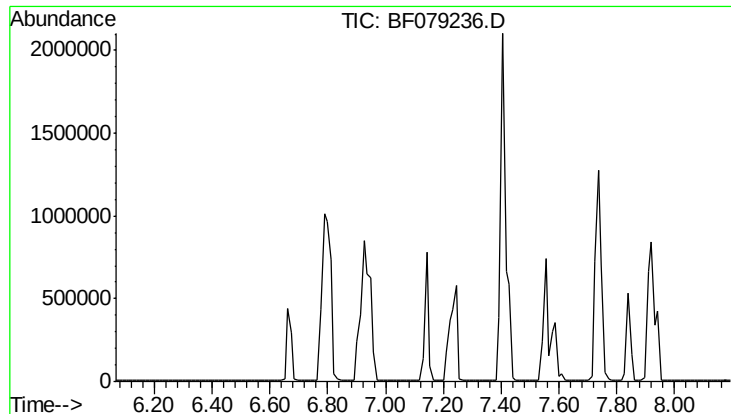

#1
 1,4-Dichlorobenzene-d4
 Concen: 0.00 ng
 Expected RT: 7.13 min
 Lab File: BF079236.D
 Acq: 14 May 2015 16:17


Instrument :
 BNA_F
 ClientSampleId :
 SSTDCCC040


Tot Ion	152
Sig	Exp Ratio
152	100
150	154.8
115	61.7

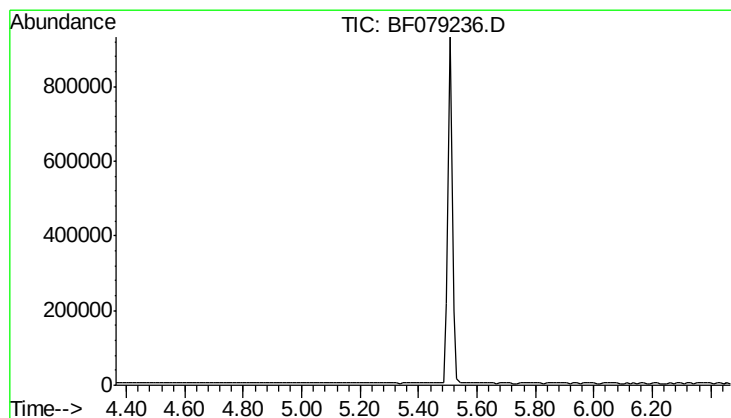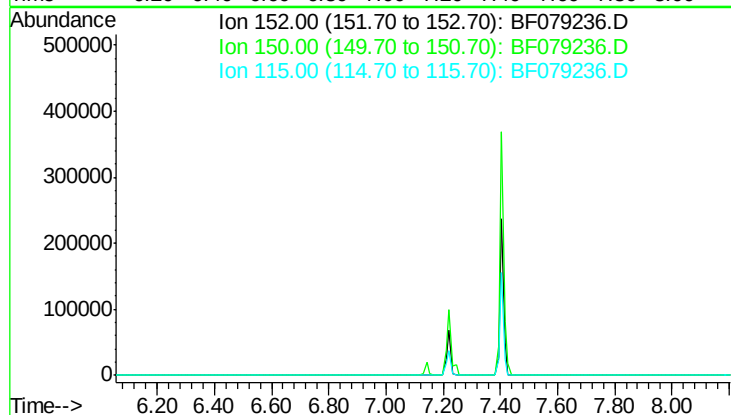

#5
 2-Fluorophenol
 Concen: 0.00 ng
 Expected RT: 5.42 min
 Lab File: BF079236.D
 Acq: 14 May 2015 16:17

Tgt Ion	112
Sig	Exp Ratio
112	100
64	55.2
63	28.4

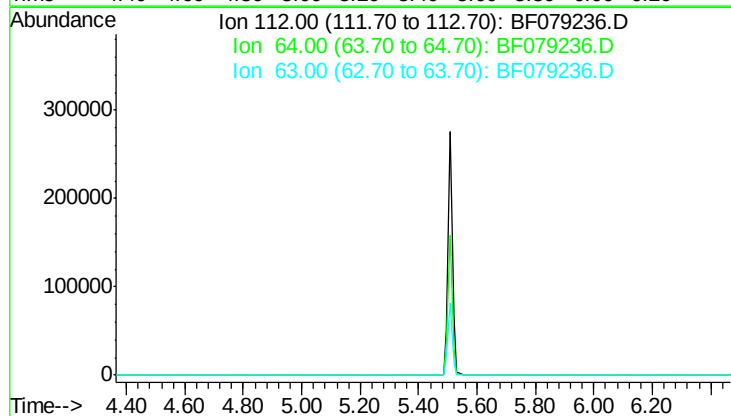

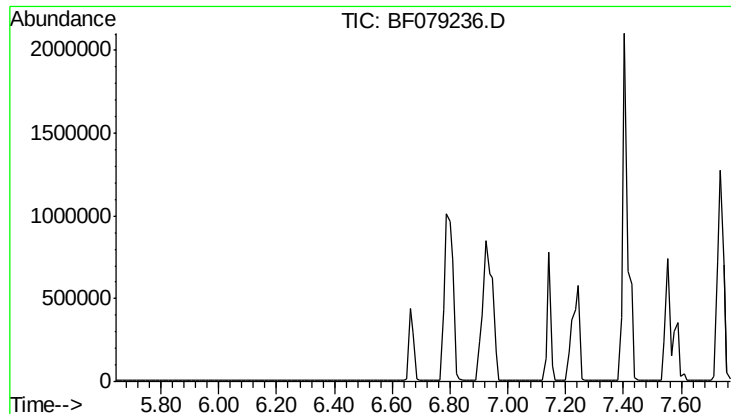

#7

Phenol-d6

Concen: 0.00 ng

Expected RT: 6.71 min

Lab File: BF079236.D

Acq: 14 May 2015 16:17

Instrument :

BNA_F

ClientSampleId :

SSTDCCC040



Tot Ion: 99

Sig Exp Ratio

99 100

42 21.4

71 32.9

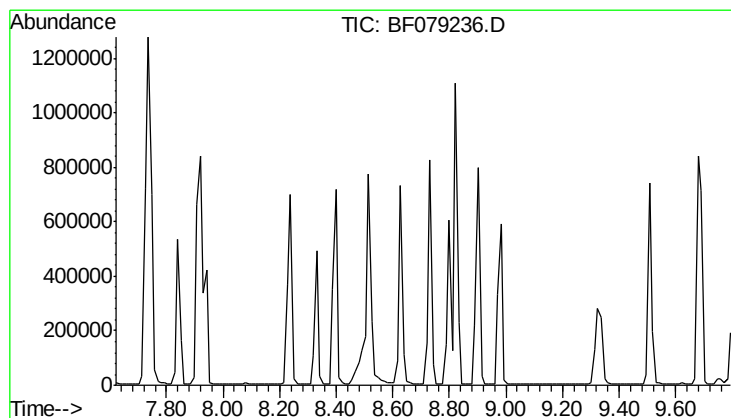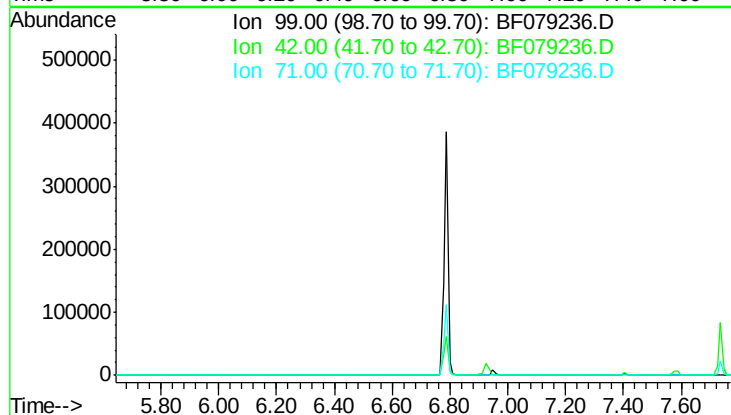

#21

Naphthalene-d8

Concen: 0.00 ng

Expected RT: 8.71 min

Lab File: BF079236.D

Acq: 14 May 2015 16:17

Tgt Ion: 136


Sig Exp Ratio


136 100

137 11.0

54 8.6

68 6.1

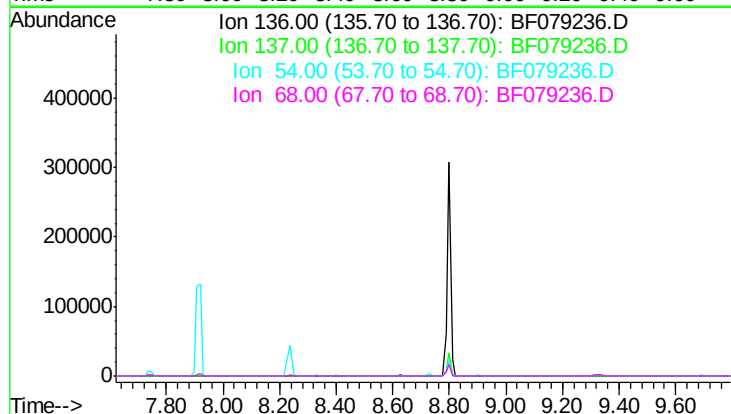


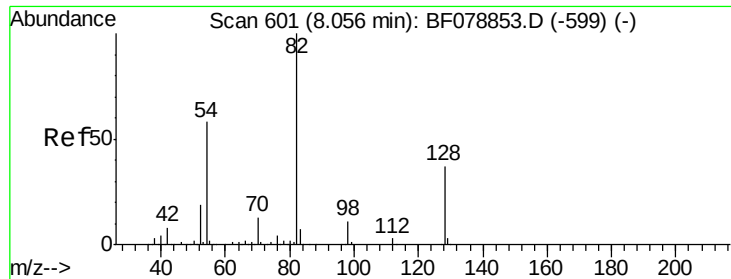




#23
 Nitrobenzene-d5
 Concen: 0.00 ng
 RT: 7.84 min Scan# 582
 Delta R.T. 0.01 min
 Lab File: BF079236.D
 Acq: 14 May 2015 16:17

Instrument :
 BNA_F
 ClientSampleId :
 SSTDCCC040

Tot Ion: 82 Resp: 14038
 Ion Ratio Lower Upper
 82 100
 128 0.0 29.7 44.5#
 54 0.0 46.2 69.4#

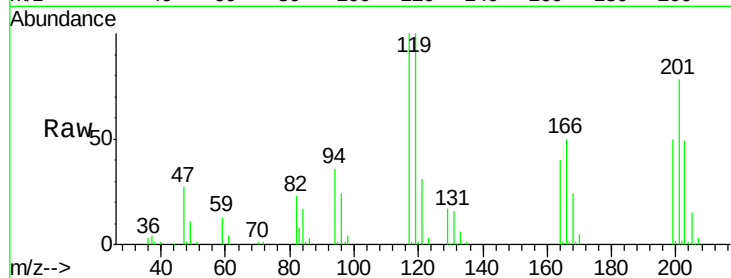



Abundance Ion 82.00 (81.70 to 82.70): BF0
 Ion 128.00 (127.70 to 128.70): B
 Ion 54.00 (53.70 to 54.70): BF0

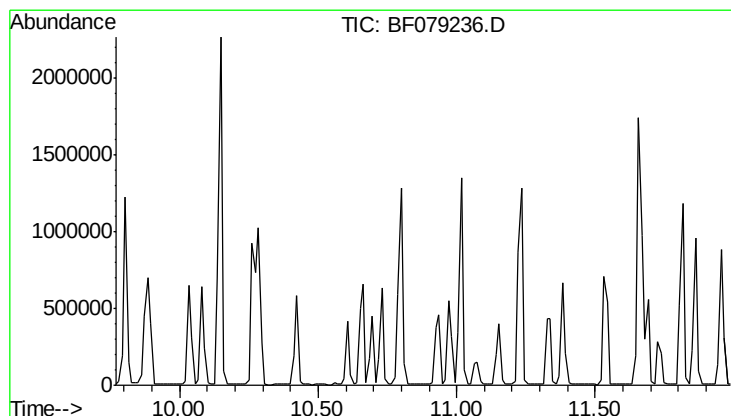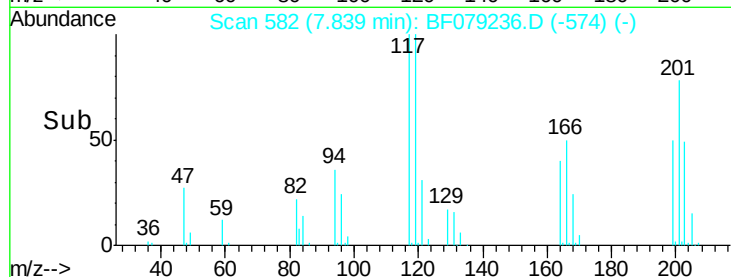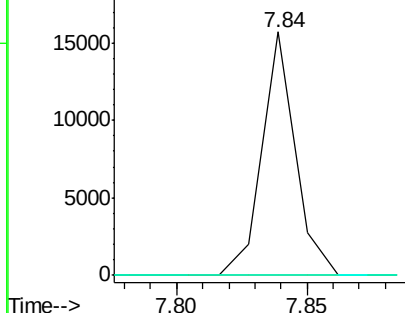

#38
 Acenaphthene-d10
 Concen: 0.00 ng
 Expected RT: 10.88 min
 Lab File: BF079236.D
 Acq: 14 May 2015 16:17

Tgt Ion: 164
 Sig Exp Ratio
 164 100
 162 101.7
 160 45.7

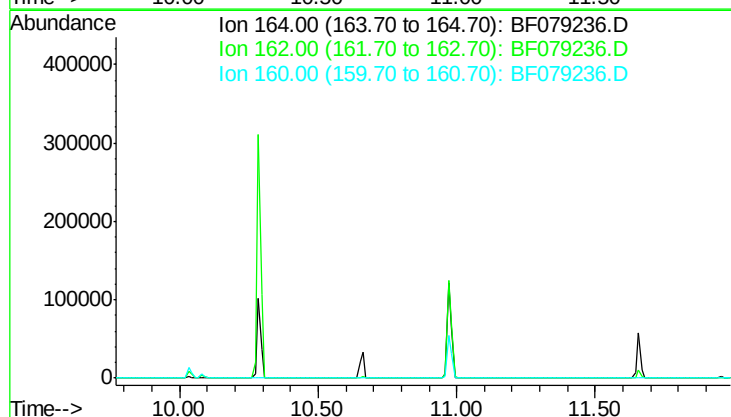

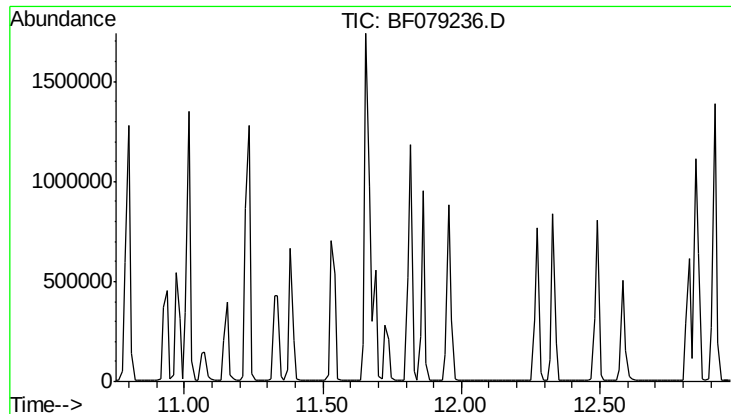

#41

2,4,6-Tribromophenol

Concen: 0.00 ng

Expected RT: 11.86 min

Lab File: BF079236.D

Acq: 14 May 2015 16:17

Instrument :

BNA_F

ClientSampleId :

SSTDCCC040



Tot Ion: 330

Sig Exp Ratio

330 100

332 96.1

141 34.8

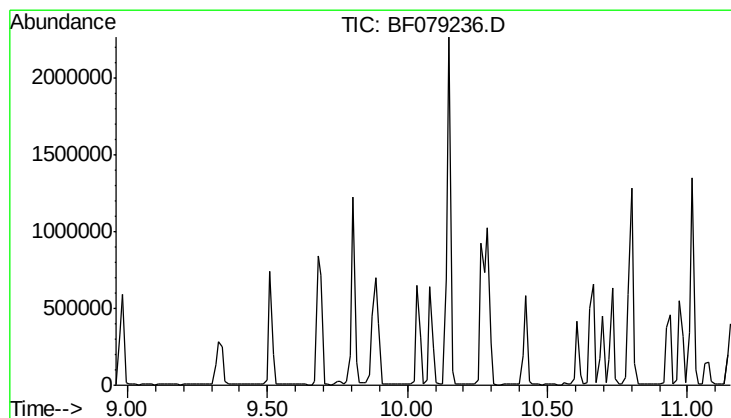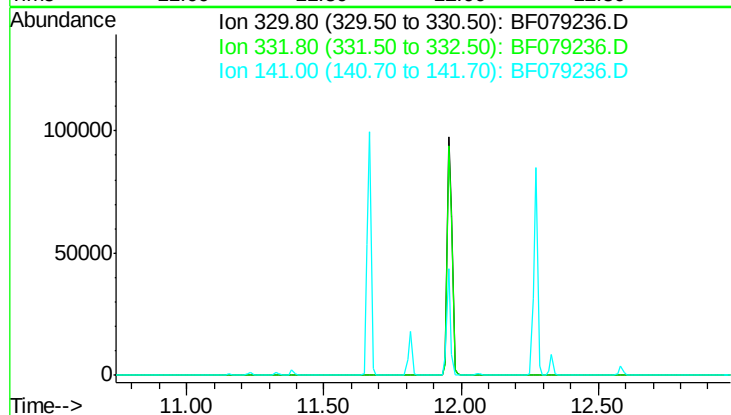

#44

2-Fluorobiphenyl

Concen: 0.00 ng

Expected RT: 10.06 min

Lab File: BF079236.D

Acq: 14 May 2015 16:17


Tgt Ion: 172


Sig Exp Ratio

172 100

171 35.4

170 24.3


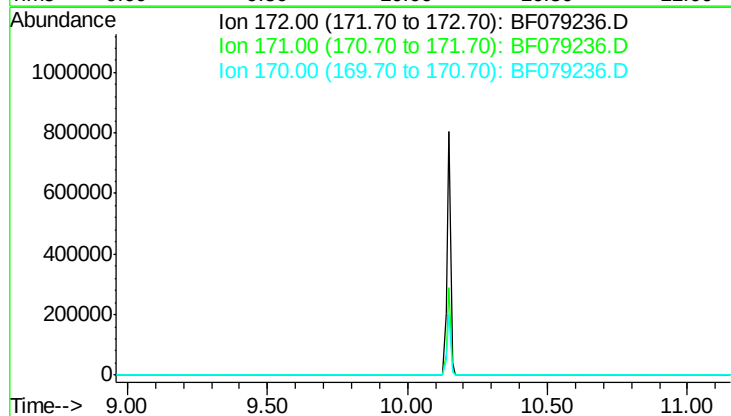


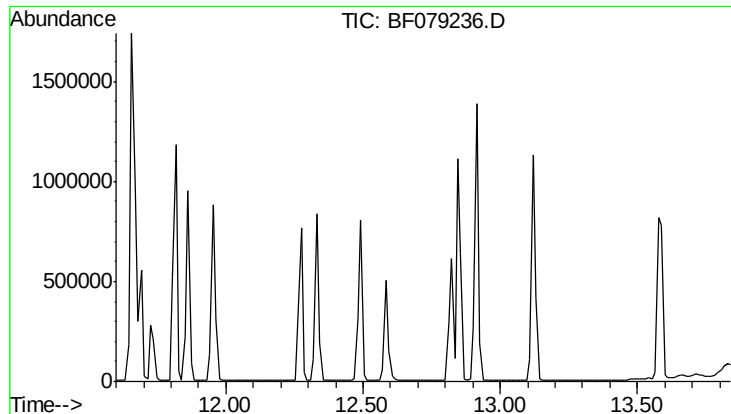

#63
 Phenanthrene-d10
 Concen: 0.00 ng
 Expected RT: 12.72 min
 Lab File: BF079236.D
 Acq: 14 May 2015 16:17


Instrument :
 BNA_F
 ClientSampleId :
 SSTDCCC040


Tot Ion: 188
 Sig Exp Ratio
 188 100
 94 11.7
 80 12.2

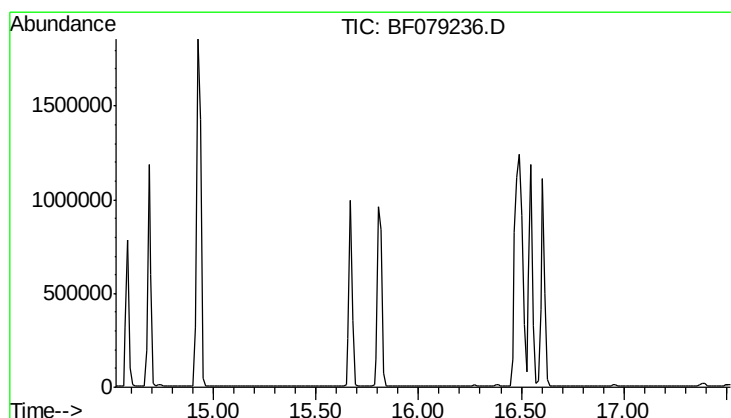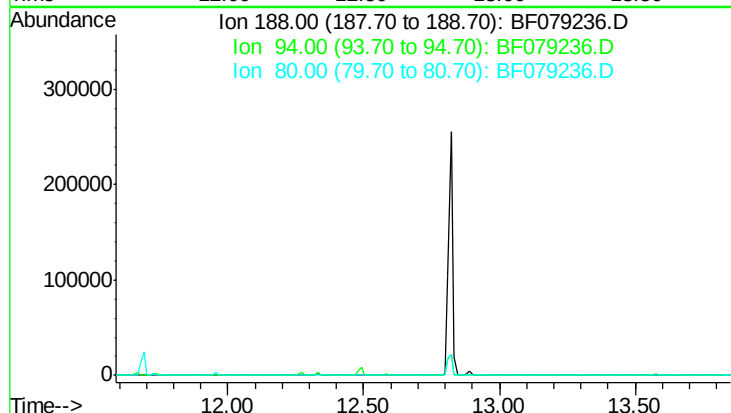

#75
 Chrysene-d12
 Concen: 0.00 ng
 Expected RT: 16.02 min
 Lab File: BF079236.D
 Acq: 14 May 2015 16:17

Tgt Ion: 240
 Sig Exp Ratio
 240 100
 120 10.7
 236 26.3


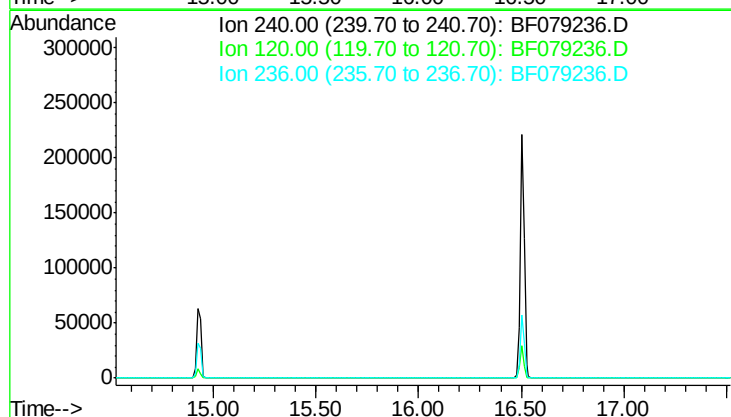


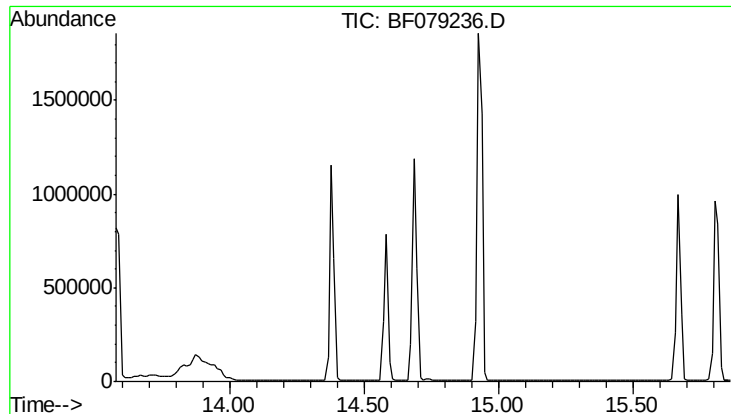

#78
 Terphenyl-d14
 Concen: 0.00 ng
 Expected RT: 14.72 min
 Lab File: BF079236.D
 Acq: 14 May 2015 16:17

Instrument :
 BNA_F
 ClientSampleId :
 SSTDCCC040

Tot Ion: 244
 Sig Exp Ratio
 244 100
 212 7.0
 122 13.1

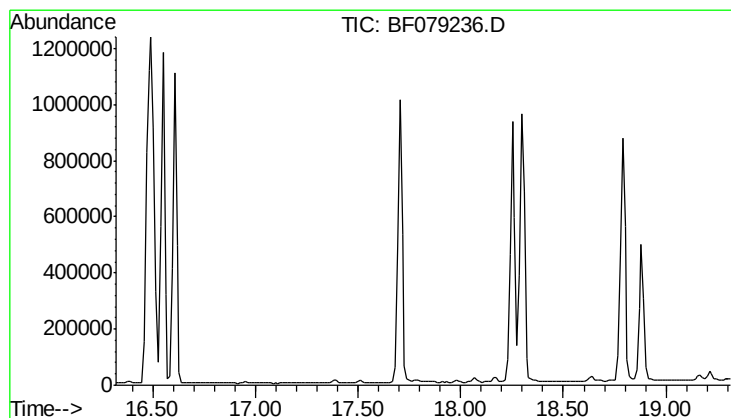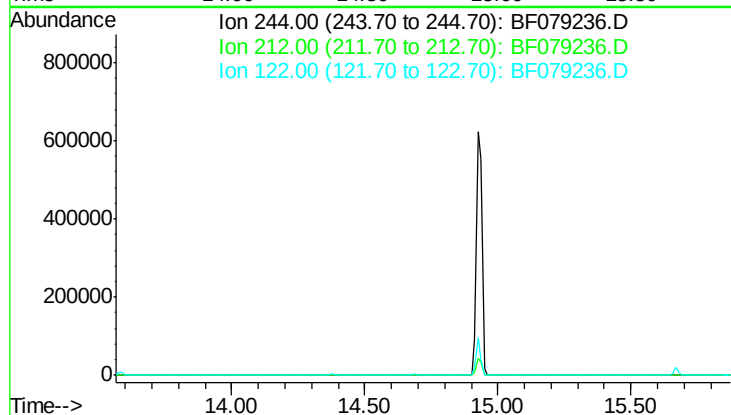

#86
 Perylene-d12
 Concen: 0.00 ng
 Expected RT: 17.82 min
 Lab File: BF079236.D
 Acq: 14 May 2015 16:17

Tgt Ion: 264
 Sig Exp Ratio
 264 100
 260 24.0
 265 21.5

