

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF080415\
 Data File : BF080874.D
 Acq On : 5 Aug 2015 10:39
 Operator : TP/UM
 Sample : G3127-19
 Misc :
 ALS Vial : 32 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 EAST-ABUT-1(0-2)

Quant Time: Aug 05 15:45:37 2015
 Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF080415.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Aug 05 01:46:16 2015
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	6.83	152	59973	20.00	ng	0.00
21) Naphthalene-d8	8.11	136	208955	20.00	ng	0.00
38) Acenaphthene-d10	9.86	164	85262	20.00	ng	0.00
63) Phenanthrene-d10	11.33	188	140032	20.00	ng	0.00
75) Chrysene-d12	13.96	240	116998	20.00	ng	0.00
86) Perylene-d12	15.38	264	146493	20.00	ng	0.01
System Monitoring Compounds						
5) 2-Fluorophenol	5.44	112	492543	124.30	ng	0.01
7) Phenol-d6	6.46	99	761547	147.01	ng	0.01
23) Nitrobenzene-d5	7.39	82	474584	107.04	ng	0.00
41) 2,4,6-Tribromophenol	10.65	330	99020	120.43	ng	0.00
44) 2-Fluorobiphenyl	9.18	172	627506	99.10	ng	0.00
78) Terphenyl-d14	12.92	244	340597	52.69	ng	0.00
Target Compounds						
49) Dimethylphthalate	9.57	163	94122	15.14	ng	Qvalue 100


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF080415\
Data File : BF080874.D
Acq On : 5 Aug 2015 10:39
Operator : TP/UM
Sample : G3127-19
Misc :
ALS Vial : 32 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
EAST-ABUT-1(0-2)

Quant Time: Aug 05 15:45:37 2015
Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF080415.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Aug 05 01:46:16 2015
Response via : Initial Calibration

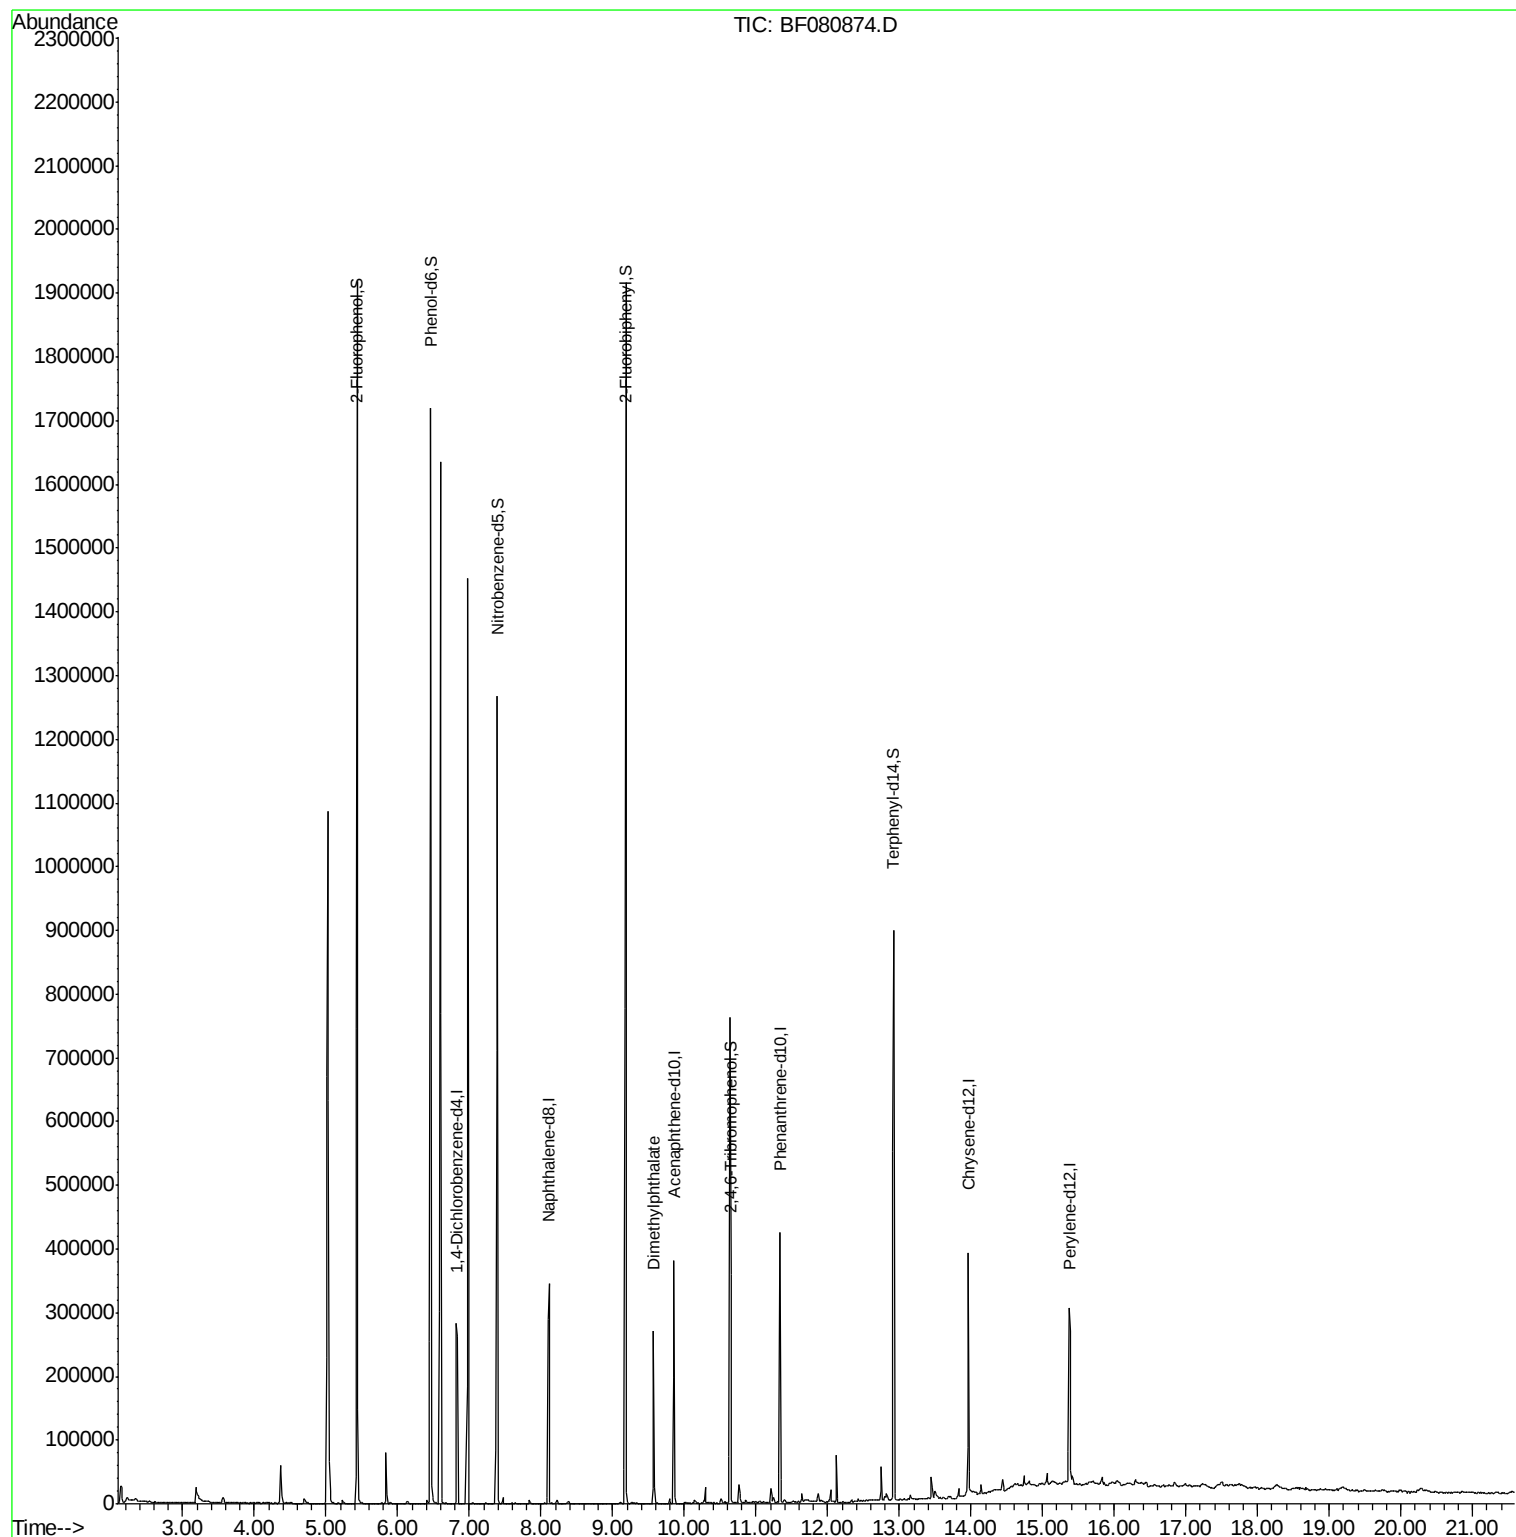

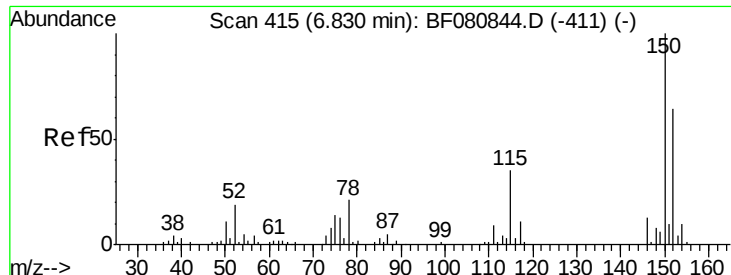


#1




1,4-Dichlorobenzene-d4
Concen: 20.00 ng
RT: 6.83 min Scan# 415
Delta R.T. -0.00 min
Lab File: BF080874.D
Acq: 5 Aug 2015 10:39

Instrument :
BNA_F
ClientSampleId :
EAST-ABUT-1(0-2)

Tgt Ion:152 Resp: 59973
Ion Ratio Lower Upper
152 100
150 156.8 124.6 187.0
115 52.4 44.2 66.4

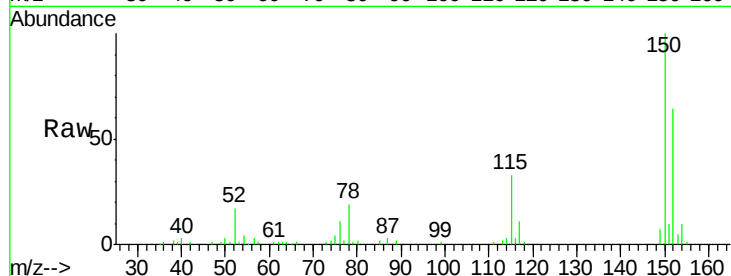


Abundance Ion 152.00 (151.70 to 152.70): E
Ion 150.00 (149.70 to 150.70): E
Ion 115.00 (114.70 to 115.70): E

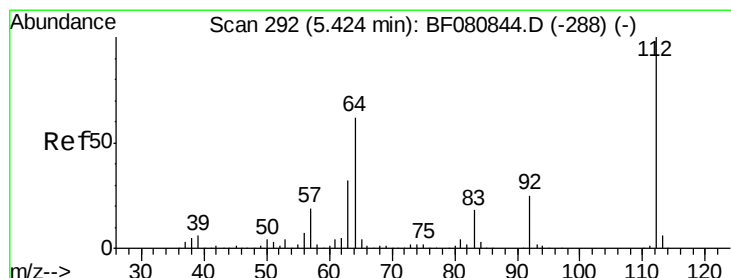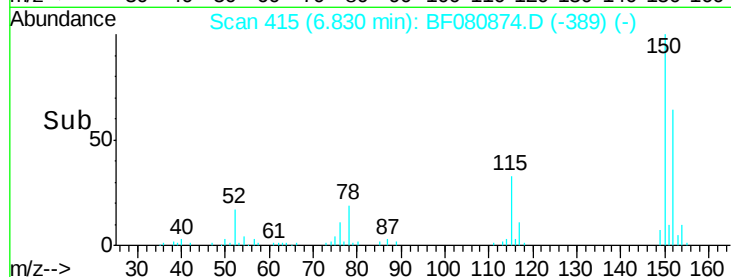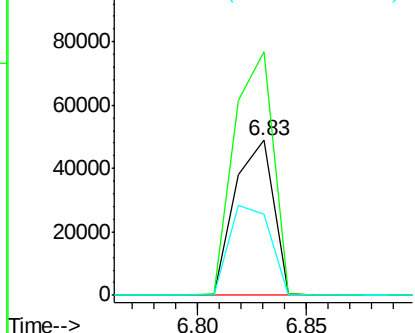



#5


2-Fluorophenol
Concen: 124.30 ng
RT: 5.44 min Scan# 293
Delta R.T. 0.01 min
Lab File: BF080874.D
Acq: 5 Aug 2015 10:39

Tgt Ion:112 Resp: 492543
Ion Ratio Lower Upper
112 100
64 76.5 49.5 74.3#
63 40.2 25.3 37.9#

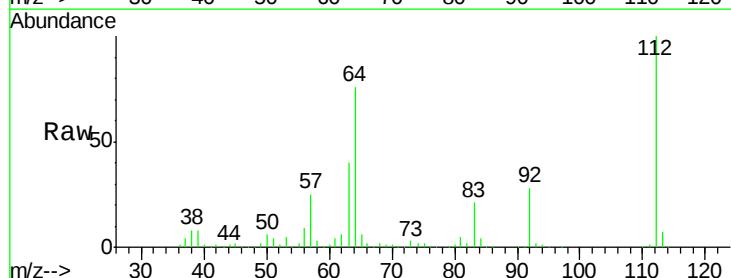

Abundance Ion 112.00 (111.70 to 112.70): E
Ion 64.00 (63.70 to 64.70): BF0
Ion 63.00 (62.70 to 63.70): BF0

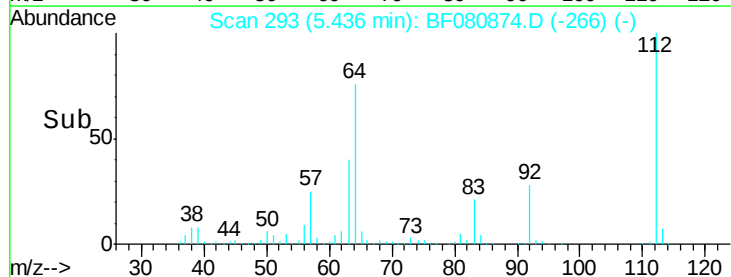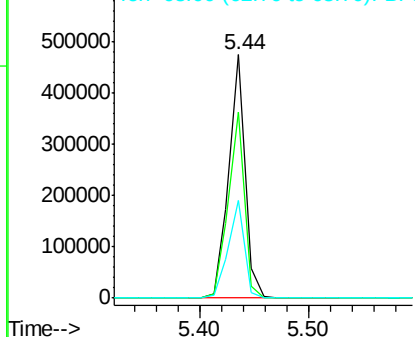

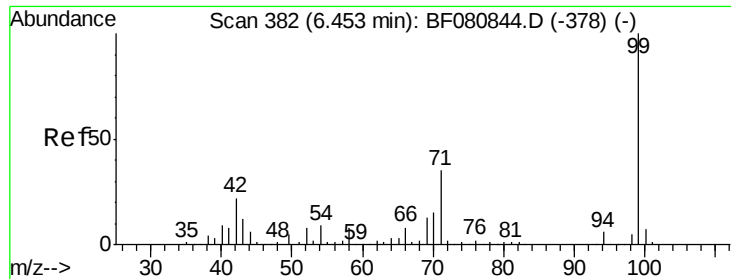

#7

Phenol-d6

Concen: 147.01 ng

RT: 6.46 min Scan# 383

Delta R.T. 0.01 min

Lab File: BF080874.D

Acq: 5 Aug 2015 10:39

Instrument :

BNA_F

ClientSampleId :

EAST-ABUT-1(0-2)


Tgt Ion: 99 Resp: 761547

Ion Ratio Lower Upper

99 100

42 18.9 17.9 26.9




71 33.5 28.2 42.4

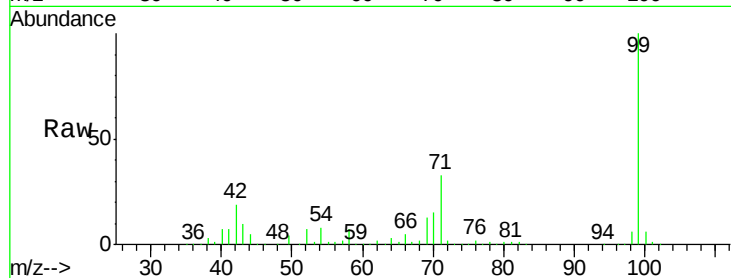

Abundance Ion 99.00 (98.70 to 99.70): BF0

Ion 42.00 (41.70 to 42.70): BF0

Ion 71.00 (70.70 to 71.70): BF0

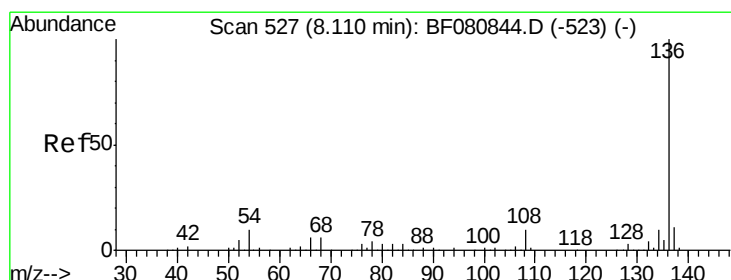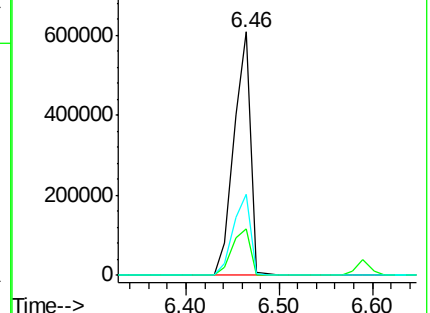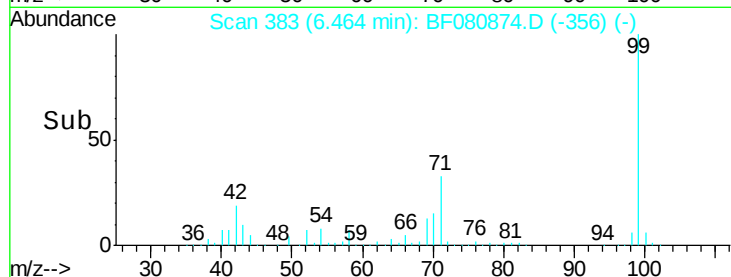

#21

Naphthalene-d8

Concen: 20.00 ng

RT: 8.11 min Scan# 527

Delta R.T. -0.00 min

Lab File: BF080874.D

Acq: 5 Aug 2015 10:39

Tgt Ion: 136 Resp: 208955


Ion Ratio Lower Upper

136 100

137 10.5 8.6 13.0

54 8.4 8.3 12.5

68 4.9 4.8 7.2


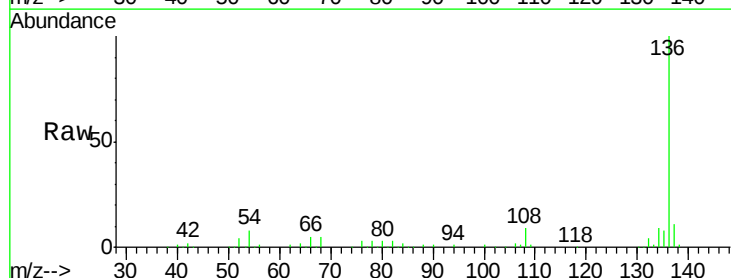



Abundance Ion 136.00 (135.70 to 136.70): E

Ion 137.00 (136.70 to 137.70): E

Ion 54.00 (53.70 to 54.70): BF0

Ion 68.00 (67.70 to 68.70): BF0

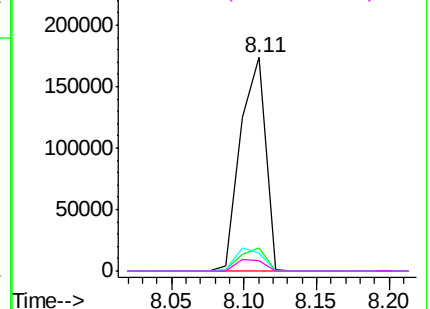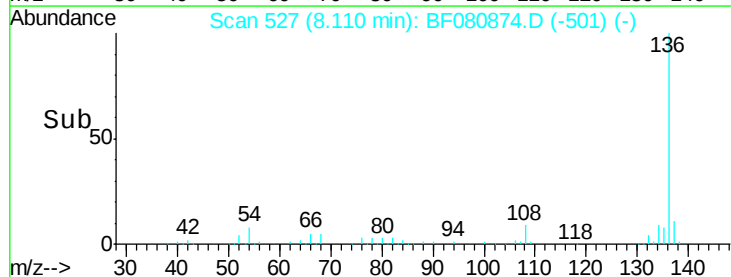


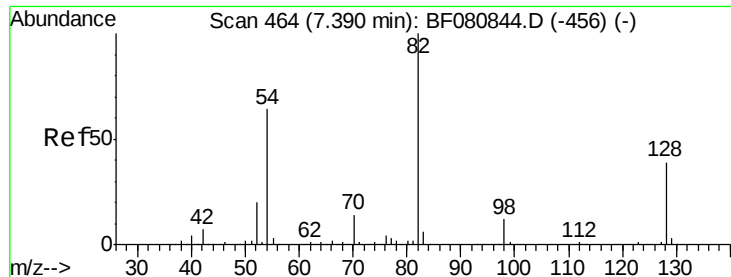




#23
 Nitrobenzene-d5
 Concen: 107.04 ng
 RT: 7.39 min Scan# 464
 Delta R.T. -0.00 min
 Lab File: BF080874.D
 Acq: 5 Aug 2015 10:39

Instrument :
 BNA_F
 ClientSampleId :
 EAST-ABUT-1(0-2)

Tgt Ion: 82 Resp: 474584
 Ion Ratio Lower Upper
 82 100
 128 41.6 31.0 46.4
 54 59.3 51.0 76.6

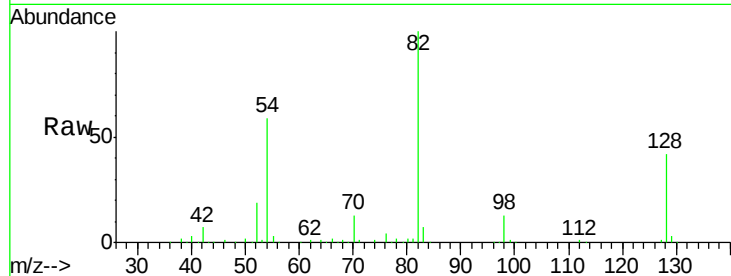


Abundance Ion 82.00 (81.70 to 82.70): BF0
 Ion 128.00 (127.70 to 128.70): B
 Ion 54.00 (53.70 to 54.70): BF0

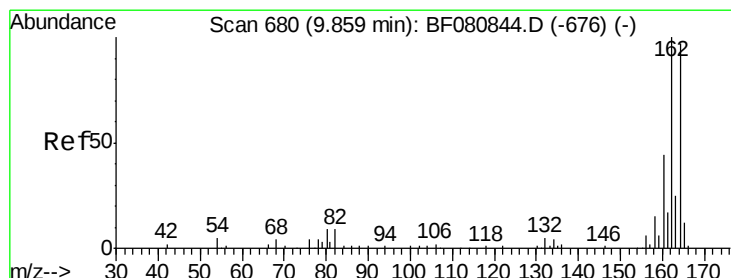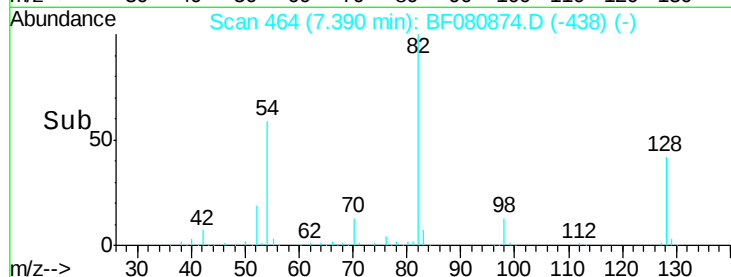
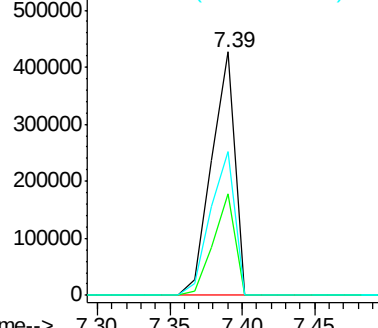



#38
 Acenaphthene-d10
 Concen: 20.00 ng
 RT: 9.86 min Scan# 680
 Delta R.T. -0.00 min
 Lab File: BF080874.D
 Acq: 5 Aug 2015 10:39

Tgt Ion: 164 Resp: 85262
 Ion Ratio Lower Upper
 164 100
 162 104.9 82.9 124.3
 160 47.0 36.6 54.8

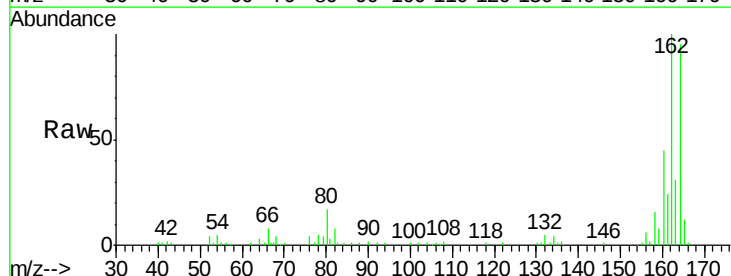

Abundance Ion 164.00 (163.70 to 164.70): E
 Ion 162.00 (161.70 to 162.70): E
 Ion 160.00 (159.70 to 160.70): E

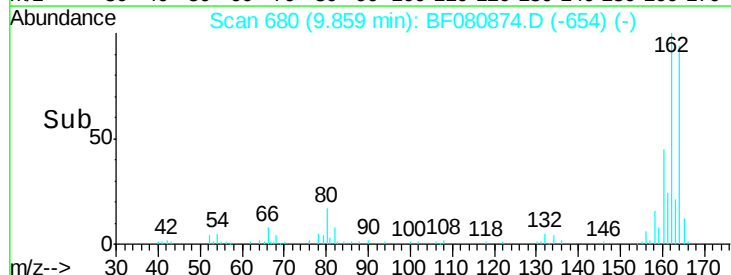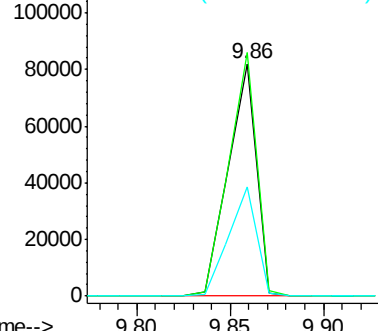


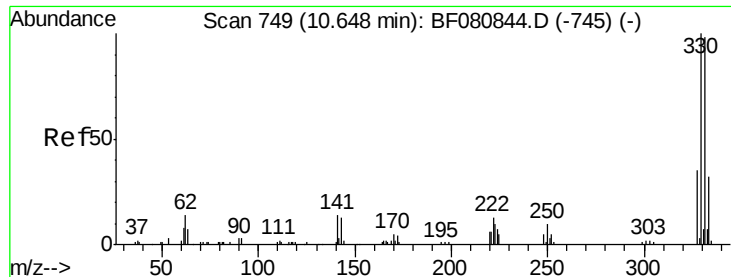




#41
 2,4,6-Tribromophenol
 Concen: 120.43 ng
 RT: 10.65 min Scan# 749
 Delta R.T. -0.00 min
 Lab File: BF080874.D
 Acq: 5 Aug 2015 10:39

Instrument :
 BNA_F
 ClientSampleId :
 EAST-ABUT-1(0-2)

Tgt Ion:330 Resp: 99020
 Ion Ratio Lower Upper
 330 100
 332 95.0 77.8 116.8
 141 34.9 28.4 42.6

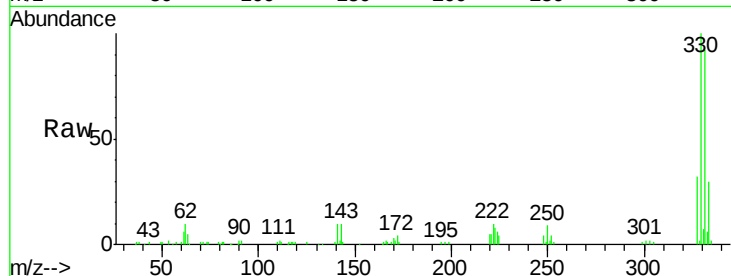


Abundance Ion 329.80 (329.50 to 330.50): E
 Ion 331.80 (331.50 to 332.50): E
 Ion 141.00 (140.70 to 141.70): E

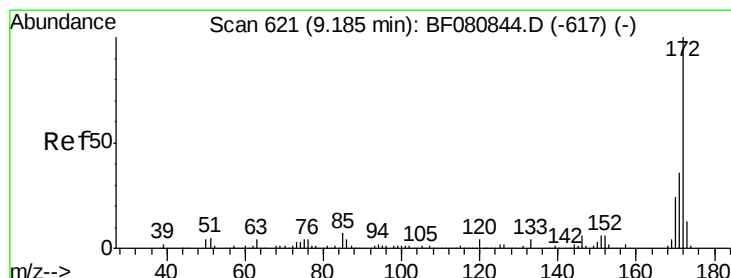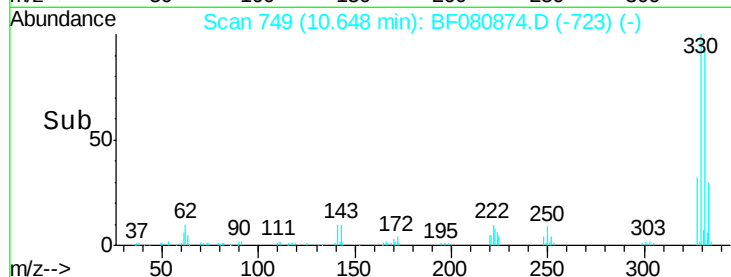
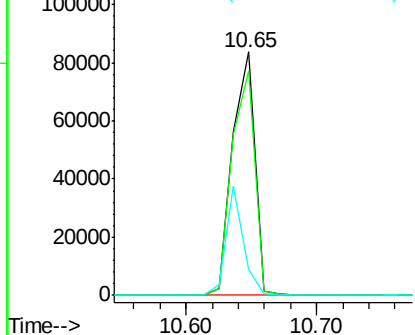



#44
 2-Fluorobiphenyl
 Concen: 99.10 ng
 RT: 9.18 min Scan# 621
 Delta R.T. -0.00 min
 Lab File: BF080874.D
 Acq: 5 Aug 2015 10:39

Tgt Ion:172 Resp: 627506
 Ion Ratio Lower Upper
 172 100
 171 36.1 28.9 43.3
 170 24.3 19.4 29.2

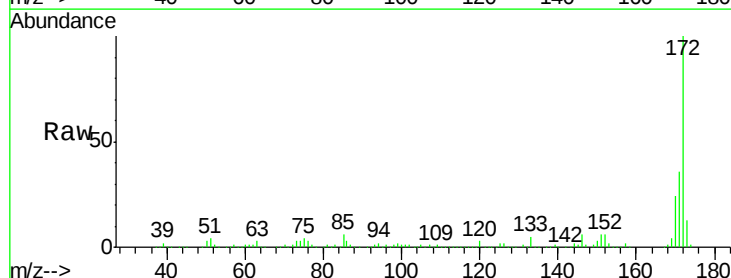

Abundance Ion 172.00 (171.70 to 172.70): E
 Ion 171.00 (170.70 to 171.70): E
 Ion 170.00 (169.70 to 170.70): E

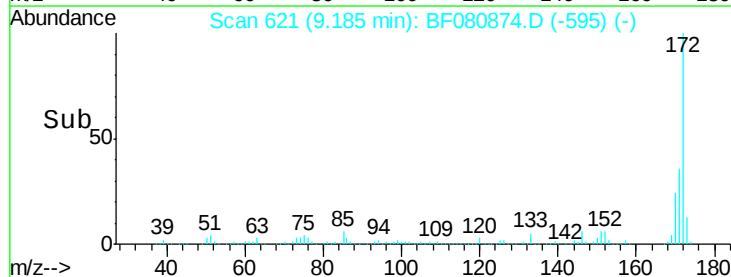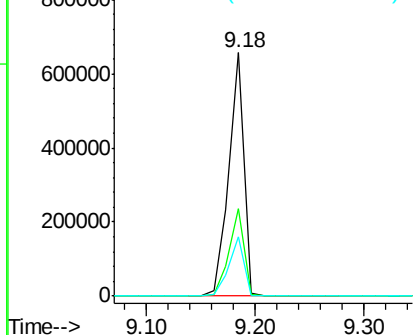

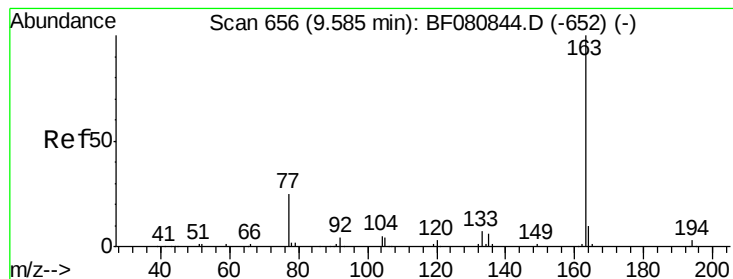

#49

Dimethylphthalate

Concen: 15.14 ng

RT: 9.57 min Scan# 655

Delta R.T. -0.01 min

Lab File: BF080874.D

Acq: 5 Aug 2015 10:39

Instrument :

BNA_F

ClientSampleId :

EAST-ABUT-1(0-2)


Tgt Ion:163 Resp: 94122

Ion Ratio Lower Upper

163 100

194 3.1 2.6 4.0




164 10.3 8.2 12.4

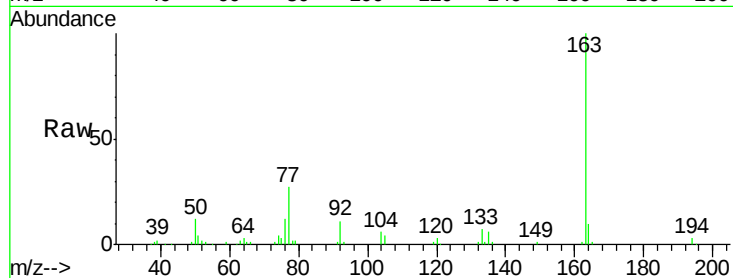

Abundance Ion 163.00 (162.70 to 163.70): E

Ion 194.00 (193.70 to 194.70): E

Ion 164.00 (163.70 to 164.70): E

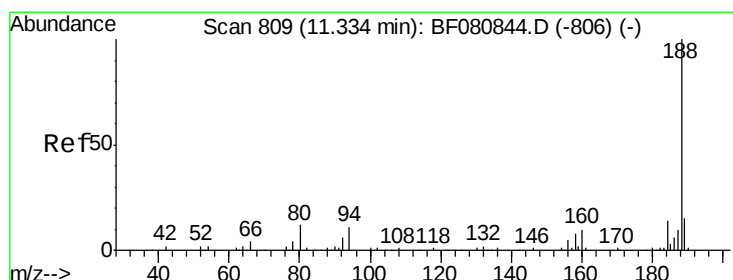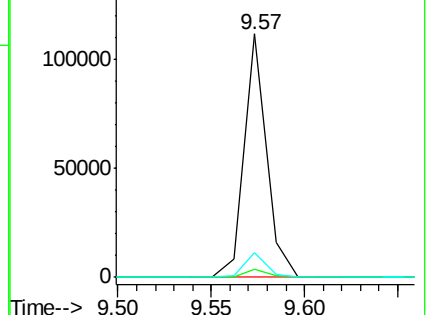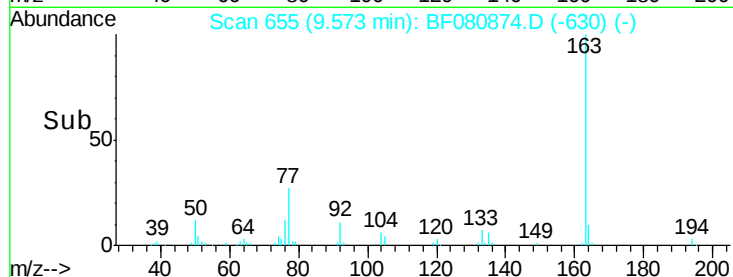

#63

Phenanthrene-d10

Concen: 20.00 ng

RT: 11.33 min Scan# 809

Delta R.T. -0.00 min

Lab File: BF080874.D

Acq: 5 Aug 2015 10:39


Tgt Ion:188 Resp: 140032

Ion Ratio Lower Upper

188 100

94 10.3 8.6 12.8



80 11.0 9.3 13.9

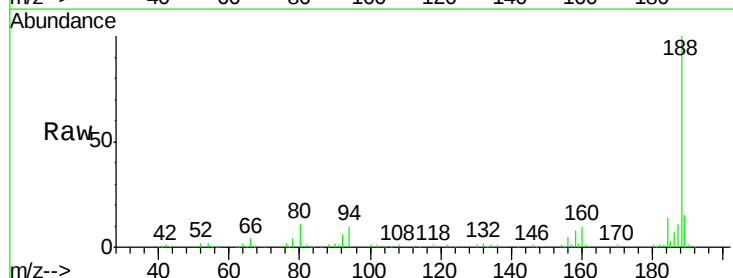


Abundance Ion 188.00 (187.70 to 188.70): E

Ion 94.00 (93.70 to 94.70): BF0

Ion 80.00 (79.70 to 80.70): BF0

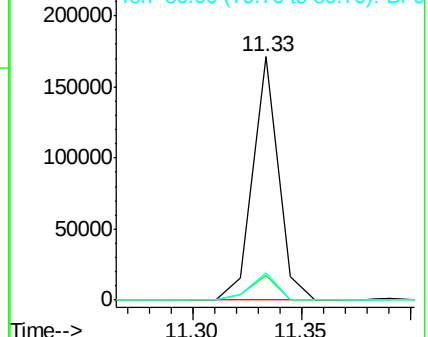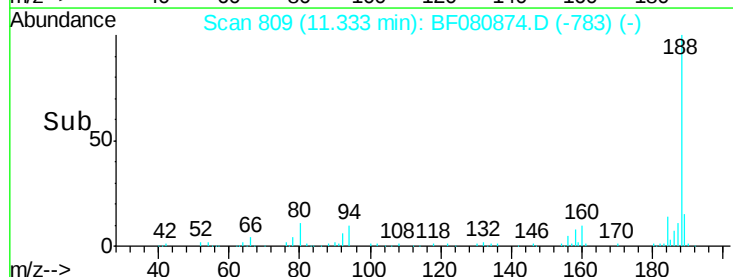

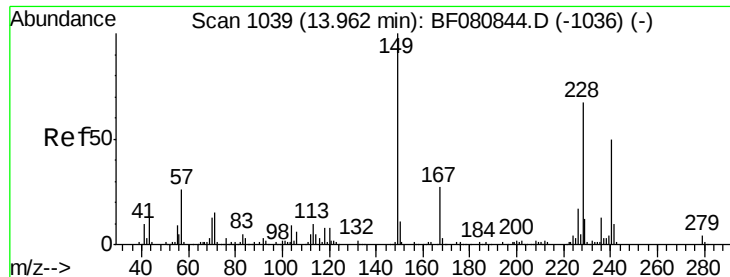

#75

Chrysene-d12

Concen: 20.00 ng

RT: 13.96 min Scan# 1039

Delta R.T. -0.00 min

Lab File: BF080874.D

Acq: 5 Aug 2015 10:39

Instrument :

BNA_F

ClientSampleId :

EAST-ABUT-1(0-2)


Tgt Ion:240 Resp: 116998

Ion Ratio Lower Upper

240 100

120 11.7 13.0 19.6#




236 26.0 20.7 31.1

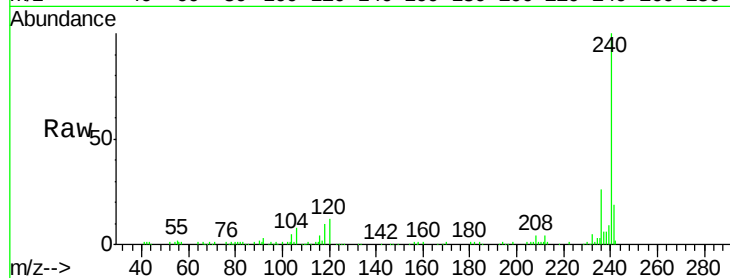

Abundance Ion 240.00 (239.70 to 240.70): E

Ion 120.00 (119.70 to 120.70): E

Ion 236.00 (235.70 to 236.70): E

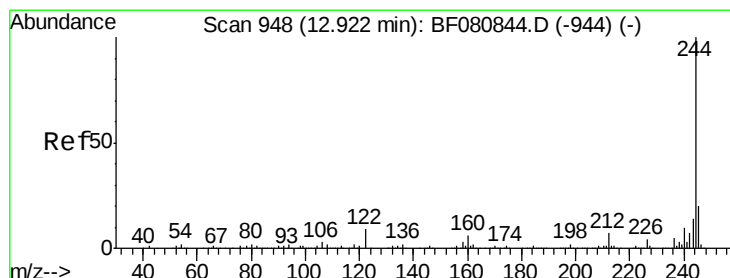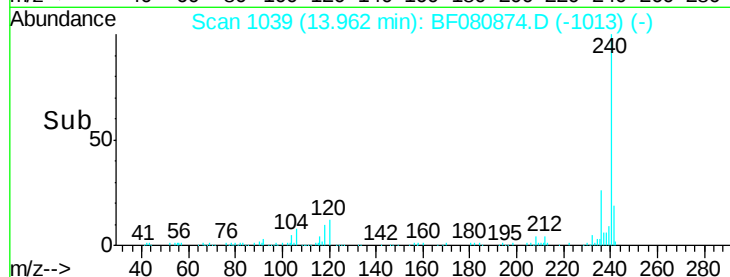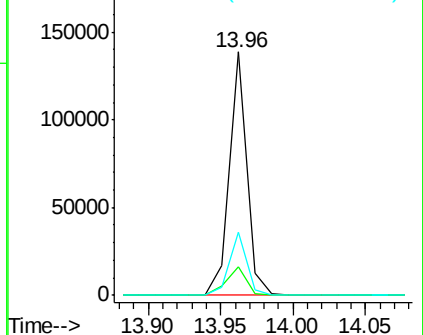

#78

Terphenyl-d14

Concen: 52.69 ng

RT: 12.92 min Scan# 948

Delta R.T. -0.00 min

Lab File: BF080874.D

Acq: 5 Aug 2015 10:39


Tgt Ion:244 Resp: 340597

Ion Ratio Lower Upper

244 100

212 6.8 5.5 8.3



122 8.0 7.1 10.7

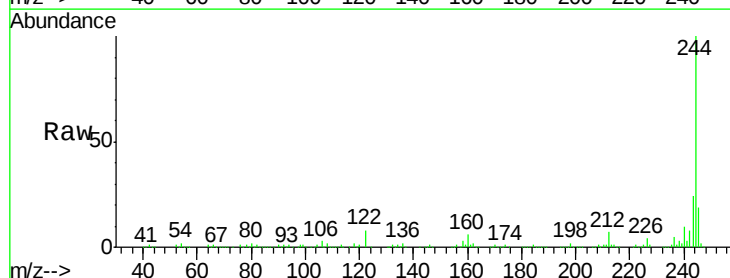


Abundance Ion 244.00 (243.70 to 244.70): E

Ion 212.00 (211.70 to 212.70): E

Ion 122.00 (121.70 to 122.70): E

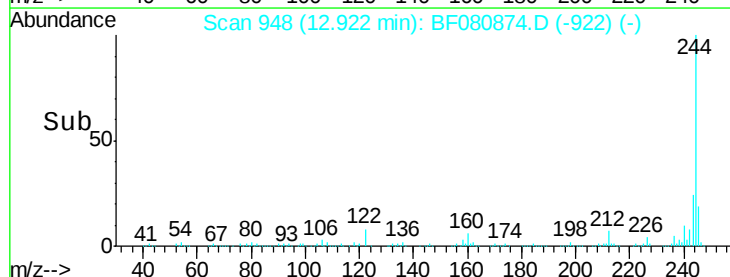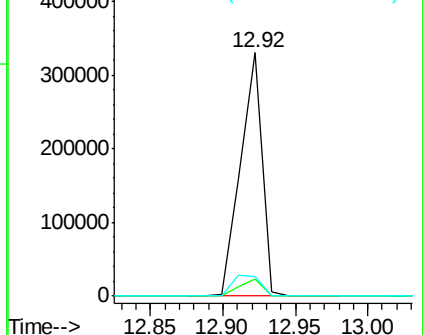

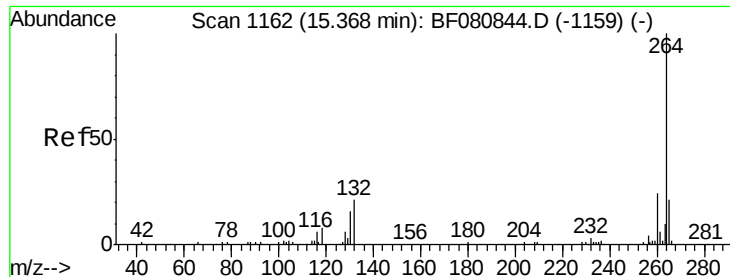

#86
Perylene-d12
Concen: 20.00 ng
RT: 15.38 min Scan# 1163
Delta R.T. 0.01 min
Lab File: BF080874.D
Acq: 5 Aug 2015 10:39

Instrument :
BNA_F
ClientSampleId :
EAST-ABUT-1(0-2)

Tgt Ion: 264 Resp: 146493
Ion Ratio Lower Upper
264 100
260 24.3 18.9 28.3
265 20.9 16.8 25.2

