

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF080415\
Data File : BF080859.D
Acq On : 5 Aug 2015 1:59
Operator : TP/UM
Sample : G3173-05
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
SVOC-GPC-BLANK

Integration Parameters: rteint.p
Integrator: RTE
Smoothing : ON Filtering: 5
Sampling : 1 Min Area: 3 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF080415.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	2.224	5	12	16	rBV	4690	17046	2.42%	0.522%
2	6.819	412	414	417	rBB	536353	537686	76.22%	16.455%
3	8.110	524	527	529	rBV	507096	705429	100.00%	21.588%
4	9.859	677	680	682	rBB	618517	700311	99.27%	21.431%
5	11.334	806	809	811	rBV	775629	638765	90.55%	19.548%
6	13.962	1036	1039	1041	rBV	435221	403857	57.25%	12.359%
7	15.368	1159	1162	1165	rBV	238770	264583	37.51%	8.097%


Sum of corrected areas: 3267677

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF080415\
Data File : BF080859.D
Acq On : 5 Aug 2015 1:59
Operator : TP/UM
Sample : G3173-05
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
SVOC-GPC-BLANK

Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF080415.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

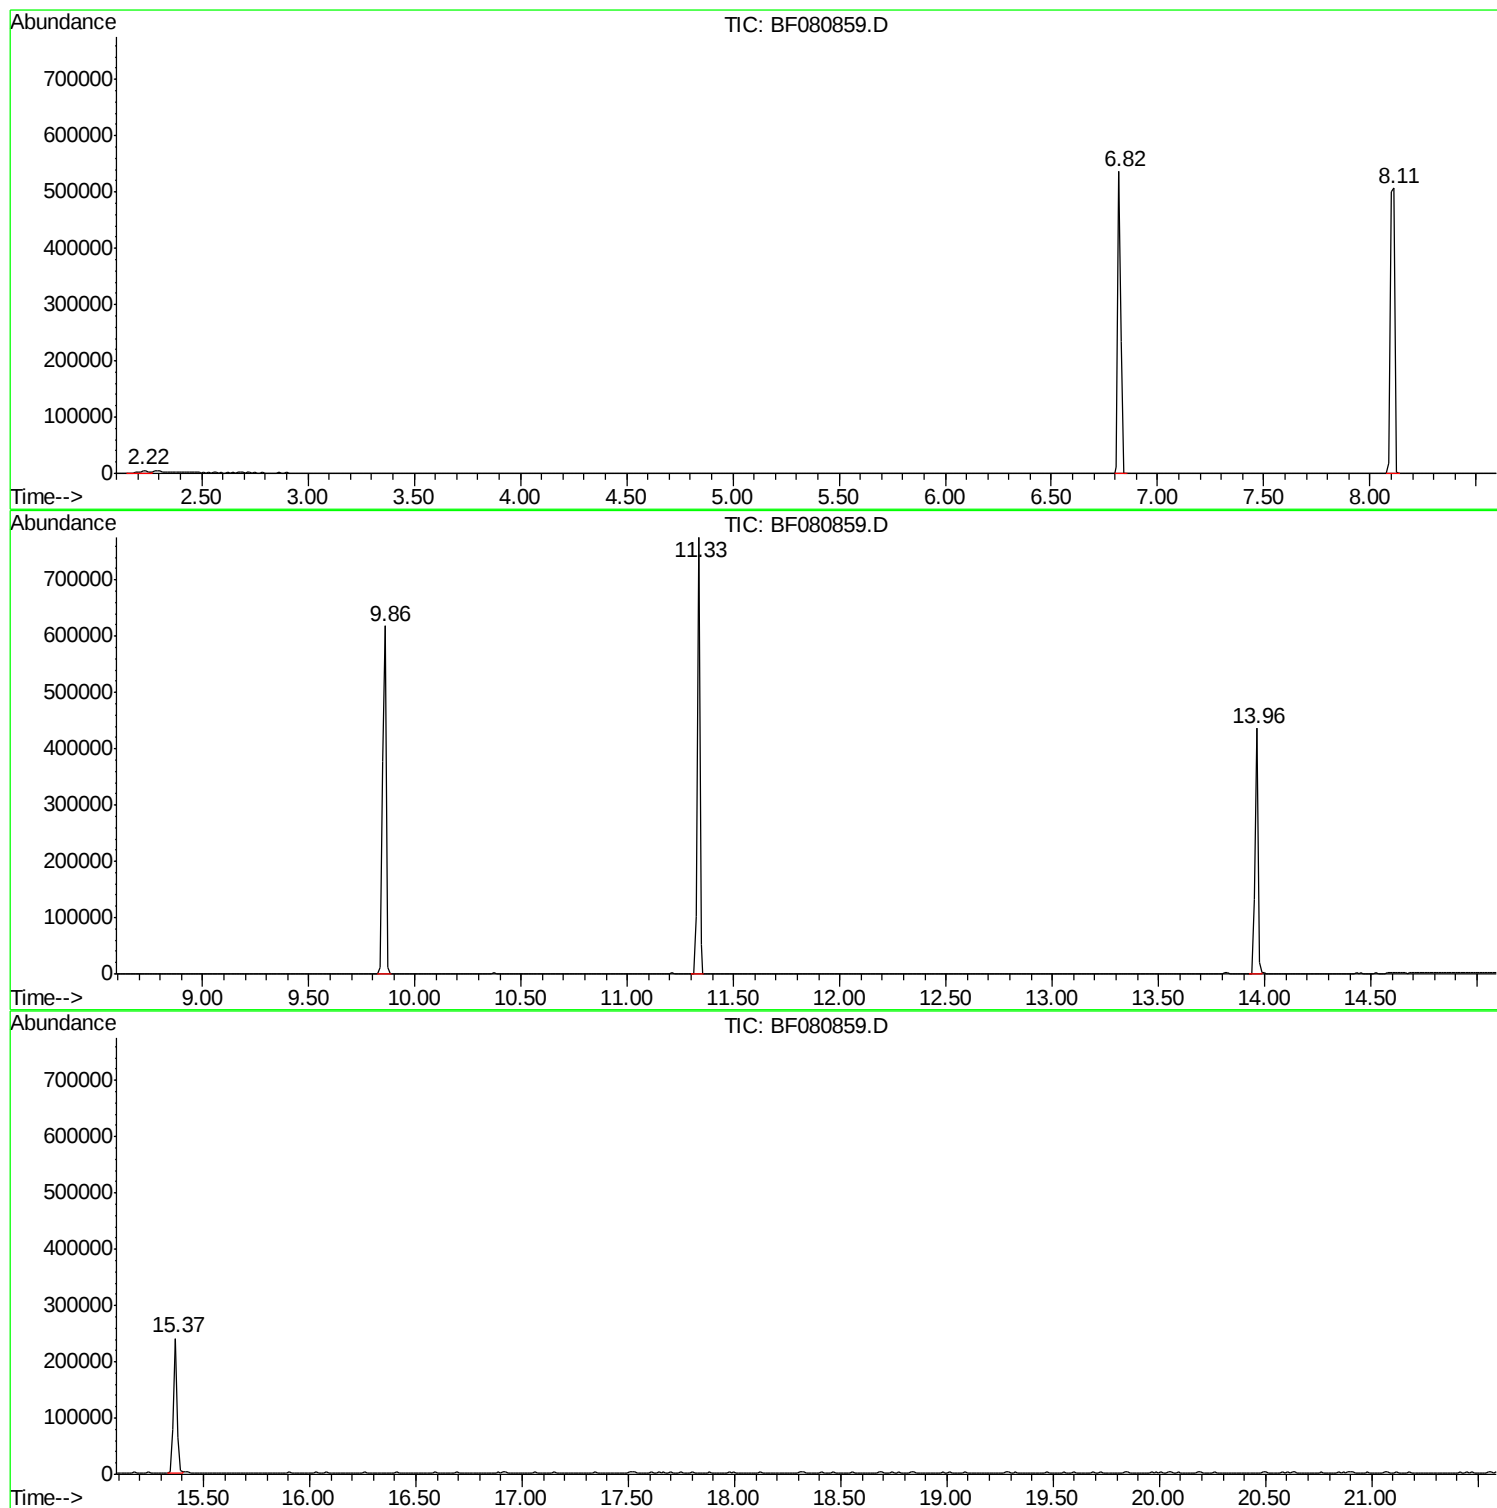

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF080415\
Data File : BF080859.D
Acq On : 5 Aug 2015 1:59
Operator : TP/UM
Sample : G3173-05
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
SVOC-GPC-BLANK

Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF080415.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF080415\
Data File : BF080859.D
Acq On : 5 Aug 2015 1:59
Operator : TP/UM
Sample : G3173-05
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
SVOC-GPC-BLANK

Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF080415.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	---Internal Standard---
					# RT Resp Conc
