


Data Path : Z:\HPCHEM1\BNA_F\DATA\BF080415\
 Data File : BF080861.D
 Acq On : 5 Aug 2015 4:02
 Operator : TP/UM
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF080415.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed Aug 05 01:46:16 2015

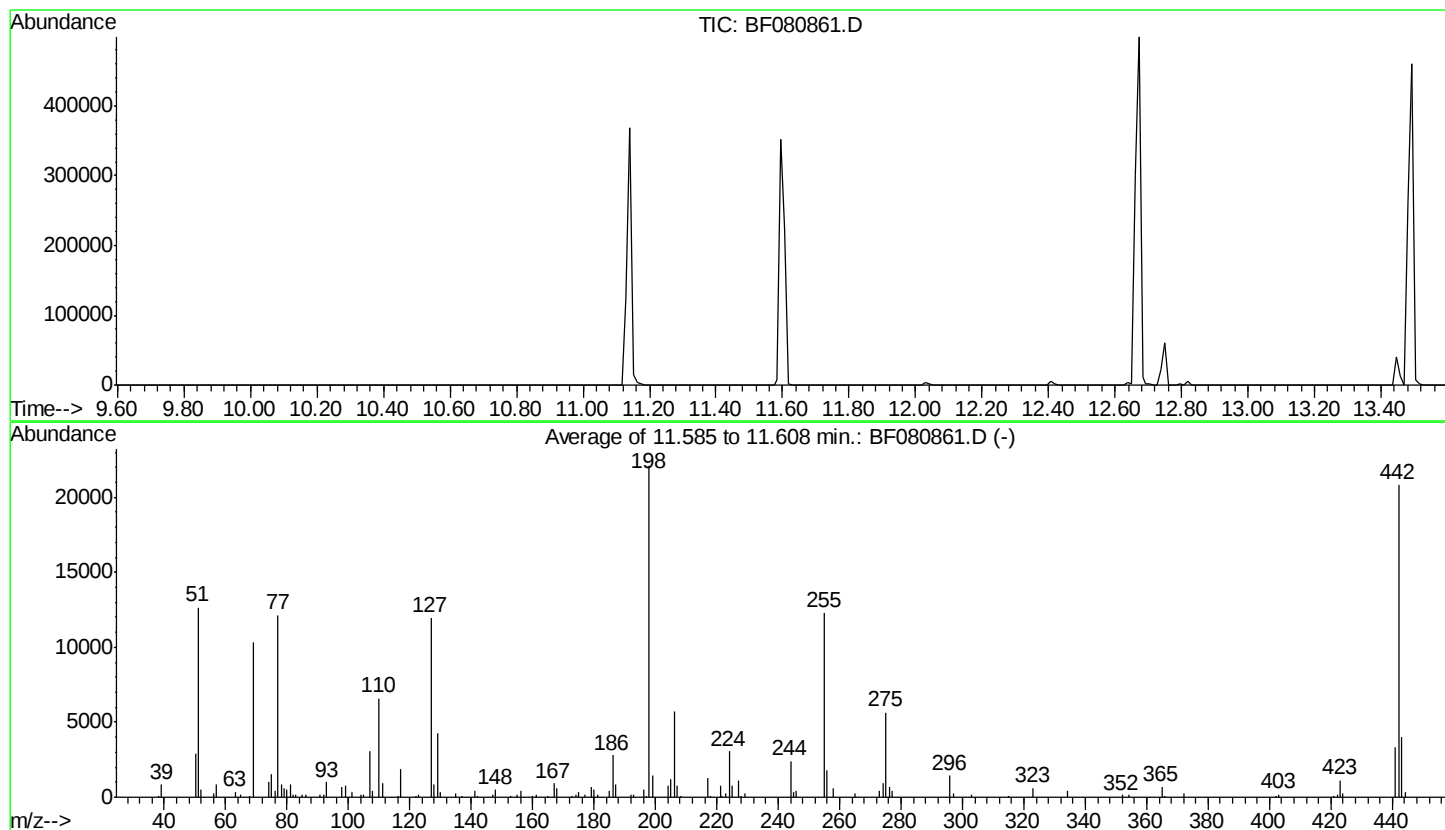

AutoFind: Scans 831, 832, 833; Background Corrected with Scan 828

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	57.2	12646	PASS
68	69	0.00	2	1.1	110	PASS
69	198	0.00	100	46.8	10348	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	54.1	11952	PASS
197	198	0.00	2	0.5	104	PASS
198	198	100	100	100.0	22108	PASS
199	198	5	9	6.7	1474	PASS
275	198	10	60	25.6	5663	PASS
365	198	1	100	3.2	713	PASS
441	442	0.01	24	16.0	3342	PASS
442	198	50	100	94.2	20828	PASS
443	442	15	24	19.2	4001	PASS