
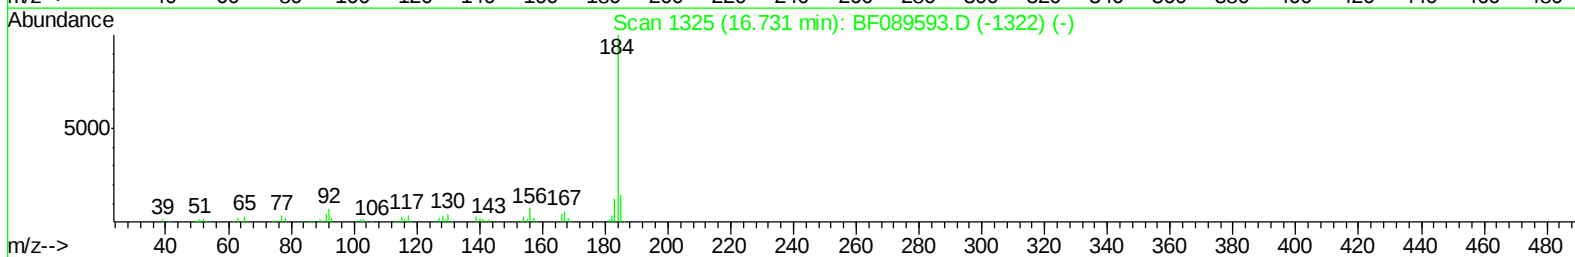
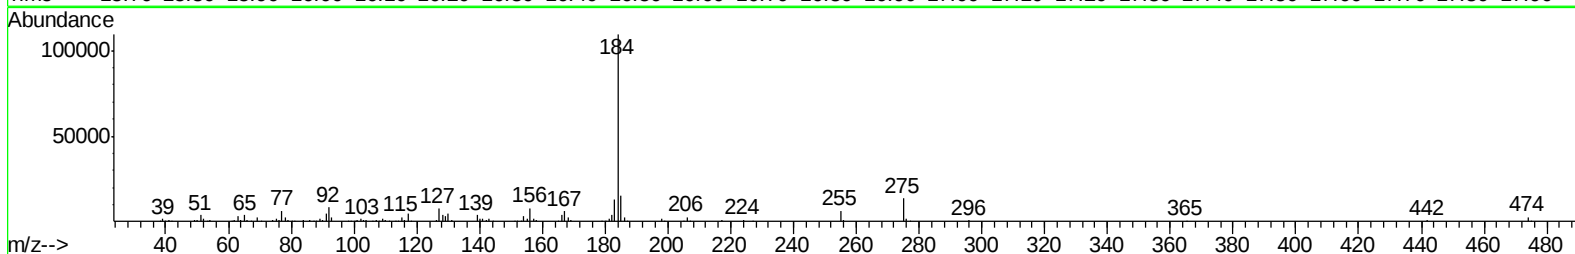


Data Path : Z:\HPCHEM1\BNA_F\DATA\BF080416\
Data File : BF089589.D
Acq On : 4 Aug 2016 15:12
Operator : UM/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Aug 05 07:54:39 2016
Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF080416.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Aug 05 01:39:23 2016
Response via : Initial Calibration

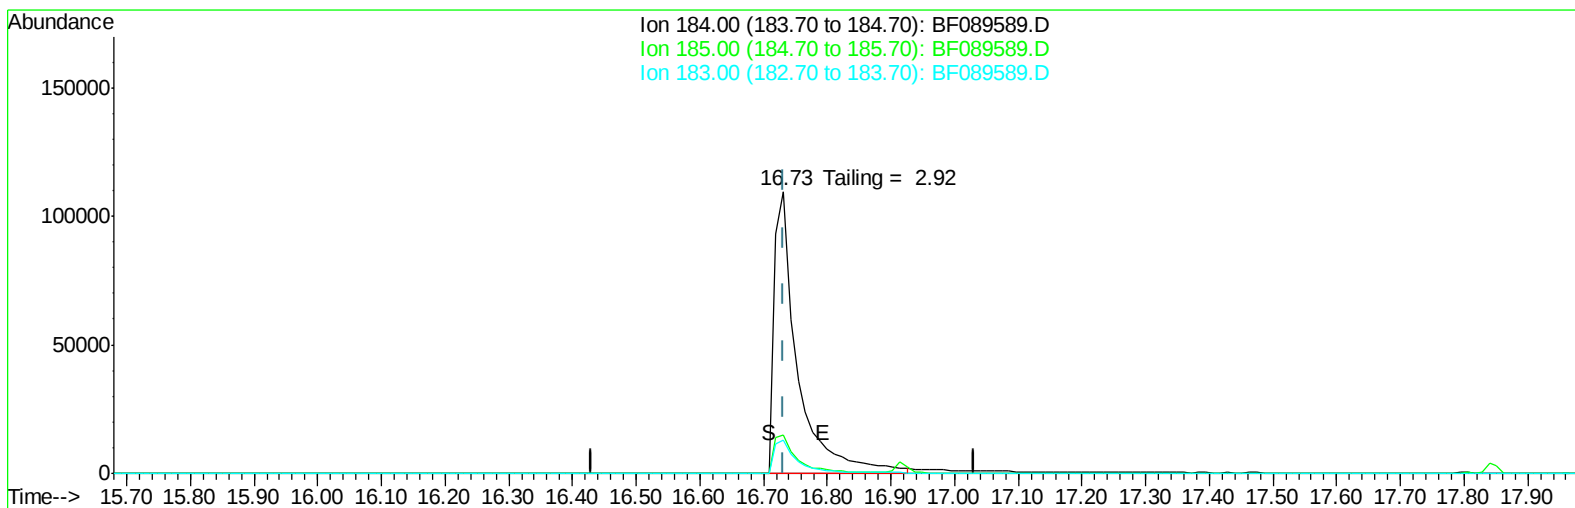

TIC: BF089589.D

(76) Benzidine




16.731min (+0.000) 0.00ng

response 282030

Ion	Exp%	Act%
184.00	100	100
185.00	14.40	13.63
183.00	12.30	11.79
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF080416\
Data File : BF089589.D
Acq On : 4 Aug 2016 15:12
Operator : UM/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Aug 05 07:54:39 2016
Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF080416.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Aug 05 01:39:23 2016
Response via : Initial Calibration

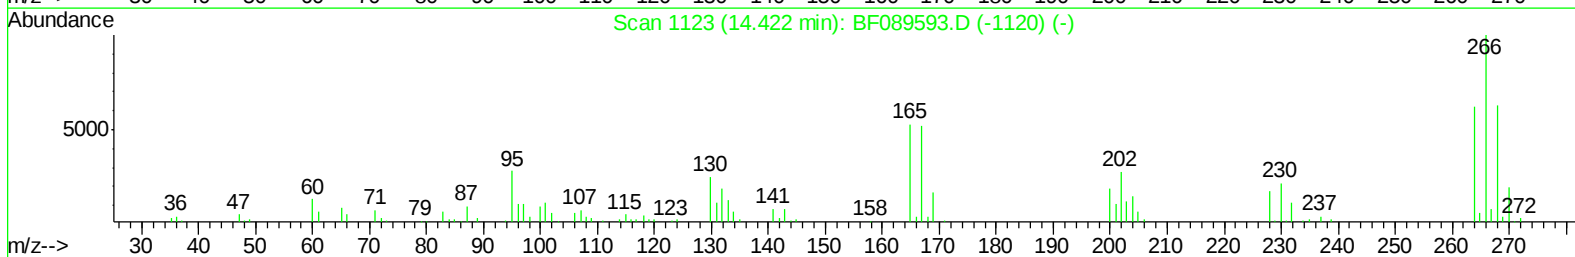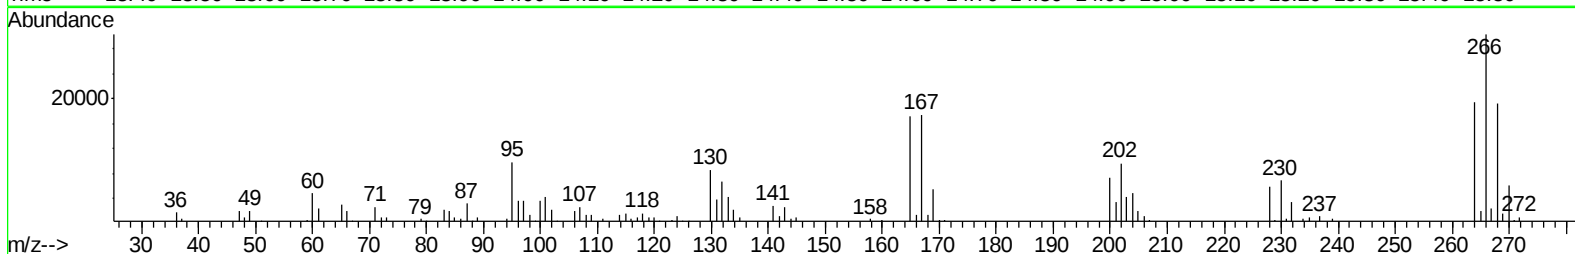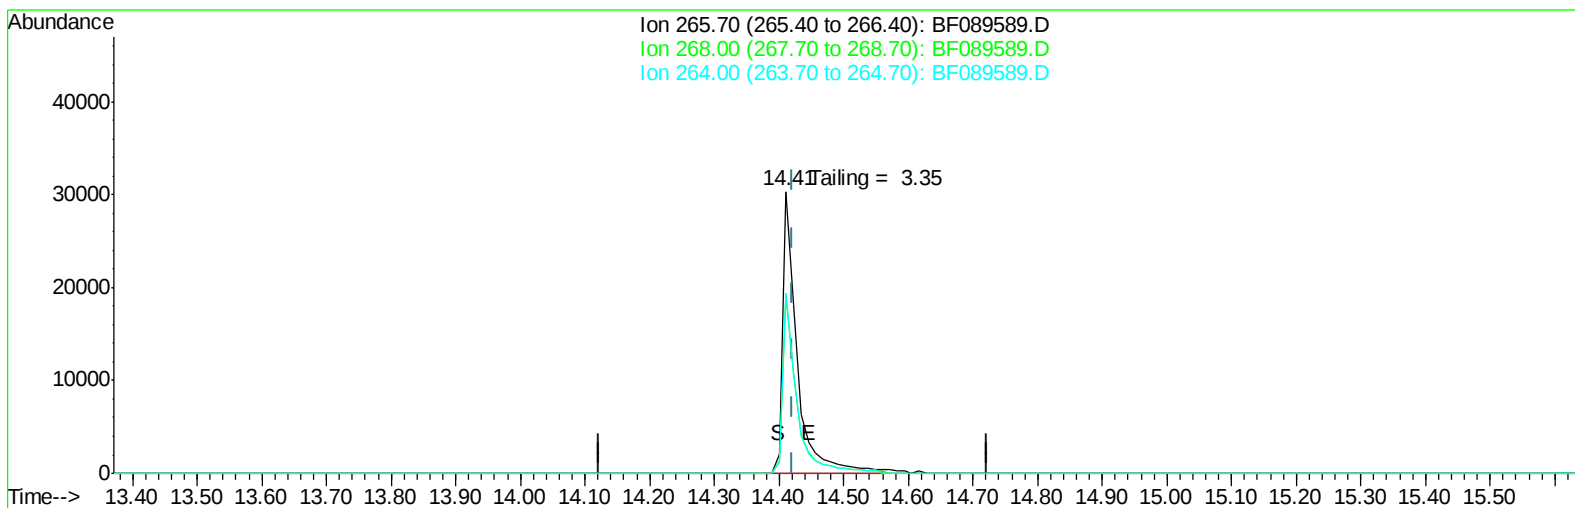

TIC: BF089589.D

(69) Pentachlorophenol (C)

14.411min (-0.011) 0.00ng

response 48621

Ion	Exp%	Act%
265.70	100	100
268.00	63.20	63.41
264.00	61.90	64.04
0.00	0.00	0.00