
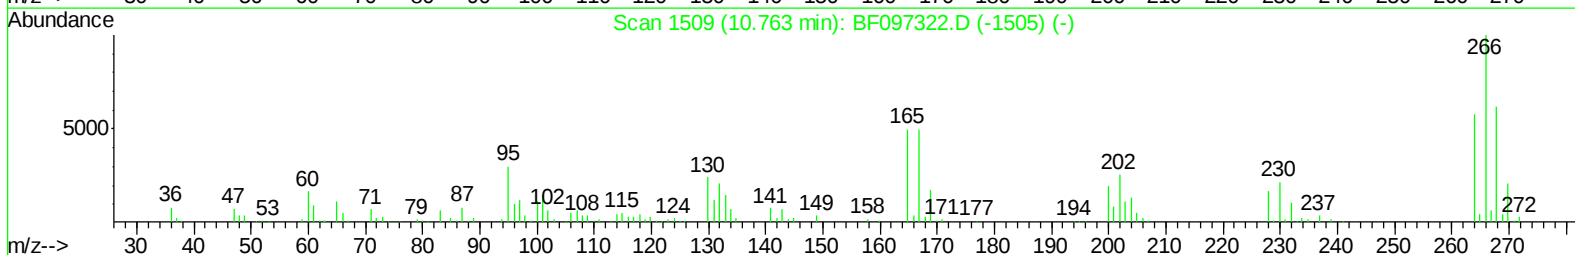
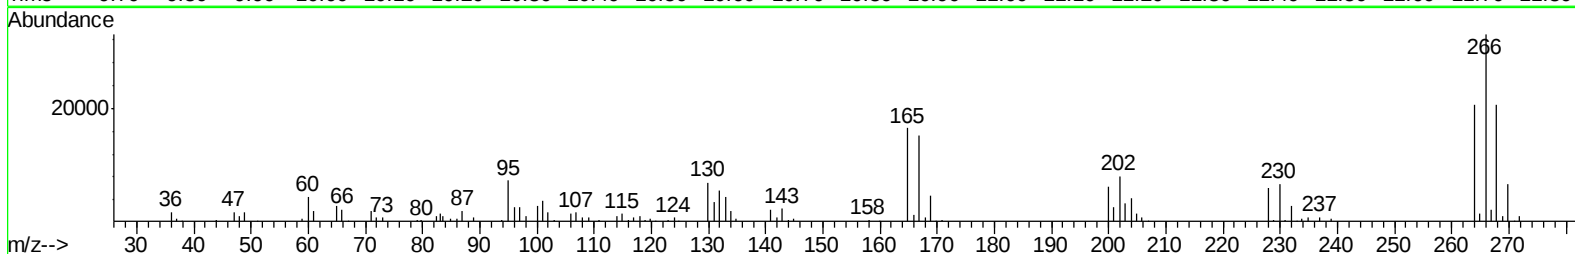


Data Path : Z:\HPCHEM1\BNA_F\Data\BF080417\
Data File : BF097351.D
Acq On : 4 Aug 2017 12:13
Operator : SJ/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Aug 07 17:59:03 2017
Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF072517.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Aug 07 16:02:51 2017
Response via : Initial Calibration

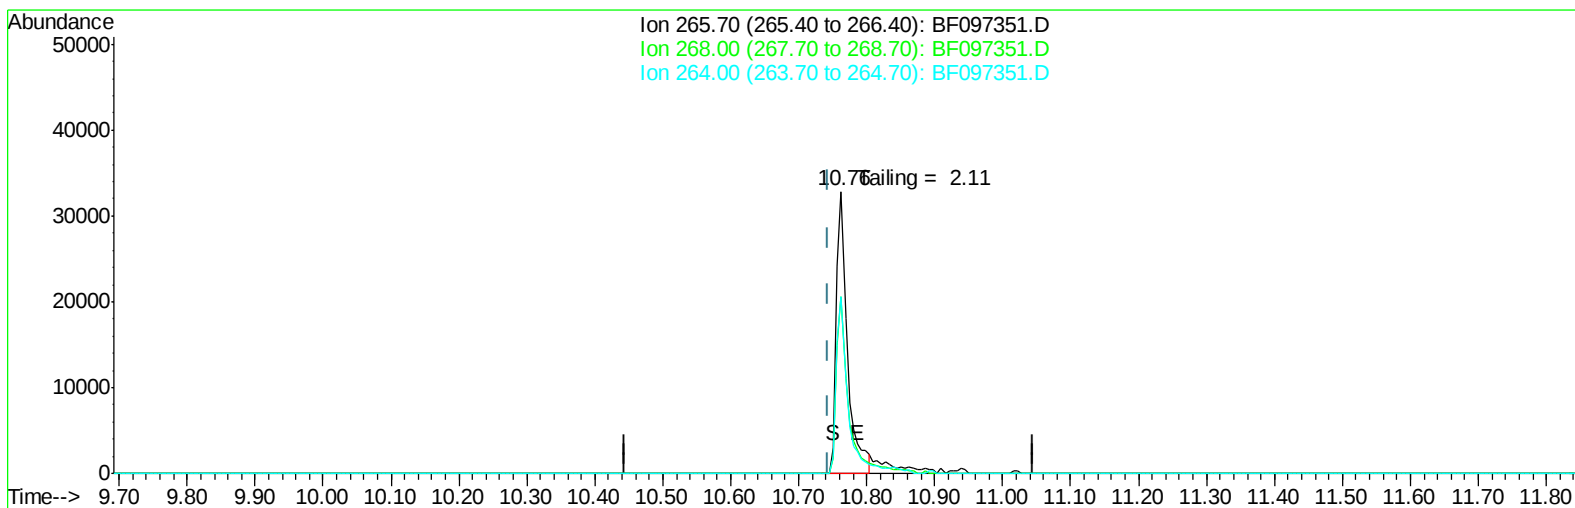

TIC: BF097351.D

(69) Pentachlorophenol (C)




10.763min (+0.018) 0.00ng

response 38882

Ion	Exp%	Act%
265.70	100	100
268.00	63.90	62.91
264.00	64.60	62.89
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA_F\Data\BF080417\
Data File : BF097351.D
Acq On : 4 Aug 2017 12:13
Operator : SJ/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Aug 07 17:59:03 2017
Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF072517.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Aug 07 16:02:51 2017
Response via : Initial Calibration

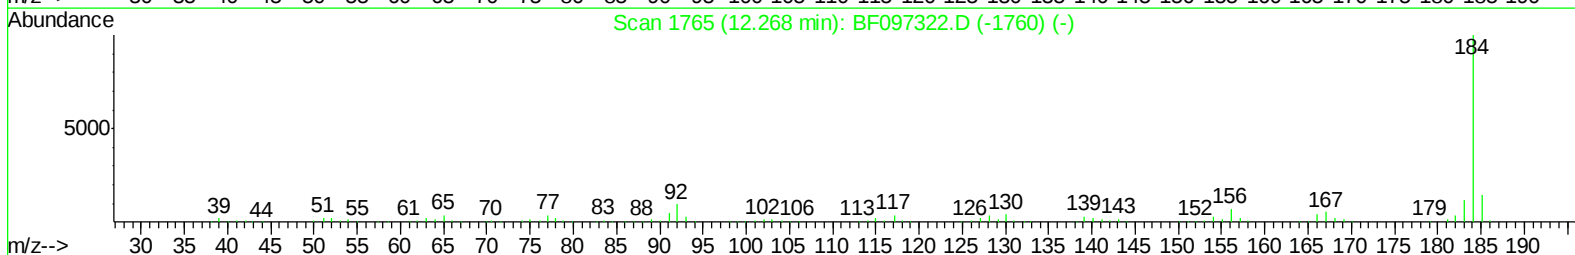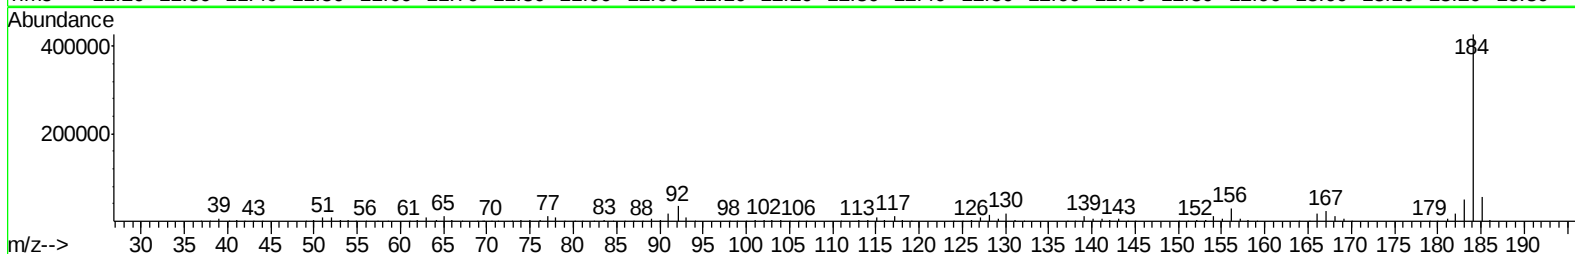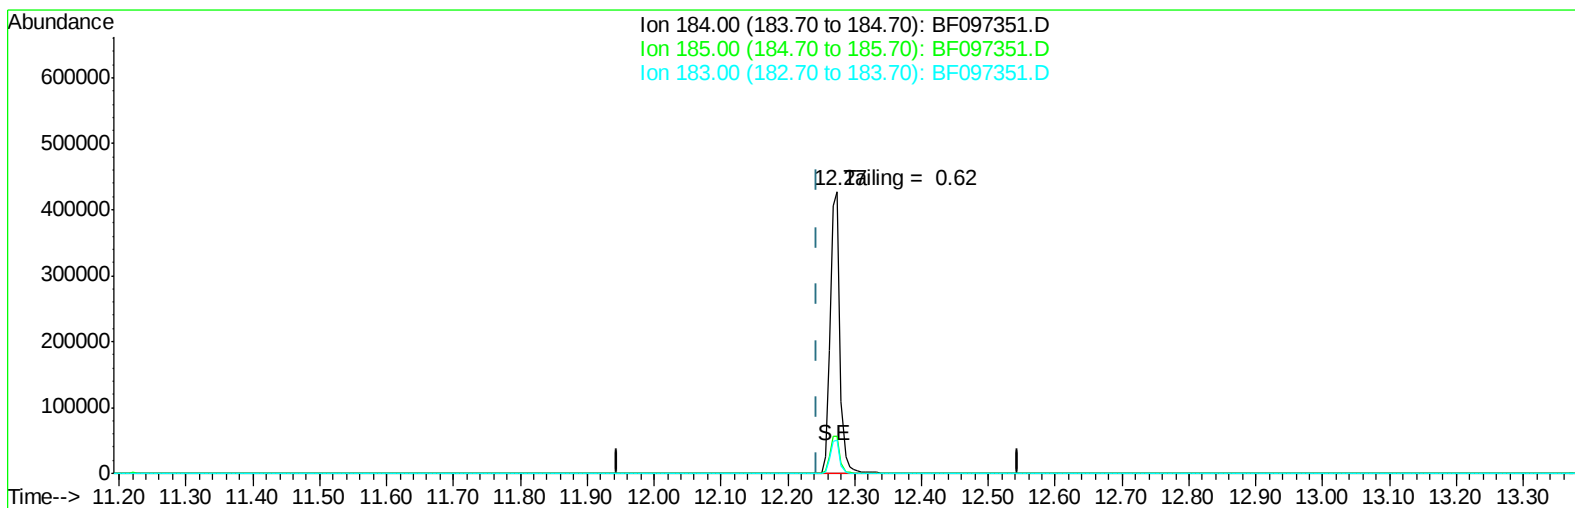

TIC: BF097351.D

(76) Benzidine

12.274min (+0.029) 0.00ng

response 428698

Ion	Exp%	Act%
184.00	100	100
185.00	19.40	13.25#
183.00	12.20	11.77
0.00	0.00	0.00