
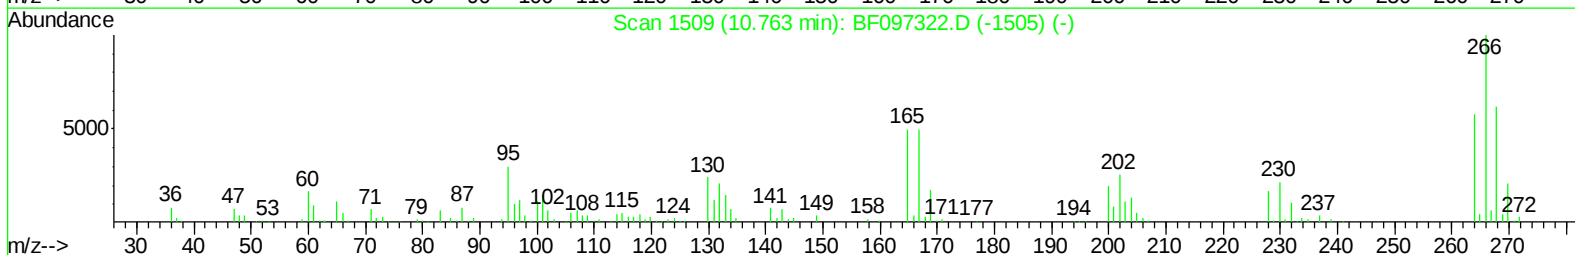
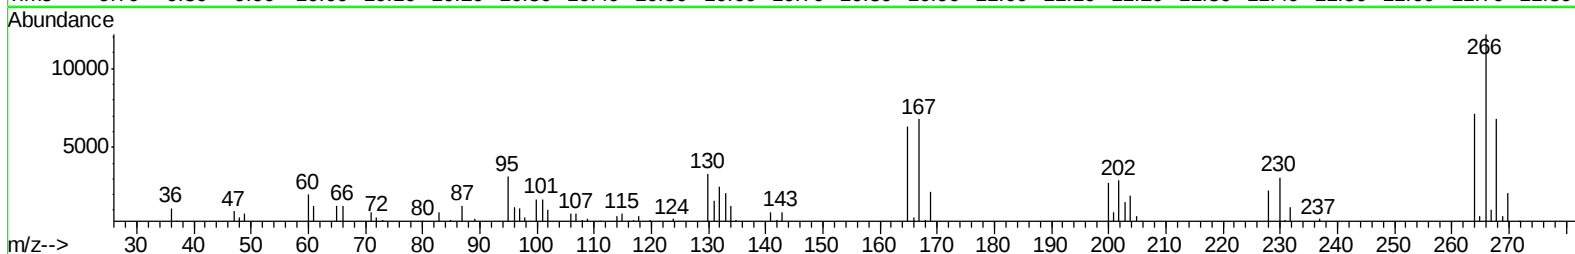


Data Path : Z:\HPCHEM1\BNA_F\Data\BF080417\
Data File : BF097377.D
Acq On : 5 Aug 2017 1:44
Operator : SJ/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Aug 07 18:01:25 2017
Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF072517.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Aug 07 16:02:51 2017
Response via : Initial Calibration

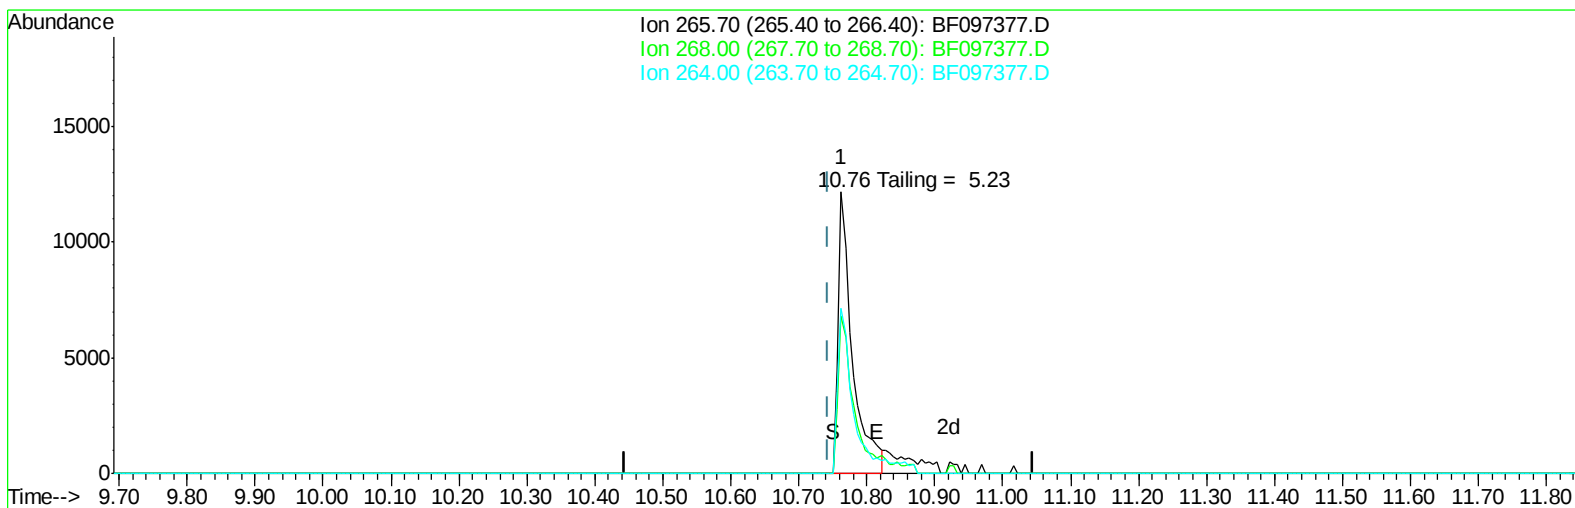

TIC: BF097377.D

(69) Pentachlorophenol (C)




10.763min (+0.018) 0.00ng

response 18344

Ion	Exp%	Act%
265.70	100	100
268.00	63.90	55.95
264.00	64.60	58.76
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA_F\Data\BF080417\
Data File : BF097377.D
Acq On : 5 Aug 2017 1:44
Operator : SJ/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Aug 07 18:01:25 2017
Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF072517.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Aug 07 16:02:51 2017
Response via : Initial Calibration

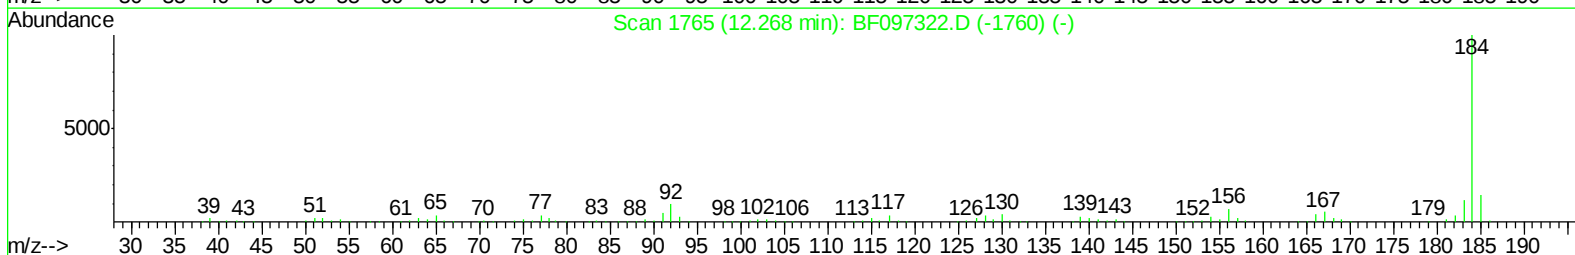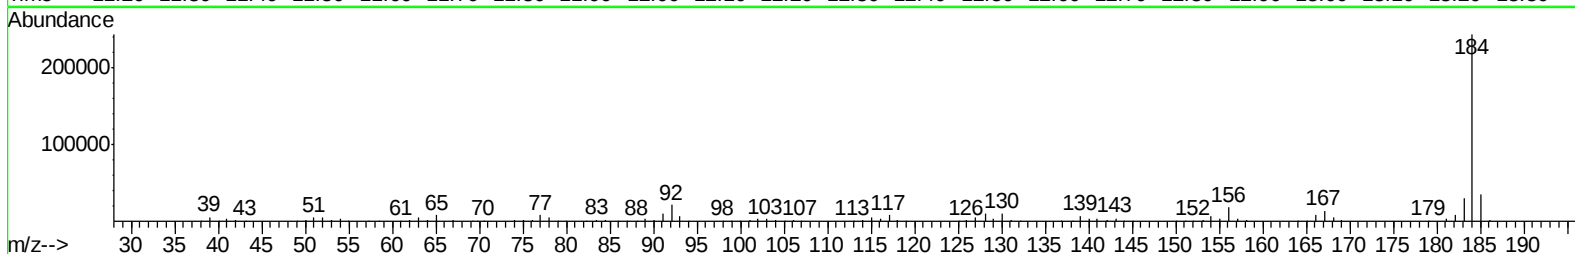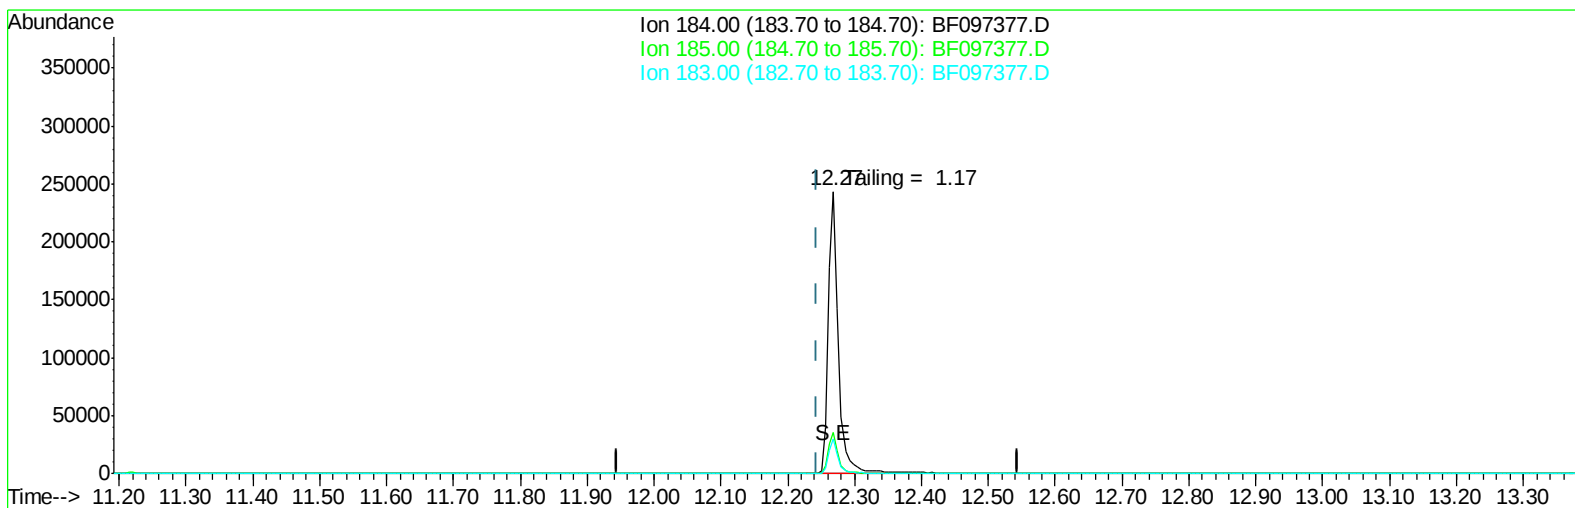

TIC: BF097377.D

(76) Benzidine

12.268min (+0.024) 62887.31ng

response 254343

Ion	Exp%	Act%
184.00	100	100
185.00	19.40	14.63#
183.00	12.20	12.50
0.00	0.00	0.00