


Data Path : Z:\HPCHEM1\BNA F\Data\BF080417\
Data File : BF097377.D
Acq On : 5 Aug 2017 1:44
Operator : SJ/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF072517.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Fri Aug 04 01:17:22 2017

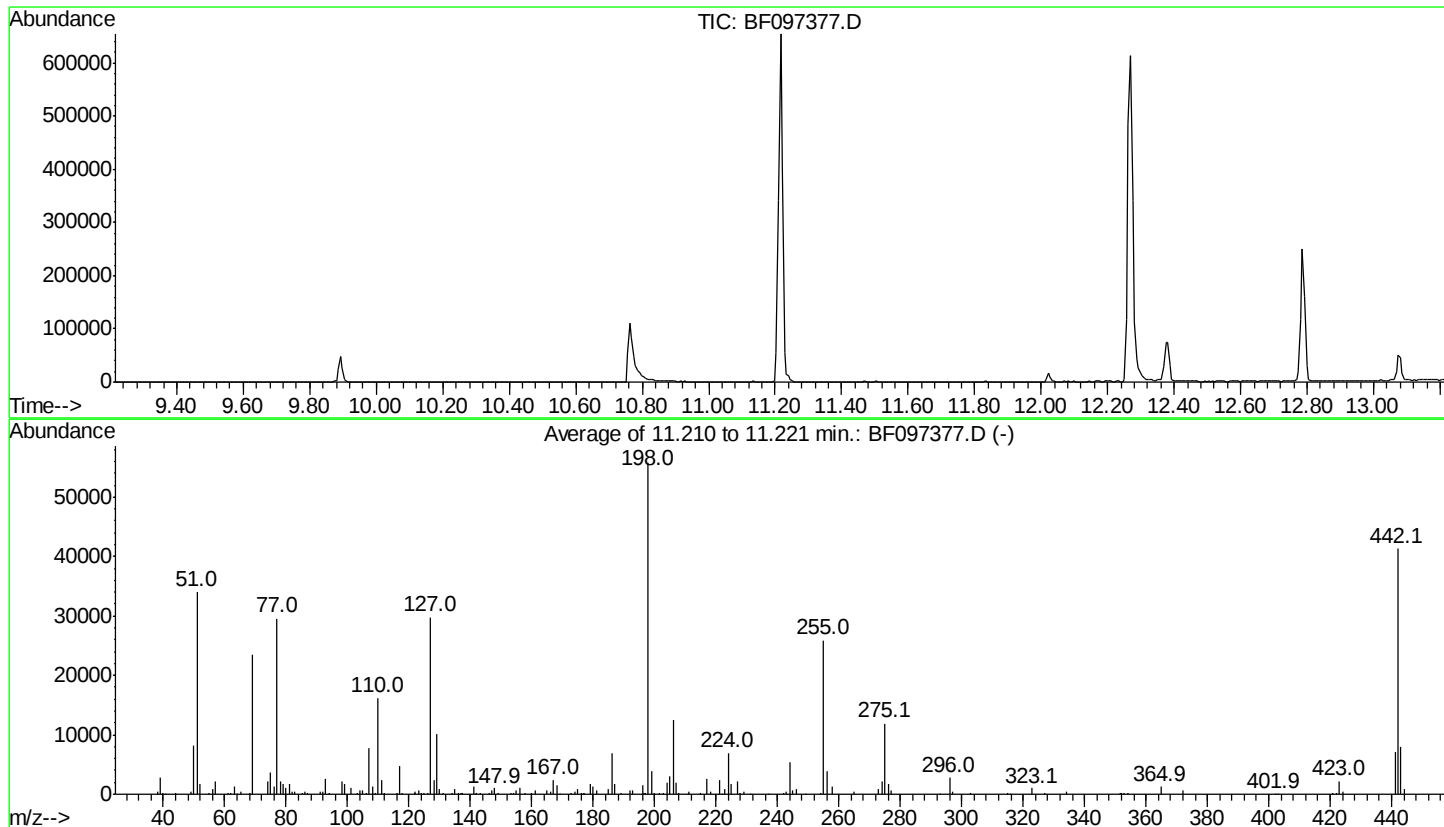

AutoFind: Scans 1602, 1603, 1604; Background Corrected with Scan 1597

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	61.1	34074	PASS
68	69	0.00	2	1.2	282	PASS
69	198	0.00	100	42.0	23415	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	53.3	29752	PASS
197	198	0.00	2	0.5	284	PASS
198	198	100	100	100.0	55789	PASS
199	198	5	9	7.1	3943	PASS
275	198	10	60	21.4	11921	PASS
365	198	1	100	2.2	1239	PASS
441	442	0.01	24	17.1	7049	PASS
442	198	50	100	74.1	41341	PASS
443	442	15	24	19.5	8048	PASS