
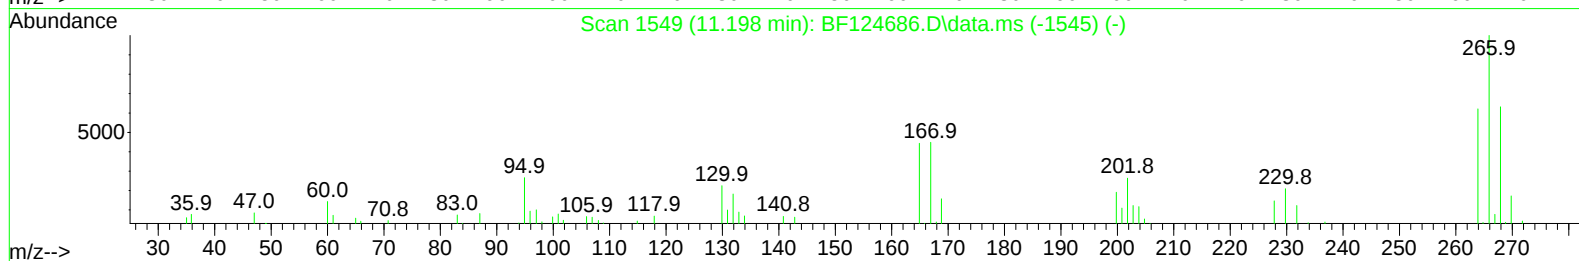
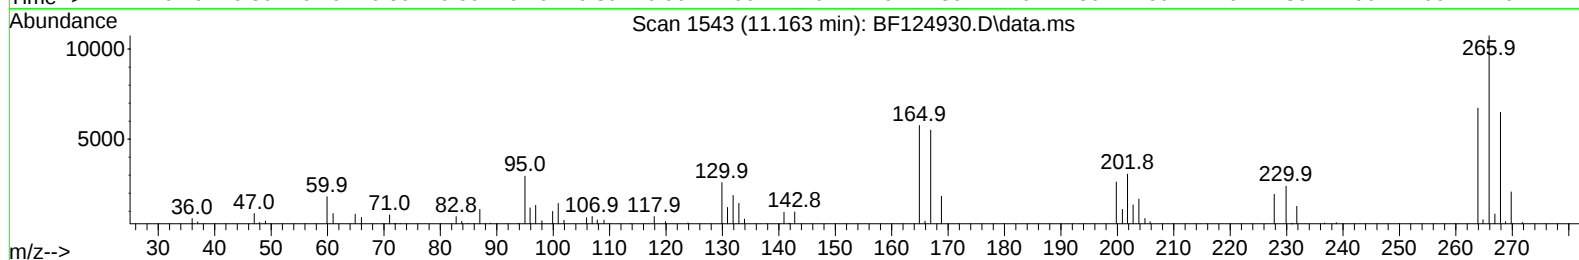


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF080421\
Data File : BF124930.D
Acq On : 4 Aug 2021 10:24
Operator : JU/CG
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Aug 04 12:20:40 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF080421.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Aug 04 12:10:25 2021
Response via : Initial Calibration

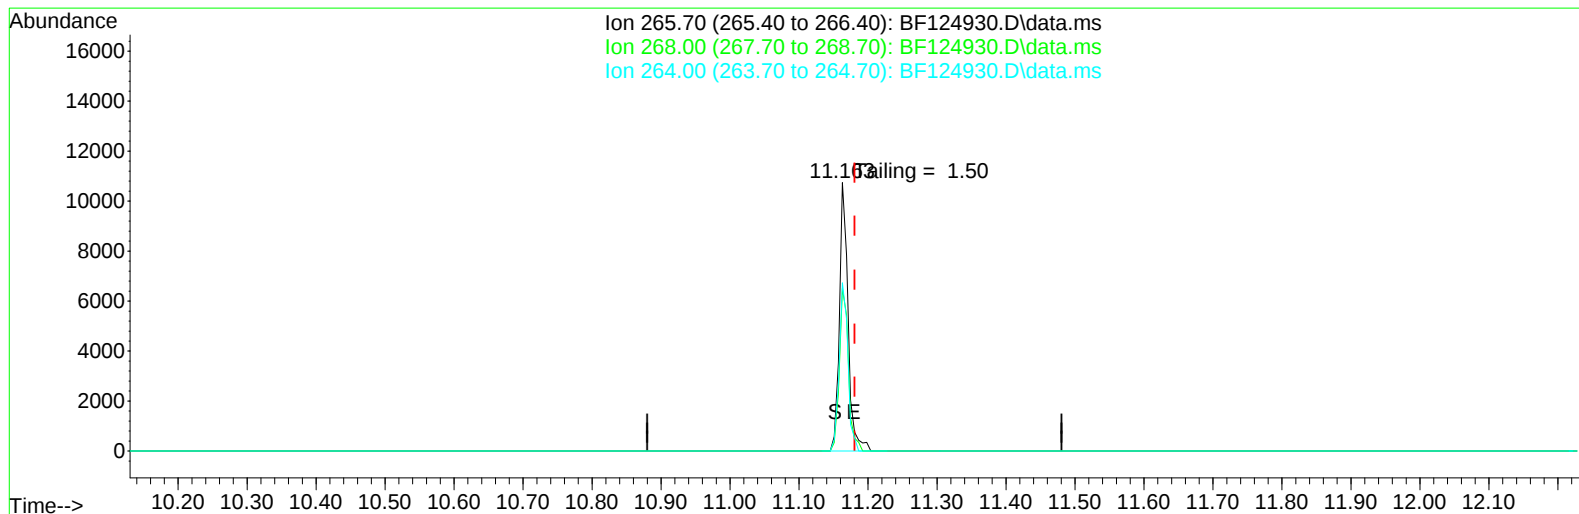

TIC: BF124930.D\data.ms

(70) Pentachlorophenol (C)




11.163min (-0.017) 0.00 ng

response 9377

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	61.10	60.49
264.00	69.90	62.65
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF080421\
 Data File : BF124930.D
 Acq On : 4 Aug 2021 10:24
 Operator : JU/CG
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Aug 04 12:20:40 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF080421.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Aug 04 12:10:25 2021
 Response via : Initial Calibration

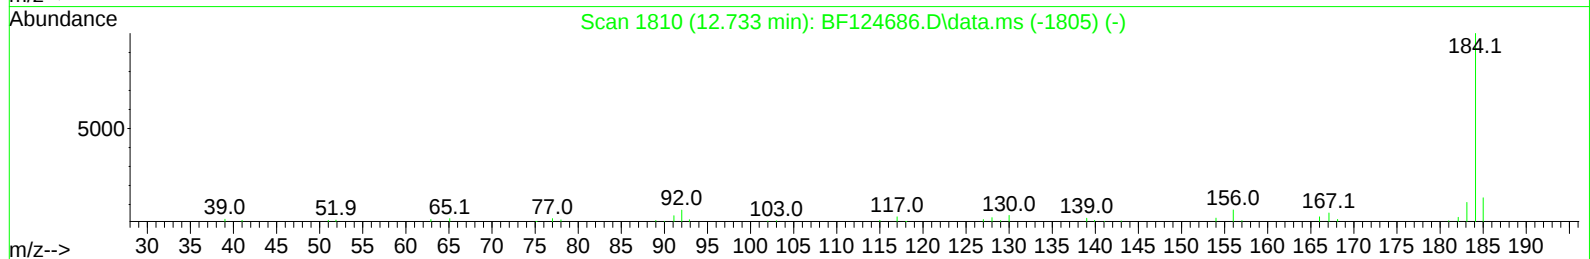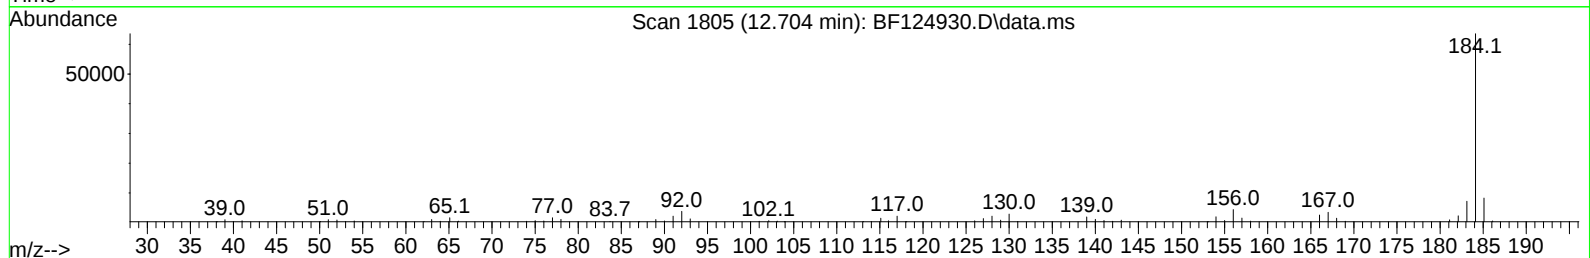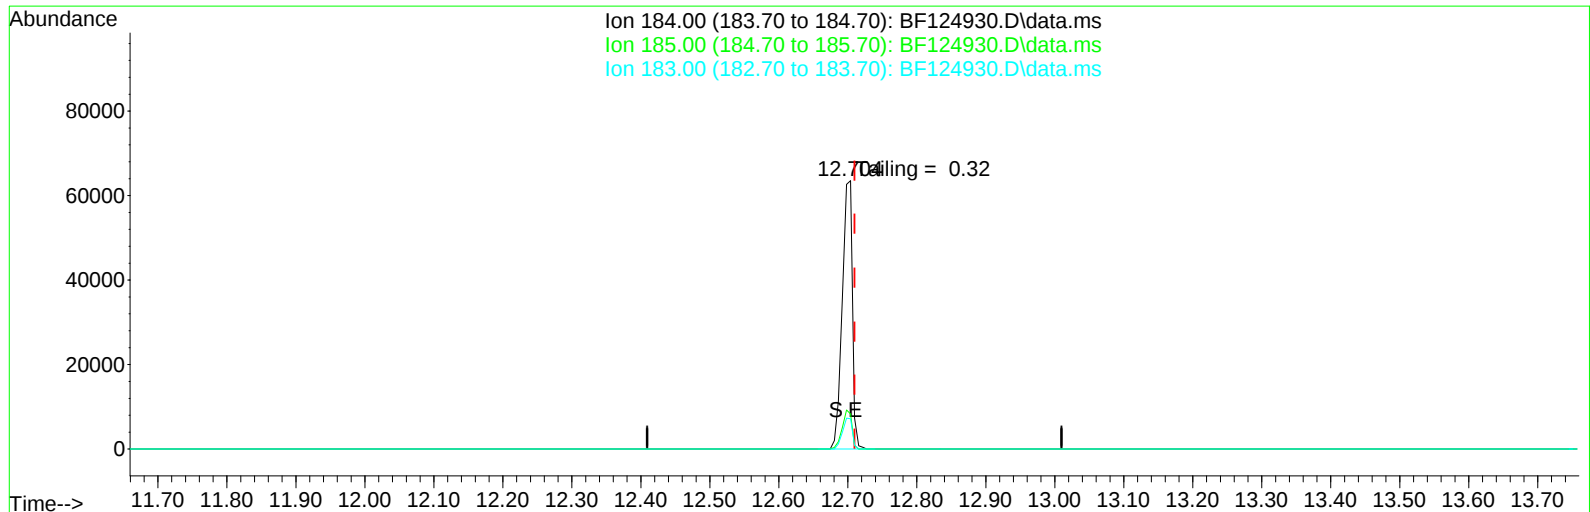

TIC: BF124930.D\data.ms

(77) Benzidine

12.704min (-0.006) 0.00 ng

response 64950

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	13.50	13.05
183.00	10.10	11.29
0.00	0.00	0.00