

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF080422\
 Data File : BF129565.D
 Acq On : 04 Aug 2022 11:22
 Operator : CG\JU
 Sample : PB146695BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 PB146695BL

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF072522.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BF129565.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.504	542	547	550	rBV	5012568	4591699	72.56%	12.323%
2	6.510	712	718	721	rBV	4447805	4663999	73.70%	12.517%
3	6.857	774	777	781	rBV	1192973	1032807	16.32%	2.772%
4	7.428	868	874	877	rBV	3014693	3105787	49.08%	8.335%
5	8.145	991	996	999	rBV	1512985	1435114	22.68%	3.852%
6	9.222	1173	1179	1182	rBV	5816456	5815210	91.89%	15.607%
7	9.898	1289	1294	1298	rBV	1993515	1695258	26.79%	4.550%
8	10.698	1424	1430	1433	rBV	3910335	3871543	61.18%	10.391%
9	11.392	1543	1548	1551	rBV	1882058	1737386	27.45%	4.663%
10	12.980	1812	1818	1821	rBV	6268720	6328467	100.00%	16.985%
11	13.768	1940	1952	1959	rBV9	15830	67019	1.06%	0.180%
12	14.033	1993	1997	2000	rBV	1659842	1410497	22.29%	3.786%
13	15.515	2243	2249	2254	rBV	922922	1201576	18.99%	3.225%
14	15.939	2317	2321	2326	rVB	72307	101913	1.61%	0.274%
15	16.451	2403	2408	2413	rVB	66053	113233	1.79%	0.304%
16	17.045	2505	2509	2514	rBV2	48140	88667	1.40%	0.238%




Sum of corrected areas: 37260175

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF080422\
Data File : BF129565.D
Acq On : 04 Aug 2022 11:22
Operator : CG\JU
Sample : PB146695BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB146695BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF072522.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

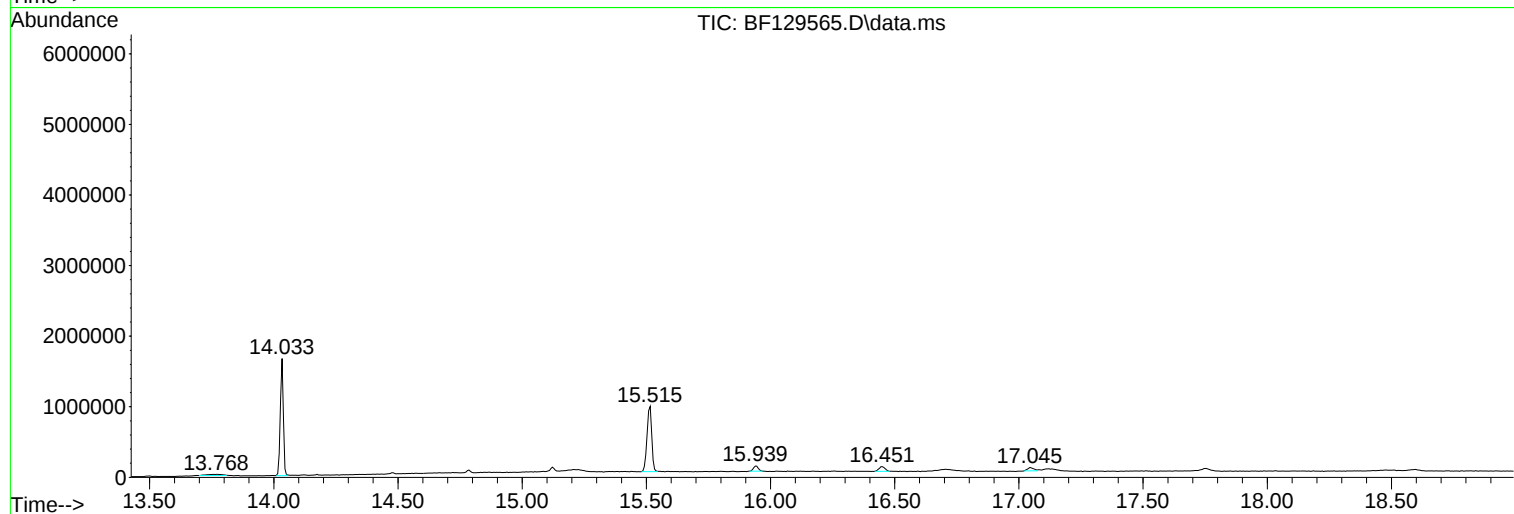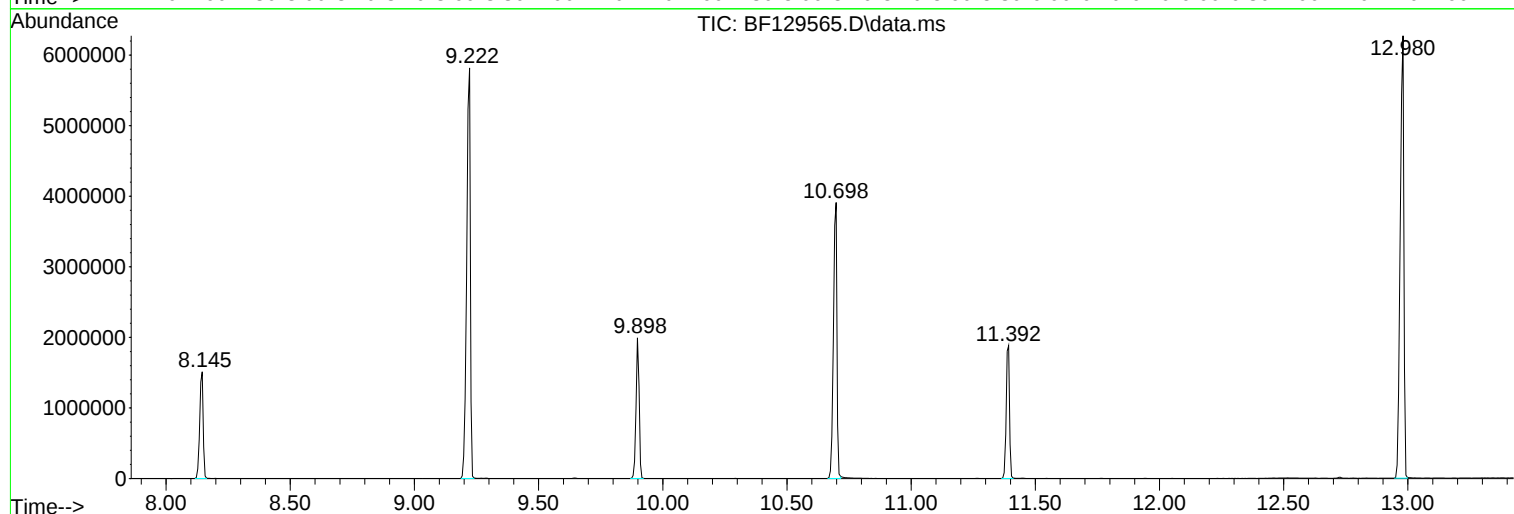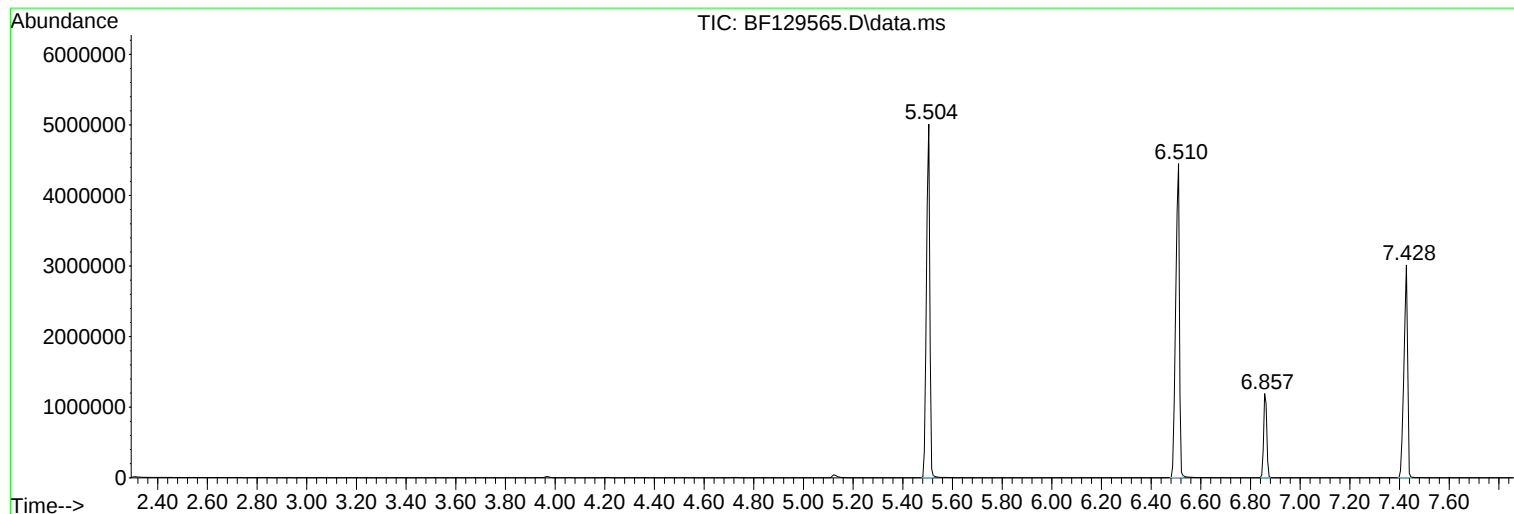

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF080422\
Data File : BF129565.D
Acq On : 04 Aug 2022 11:22
Operator : CG\JU
Sample : PB146695BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB146695BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF072522.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF080422\
Data File : BF129565.D
Acq On : 04 Aug 2022 11:22
Operator : CG\JU
Sample : PB146695BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB146695BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF072522.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------