
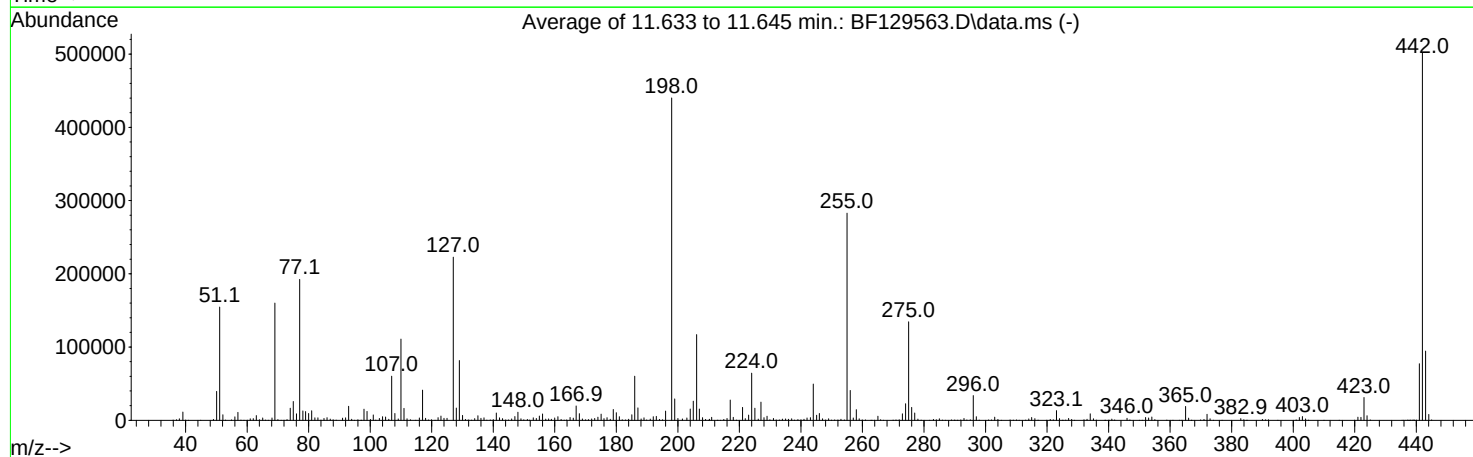


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF080422\
 Data File : BF129563.D
 Acq On : 04 Aug 2022 10:19
 Operator : CG\JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF072522.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri Aug 05 02:05:37 2022

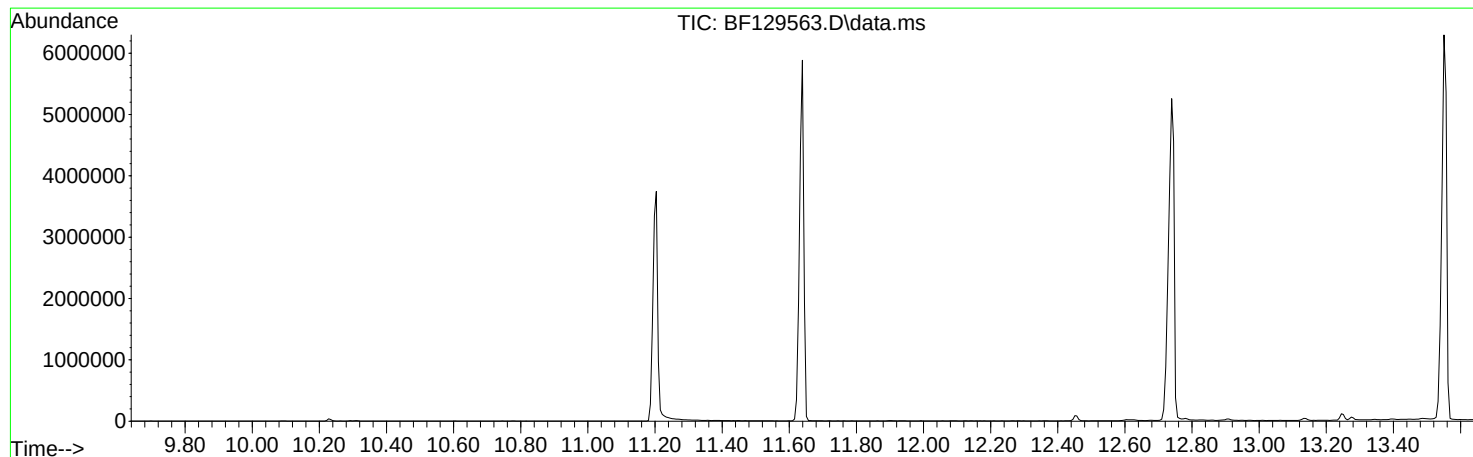




AutoFind: Scans 1589, 1590, 1591; Background Corrected with Scan 1582

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	35.1	154517	PASS
68	69	0.00	2	1.9	3109	PASS
69	198	0.00	100	36.4	160069	PASS
70	69	0.00	2	0.6	948	PASS
127	198	10	80	50.6	222677	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	440128	PASS
199	198	5	9	6.6	29254	PASS
275	198	10	60	30.5	134445	PASS
365	198	1	100	4.3	18850	PASS
441	198	0.01	100	17.6	77365	PASS
442	442	50	100	100.0	502293	PASS
443	442	15	24	18.8	94528	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF080422\
 Data File : BF129563.D
 Acq On : 04 Aug 2022 10:19
 Operator : CG\JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Quant Time: Aug 05 06:35:23 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF072522.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Aug 05 02:05:37 2022
 Response via : Initial Calibration

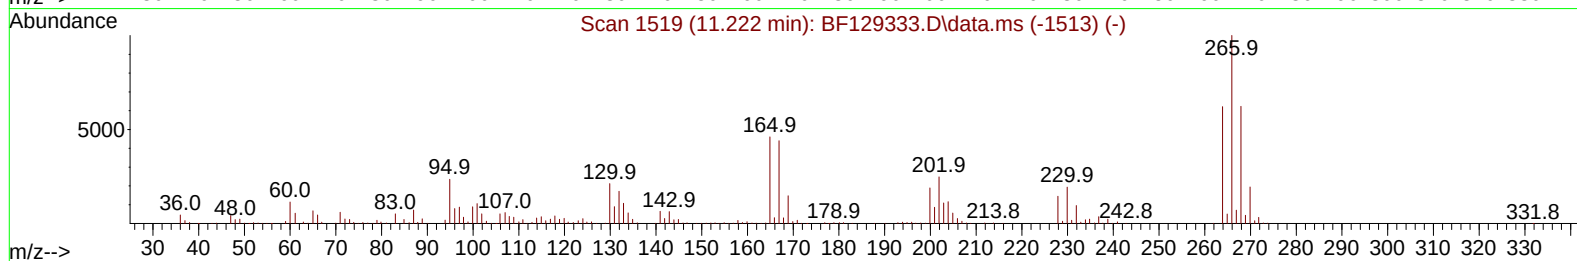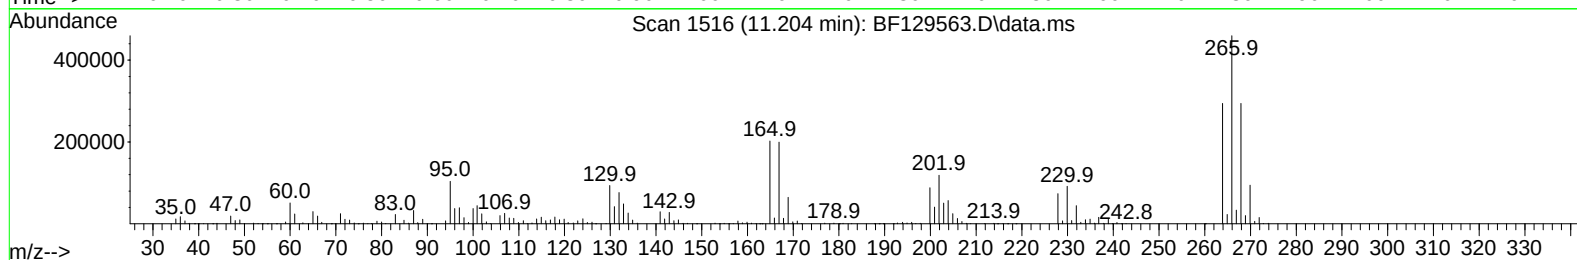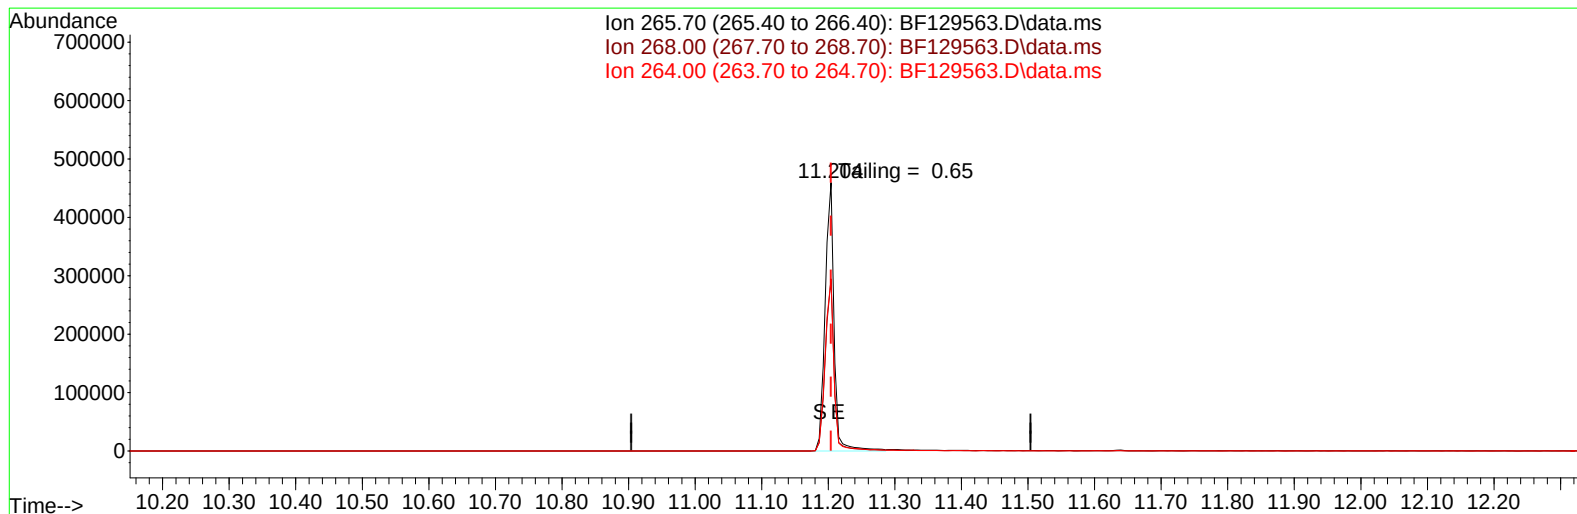

TIC: BF129563.D\data.ms

(70) Pentachlorophenol (C)

11.204min (-0.000) 173289.39 ng




response 437039

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.70	64.01
264.00	61.80	64.03
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF080422\
Data File : BF129563.D
Acq On : 04 Aug 2022 10:19
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Aug 05 06:35:23 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF072522.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Aug 05 02:05:37 2022
Response via : Initial Calibration

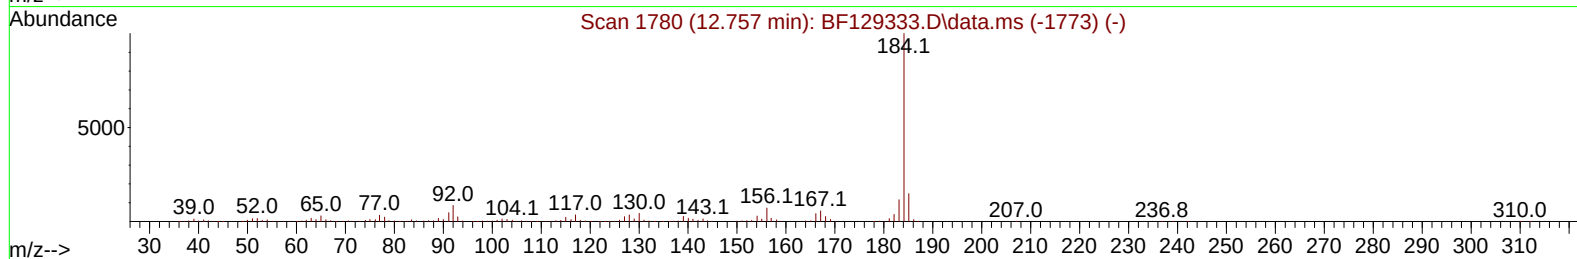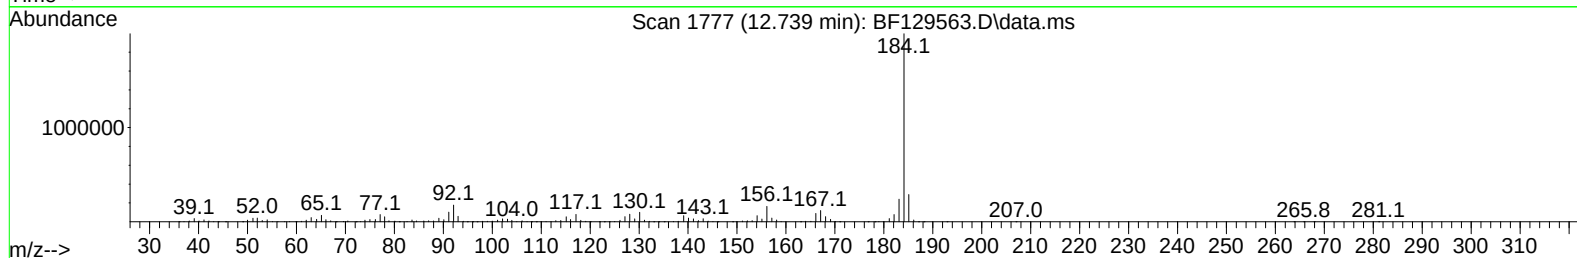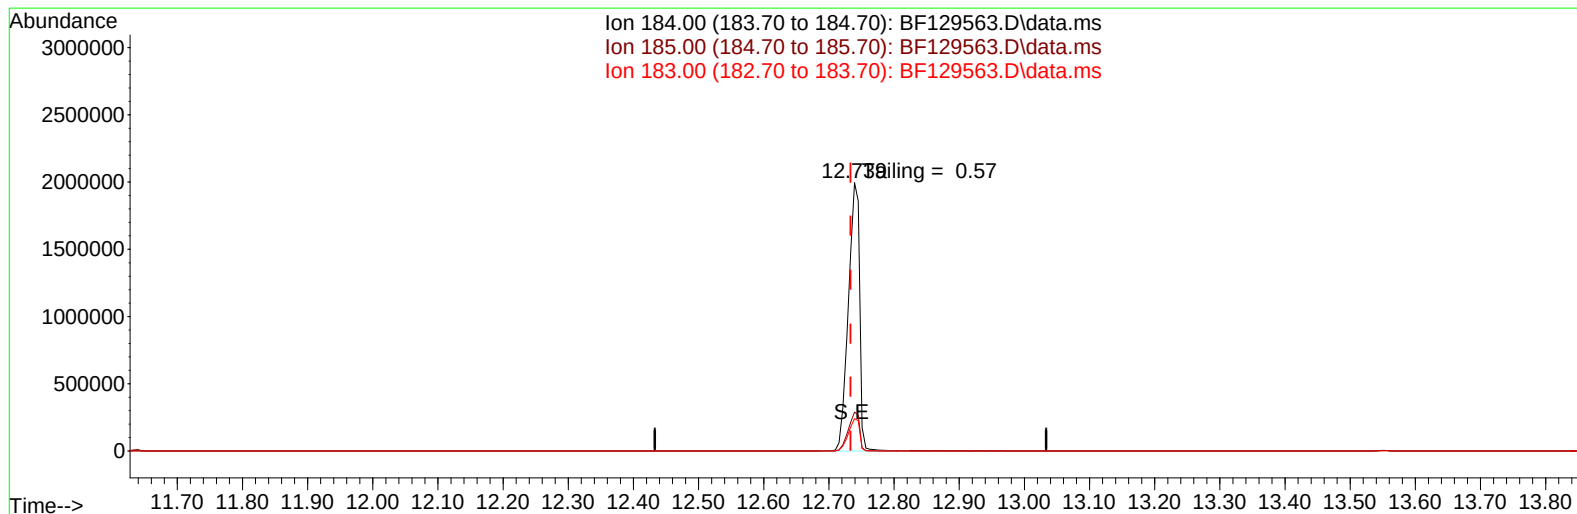

TIC: BF129563.D\data.ms

(77) Benzidine

12.739min (+ 0.006) 133674.87 ng

response 2422592

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.90	14.51
183.00	11.60	12.03
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
8/4/2022	BNA_F	<u>BF129563.D</u>
Compound Name	Response	Retention Time
DDT	1197642	13.551
DDD	25689	13.245
DDE	3348	12.91
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
29037	1226679	2.37

Instrument :
BNA_F
ClientSampleId :
DFTPP