
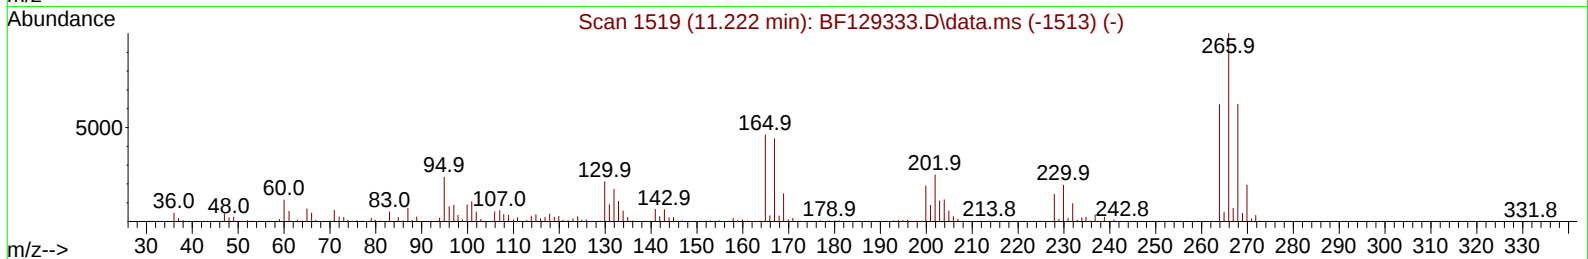
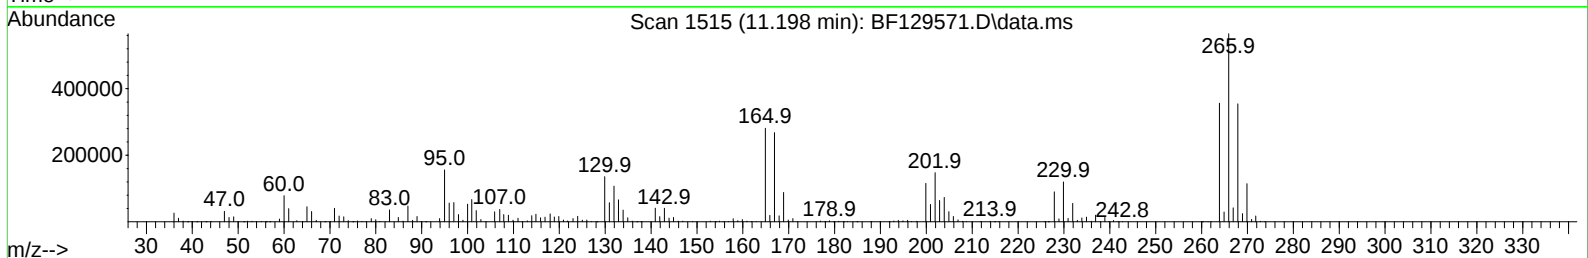


Data Path : Z:\svoasrv\HPCHEM1\BNA\_F\Data\BF080422\  
Data File : BF129571.D  
Acq On : 04 Aug 2022 15:47  
Operator : CG\JU  
Sample : DFTPP  
Misc :  
ALS Vial : 1 Sample Multiplier: 1

Instrument :  
BNA\_F  
ClientSampleId :  
DFTPP

Quant Time: Aug 05 06:36:41 2022  
Quant Method : Z:\svoasrv\HPCHEM1\BNA\_F\Methods\8270-BF072522.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Fri Aug 05 02:05:37 2022  
Response via : Initial Calibration

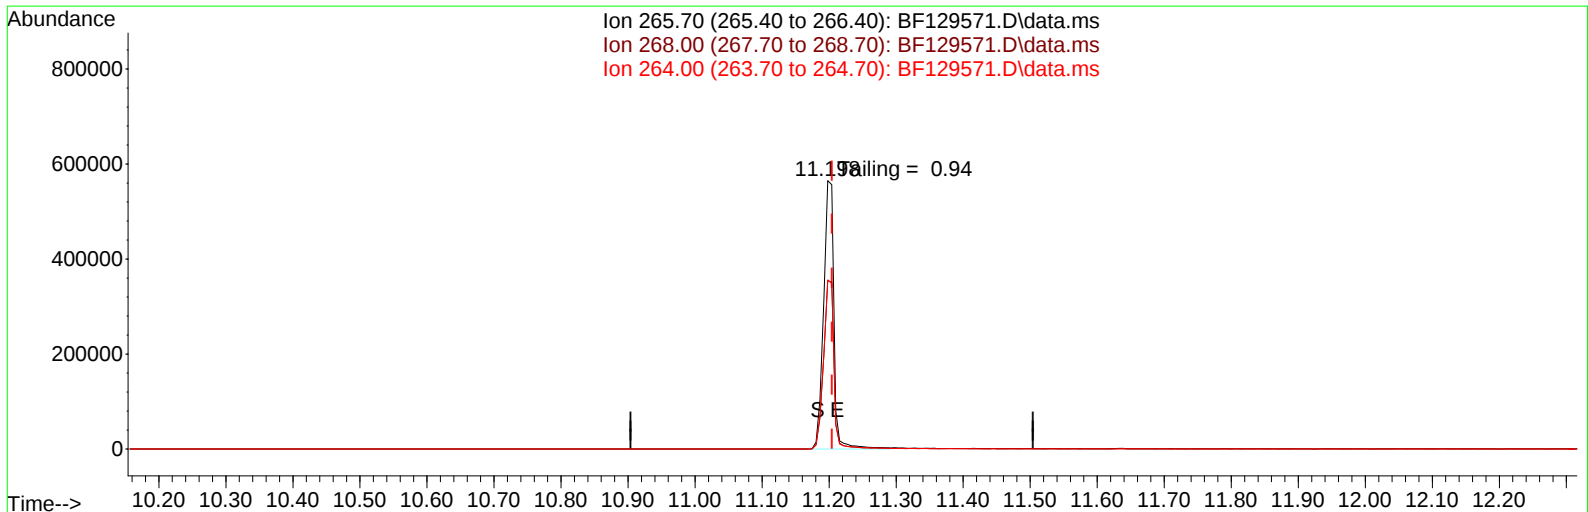

TIC: BF129571.D\data.ms

**(70) Pentachlorophenol (C)**

**11.198min (-0.006) 190640.32 ng**




**response 609913**

| Ion    | Exp%   | Act%   |
|--------|--------|--------|
| 265.70 | 100.00 | 100.00 |
| 268.00 | 63.70  | 62.77  |
| 264.00 | 61.80  | 63.04  |
| 0.00   | 0.00   | 0.00   |

Data Path : Z:\svoasrv\HPCHEM1\BNA\_F\Data\BF080422\  
Data File : BF129571.D  
Acq On : 04 Aug 2022 15:47  
Operator : CG\JU  
Sample : DFTPP  
Misc :  
ALS Vial : 1 Sample Multiplier: 1

Instrument :  
BNA\_F  
ClientSampleId :  
DFTPP

Quant Time: Aug 05 06:36:41 2022  
Quant Method : Z:\svoasrv\HPCHEM1\BNA\_F\Methods\8270-BF072522.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Fri Aug 05 02:05:37 2022  
Response via : Initial Calibration

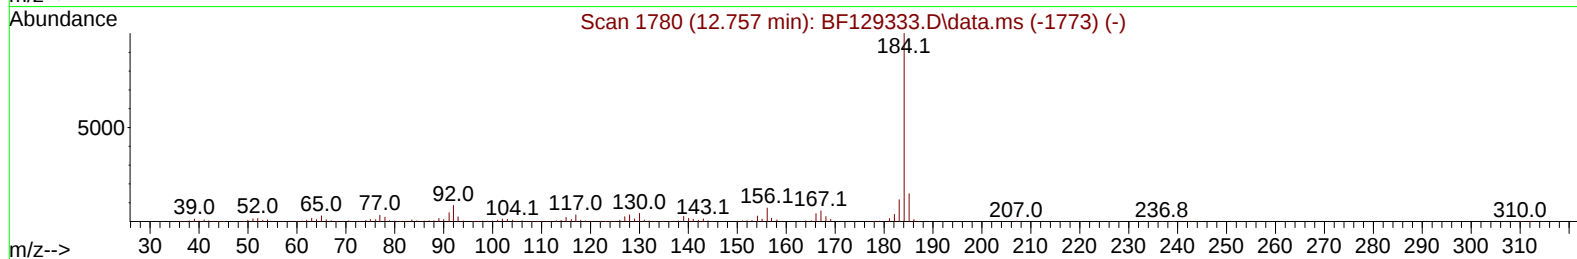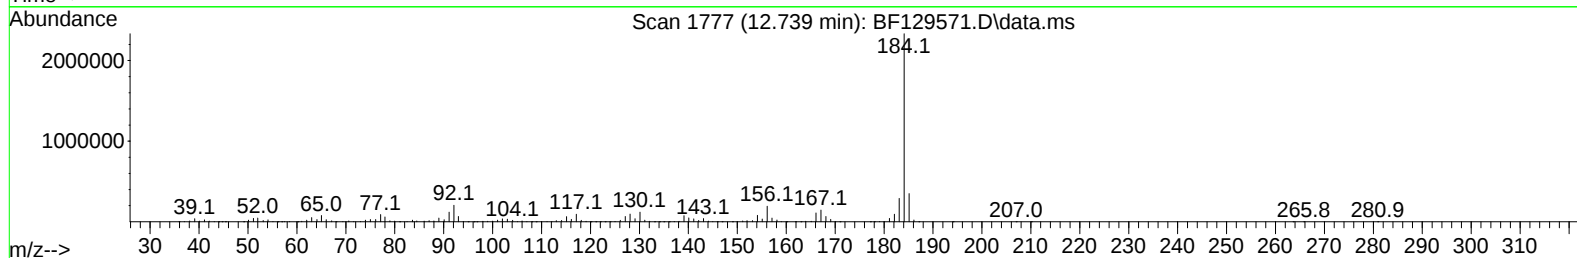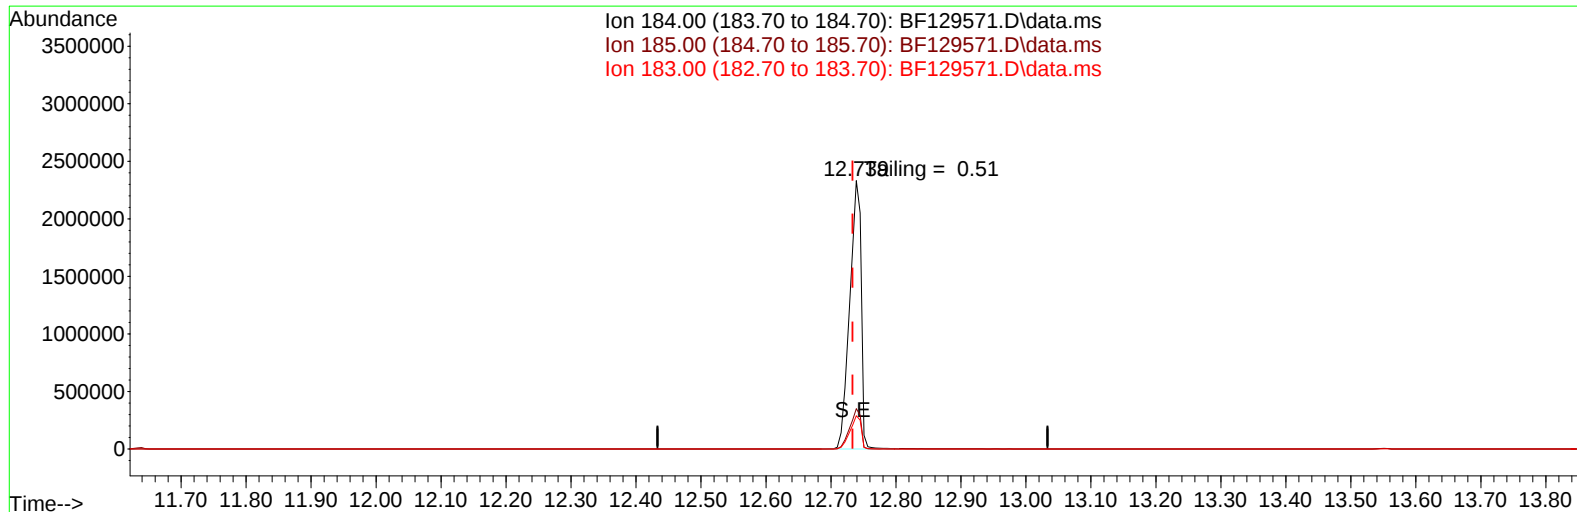

TIC: BF129571.D\data.ms

**(77) Benzidine**

**12.739min (+ 0.006) 84535.69 ng**

**response 2881911**



| Ion    | Exp%   | Act%   |
|--------|--------|--------|
| 184.00 | 100.00 | 100.00 |
| 185.00 | 14.90  | 15.03  |
| 183.00 | 11.60  | 12.43  |
| 0.00   | 0.00   | 0.00   |

Data Path : Z:\svoasrv\HPCHEM1\BNA\_F\Data\BF080422\  
 Data File : BF129571.D  
 Acq On : 04 Aug 2022 15:47  
 Operator : CG\JU  
 Sample : DFTPP  
 Misc :  
 ALS Vial : 1 Sample Multiplier: 1

Instrument :  
 BNA\_F  
 ClientSampleId :  
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA\_F\Methods\8270-BF072522.M  
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
 Last Update : Fri Aug 05 02:05:37 2022

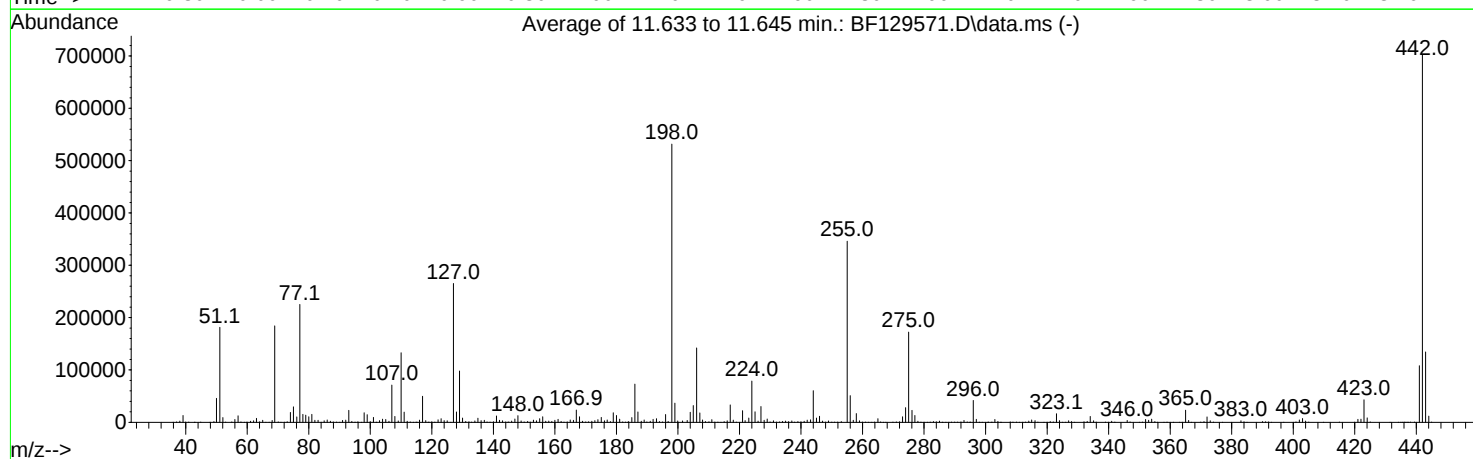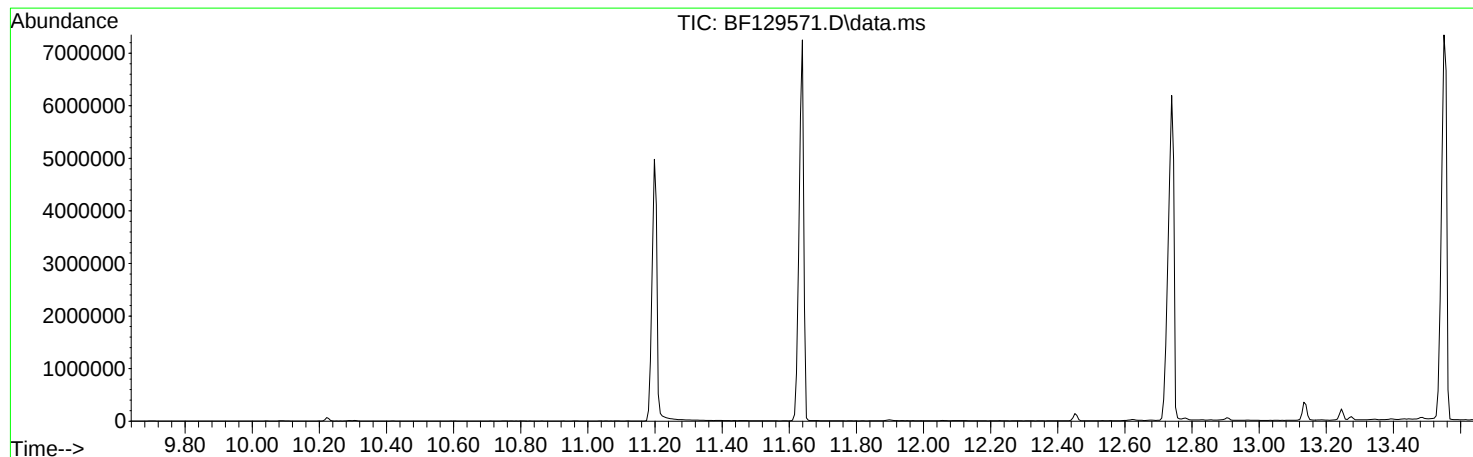

AutoFind: Scans 1589, 1590, 1591; Background Corrected with Scan 1582

| Target<br>Mass | Rel. to<br>Mass | Lower<br>Limit% | Upper<br>Limit% | Rel.<br>Abn% | Raw<br>Abn | Result<br>Pass/Fail |
|----------------|-----------------|-----------------|-----------------|--------------|------------|---------------------|
| 51             | 198             | 10              | 80              | 34.2         | 181611     | PASS                |
| 68             | 69              | 0.00            | 2               | 1.9          | 3570       | PASS                |
| 69             | 198             | 0.00            | 100             | 34.7         | 184411     | PASS                |
| 70             | 69              | 0.00            | 2               | 0.5          | 857        | PASS                |
| 127            | 198             | 10              | 80              | 49.9         | 265152     | PASS                |
| 197            | 198             | 0.00            | 2               | 0.3          | 1733       | PASS                |
| 198            | 198             | 100             | 100             | 100.0        | 531584     | PASS                |
| 199            | 198             | 5               | 9               | 6.9          | 36702      | PASS                |
| 275            | 198             | 10              | 60              | 32.4         | 172376     | PASS                |
| 365            | 198             | 1               | 100             | 4.3          | 23002      | PASS                |
| 441            | 198             | 0.01            | 100             | 20.3         | 108016     | PASS                |
| 442            | 442             | 50              | 100             | 100.0        | 702997     | PASS                |
| 443            | 442             | 15              | 24              | 19.1         | 134405     | PASS                |

### DDT Breakdown

| Date          | Instrument Name  | DFTPP Data File    |
|---------------|------------------|--------------------|
| 8/4/2022      | BNA_F            | <u>BF129571.D</u>  |
|               |                  |                    |
|               |                  |                    |
| Compound Name | Response         | Retention Time     |
|               |                  |                    |
| DDT           | 1517522          | 13.557             |
| DDD           | 43239            | 13.245             |
| DDE           | 4709             | 12.904             |
|               |                  |                    |
|               |                  |                    |
| SUM(DDD+DDE)  | SUM(DDT+DDD+DDE) | % Breakdown Of DDT |
|               |                  |                    |
| 47948         | 1565470          | 3.06               |
|               |                  |                    |

Instrument :  
BNA\_F  
ClientSampleId :  
DFTPP