
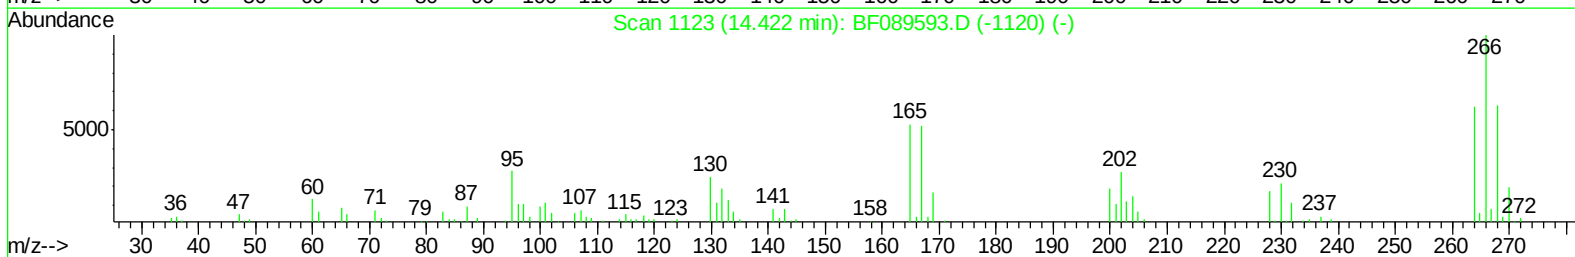
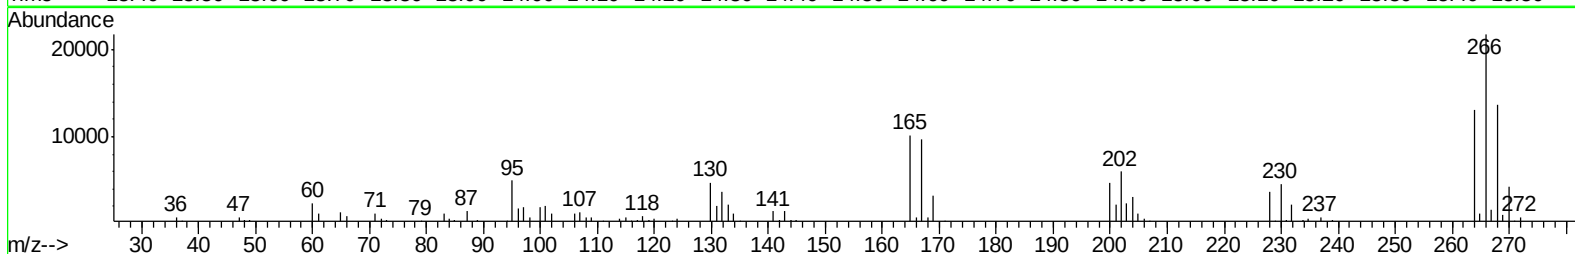


Data Path : Z:\HPCHEM1\BNA_F\DATA\BF080516\
Data File : BF089645.D
Acq On : 5 Aug 2016 23:53
Operator : UM/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Aug 06 06:39:31 2016
Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF080416.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Aug 05 01:39:23 2016
Response via : Initial Calibration

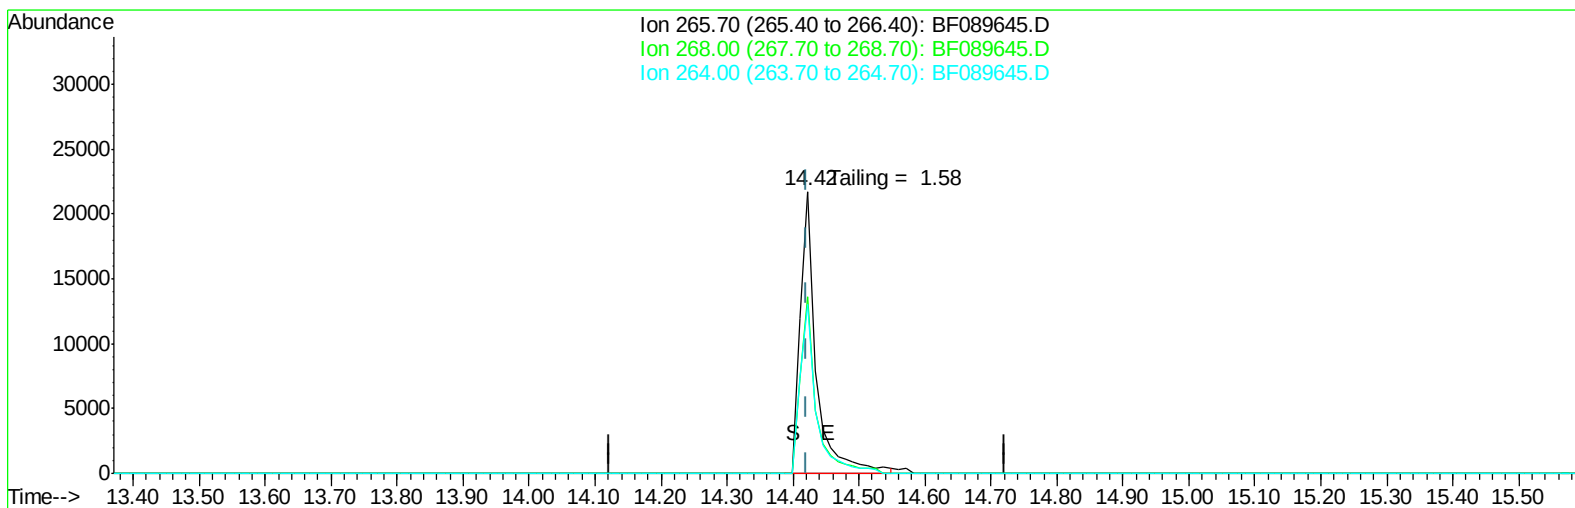

TIC: BF089645.D

(69) Pentachlorophenol (C)




14.422min (+0.000) 0.00ng

response 36585

Ion	Exp%	Act%
265.70	100	100
268.00	63.20	62.86
264.00	61.90	59.87
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF080516\
Data File : BF089645.D
Acq On : 5 Aug 2016 23:53
Operator : UM/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Aug 06 06:39:31 2016
Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF080416.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Aug 05 01:39:23 2016
Response via : Initial Calibration

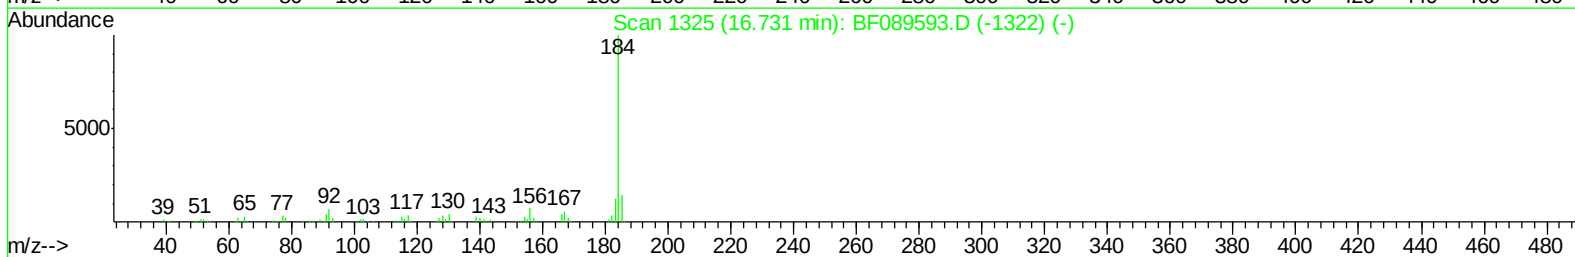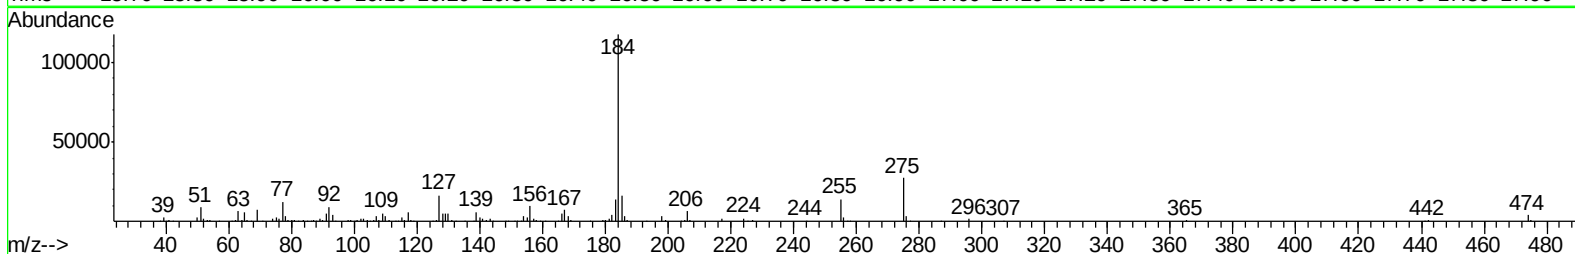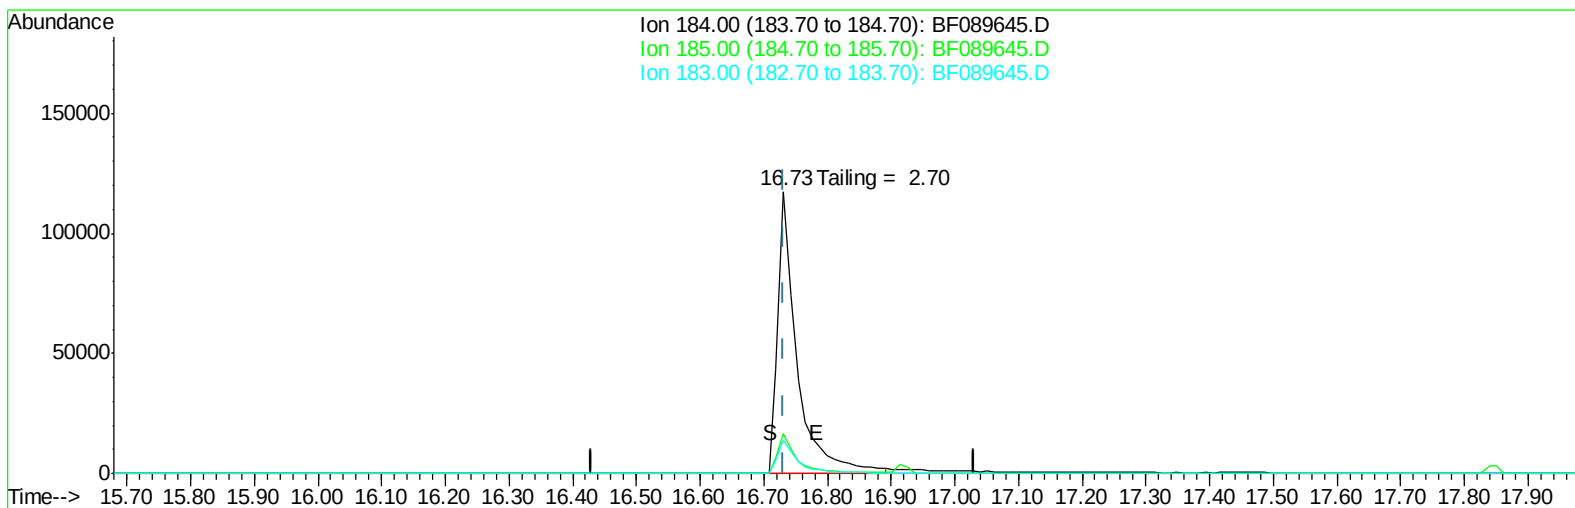

TIC: BF089645.D

(76) Benzidine

16.731min (-0.000) 0.00ng

response 251562

Ion	Exp%	Act%
184.00	100	100
185.00	14.40	14.14
183.00	12.30	11.83
0.00	0.00	0.00