


Data Path : Z:\HPCHEM1\BNA_F\DATA\BF080516\
 Data File : BF089623.D
 Acq On : 5 Aug 2016 10:53
 Operator : UM/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF080416.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri Aug 05 01:39:23 2016

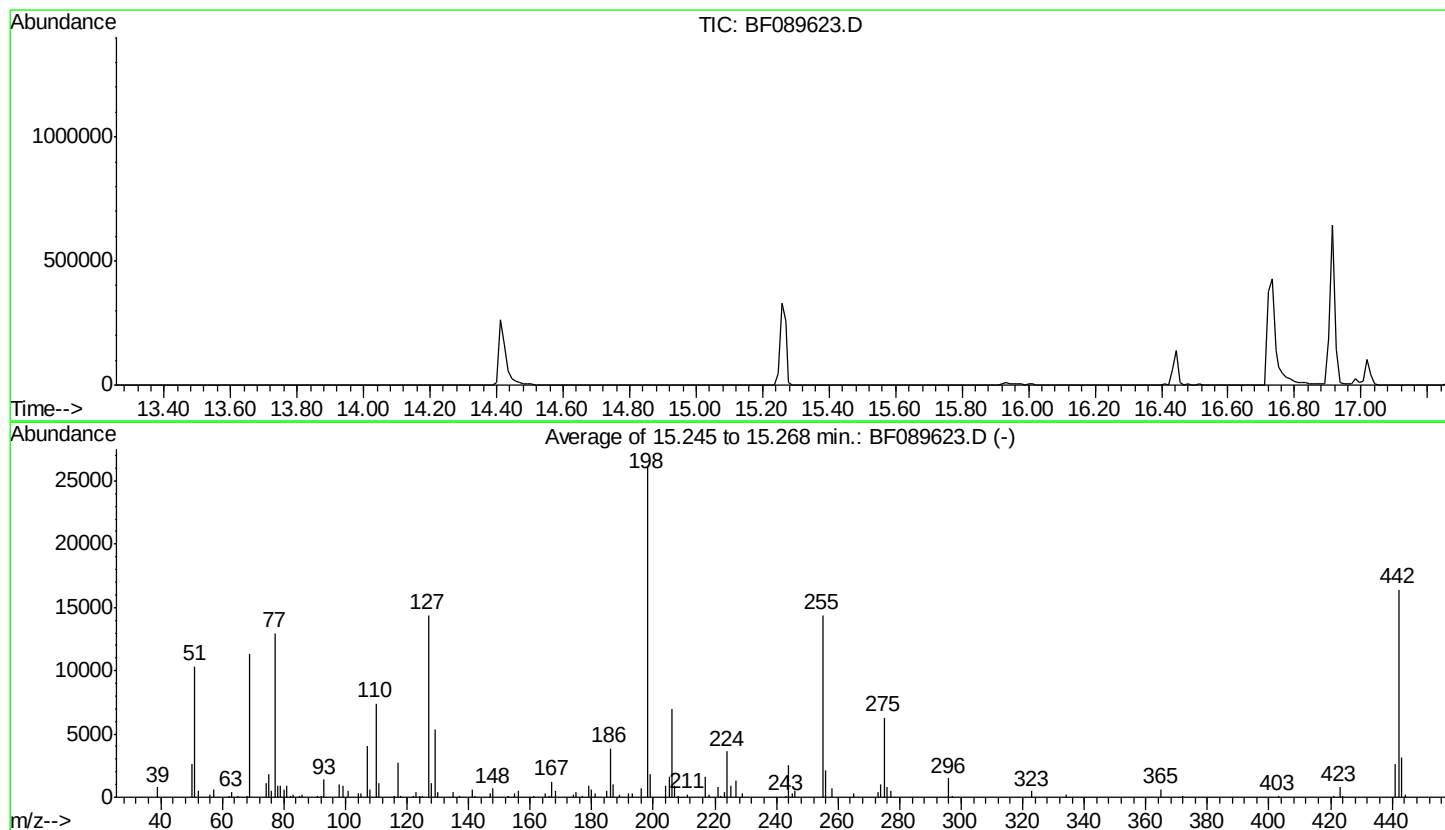

AutoFind: Scans 1195, 1196, 1197; Background Corrected with Scan 1192

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	39.5	10343	PASS
68	69	0.00	2	1.2	130	PASS
69	198	0.00	100	43.1	11291	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	54.9	14396	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	26205	PASS
199	198	5	9	6.9	1818	PASS
275	198	10	60	24.1	6310	PASS
365	198	1	100	2.3	610	PASS
441	442	0.01	24	16.0	2630	PASS
442	198	50	100	62.6	16393	PASS
443	442	15	24	19.4	3180	PASS