


Data Path : Z:\HPCHEM1\BNA_F\DATA\BF080516\
 Data File : BF089645.D
 Acq On : 5 Aug 2016 23:53
 Operator : UM/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF080416.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri Aug 05 01:39:23 2016

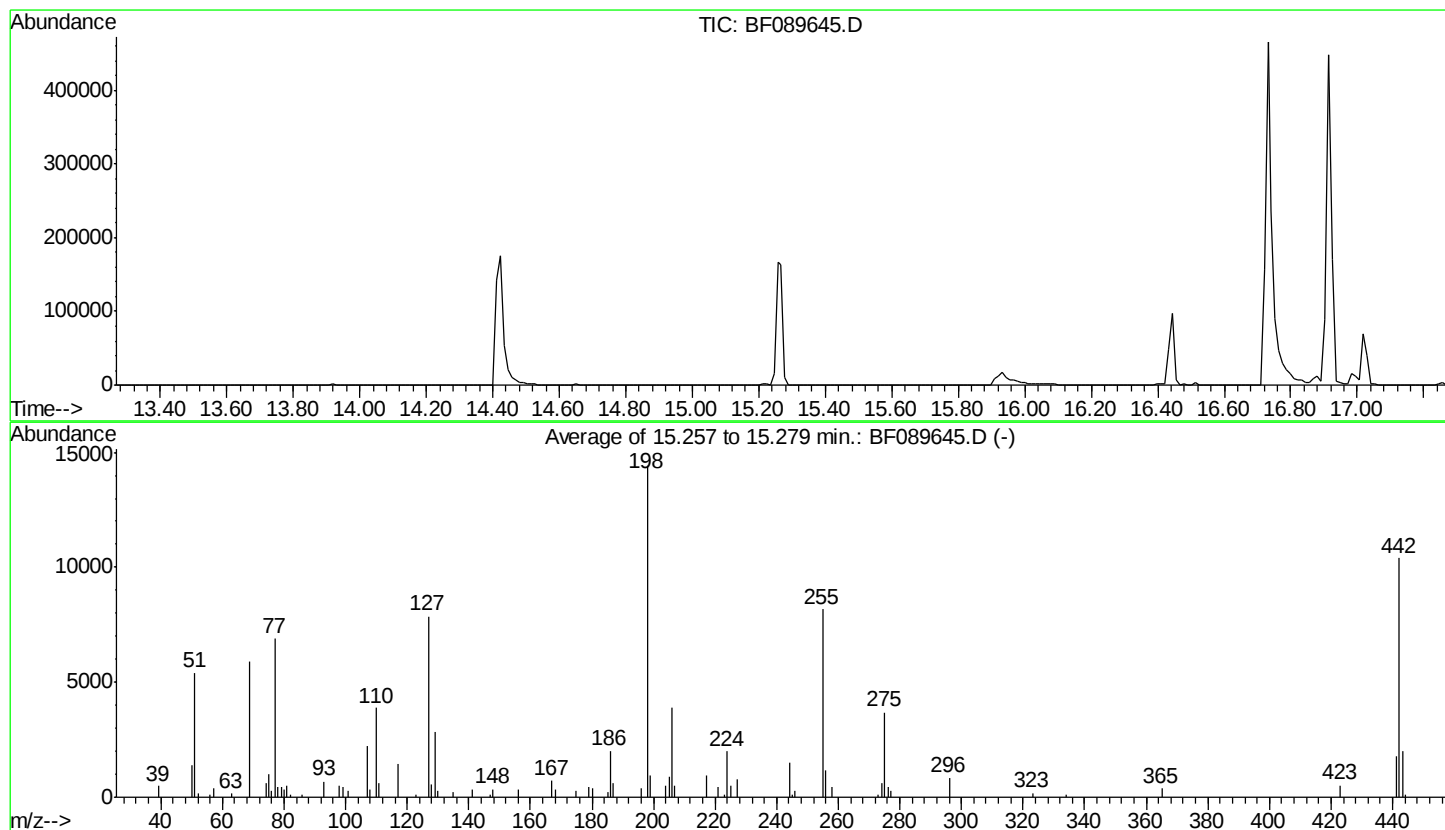

AutoFind: Scans 1196, 1197, 1198; Background Corrected with Scan 1192

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	37.6	5419	PASS
68	69	0.00	2	0.0	0	PASS
69	198	0.00	100	41.1	5920	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	54.6	7867	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	14421	PASS
199	198	5	9	6.7	971	PASS
275	198	10	60	25.6	3693	PASS
365	198	1	100	2.6	373	PASS
441	442	0.01	24	16.9	1762	PASS
442	198	50	100	72.1	10401	PASS
443	442	15	24	19.4	2019	PASS