
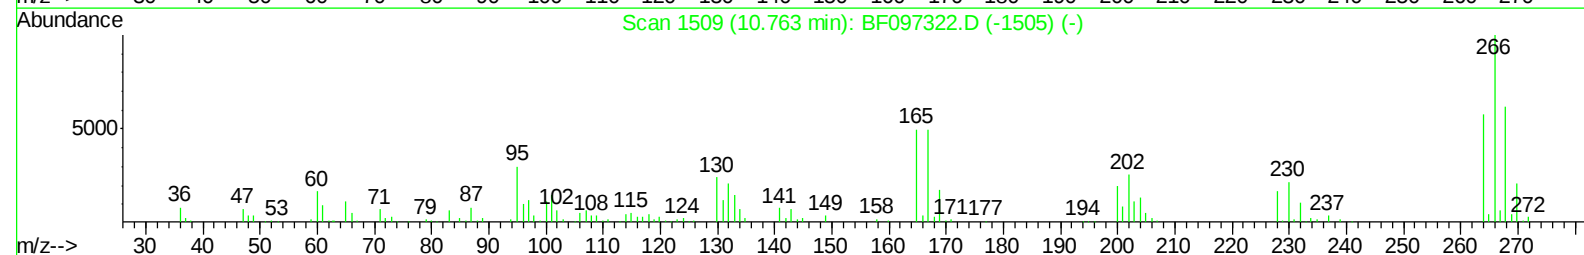
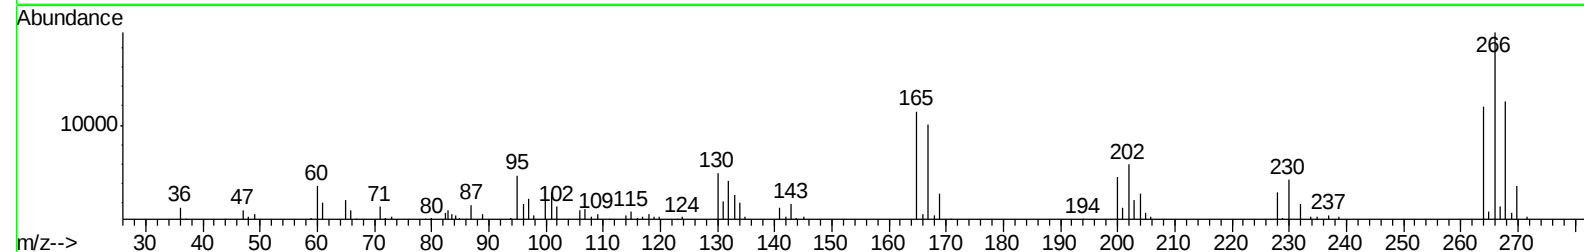


Data Path : Z:\HPCHEM1\BNA\_F\Data\BF080517\  
Data File : BF097390.D  
Acq On : 5 Aug 2017 11:28  
Operator : SJ/JU  
Sample : DFTPP  
Misc :  
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Aug 07 18:17:10 2017  
Quant Method : Z:\HPCHEM1\BNA\_F\METHODS\8270-BF072517.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Mon Aug 07 16:02:51 2017  
Response via : Initial Calibration

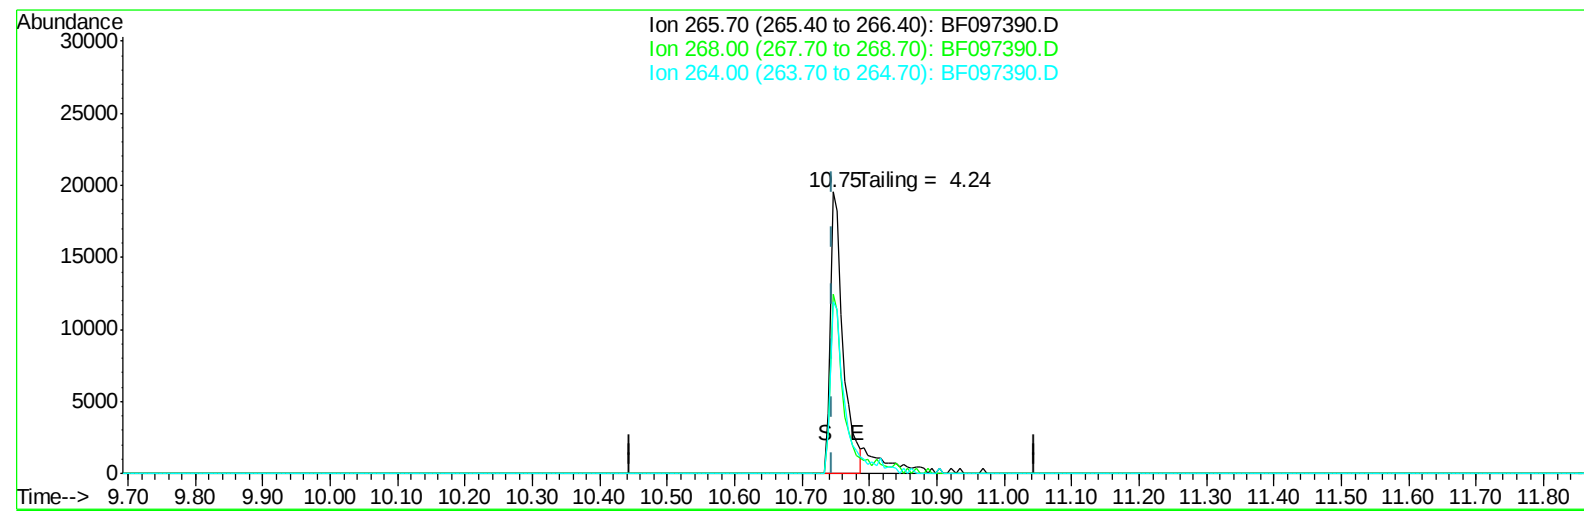

TIC: BF097390.D

(69) Pentachlorophenol (C)




10.745min (+0.000) 0.00ng

response 28939

| Ion    | Exp%  | Act%  |
|--------|-------|-------|
| 265.70 | 100   | 100   |
| 268.00 | 63.90 | 63.74 |
| 264.00 | 64.60 | 60.82 |
| 0.00   | 0.00  | 0.00  |

Data Path : Z:\HPCHEM1\BNA\_F\Data\BF080517\  
Data File : BF097390.D  
Acq On : 5 Aug 2017 11:28  
Operator : SJ/JU  
Sample : DFTPP  
Misc :  
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Aug 07 18:17:10 2017  
Quant Method : Z:\HPCHEM1\BNA\_F\METHODS\8270-BF072517.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Mon Aug 07 16:02:51 2017  
Response via : Initial Calibration

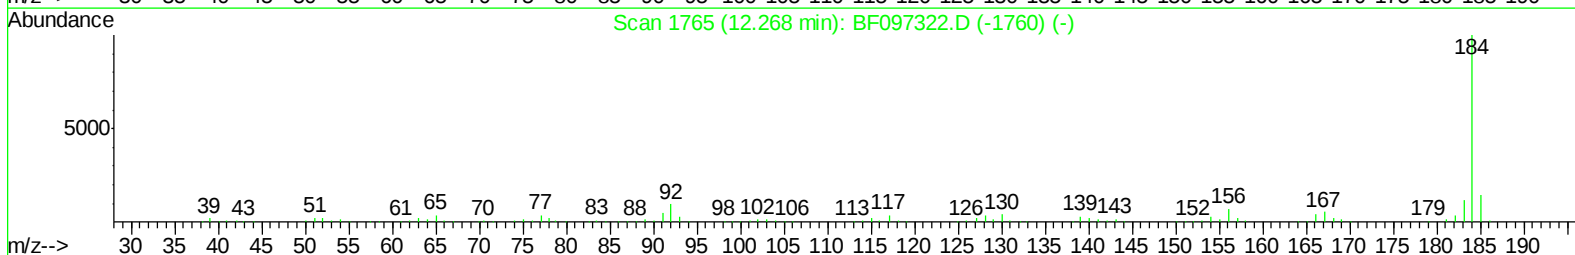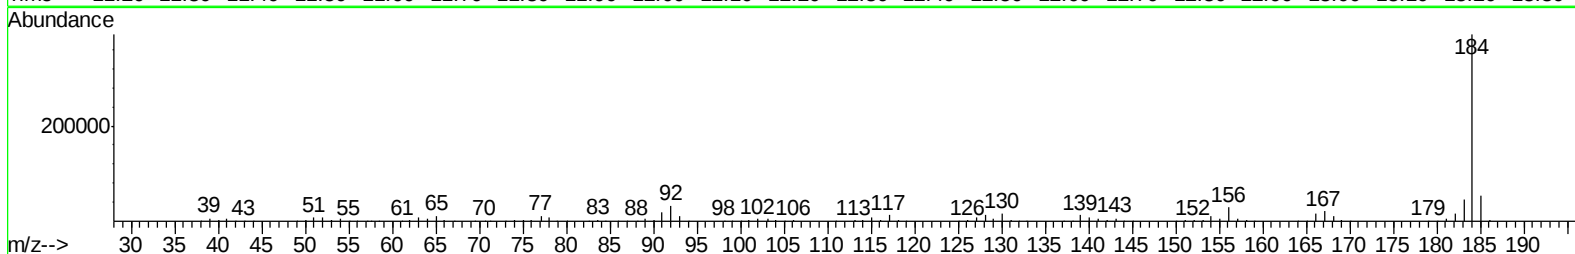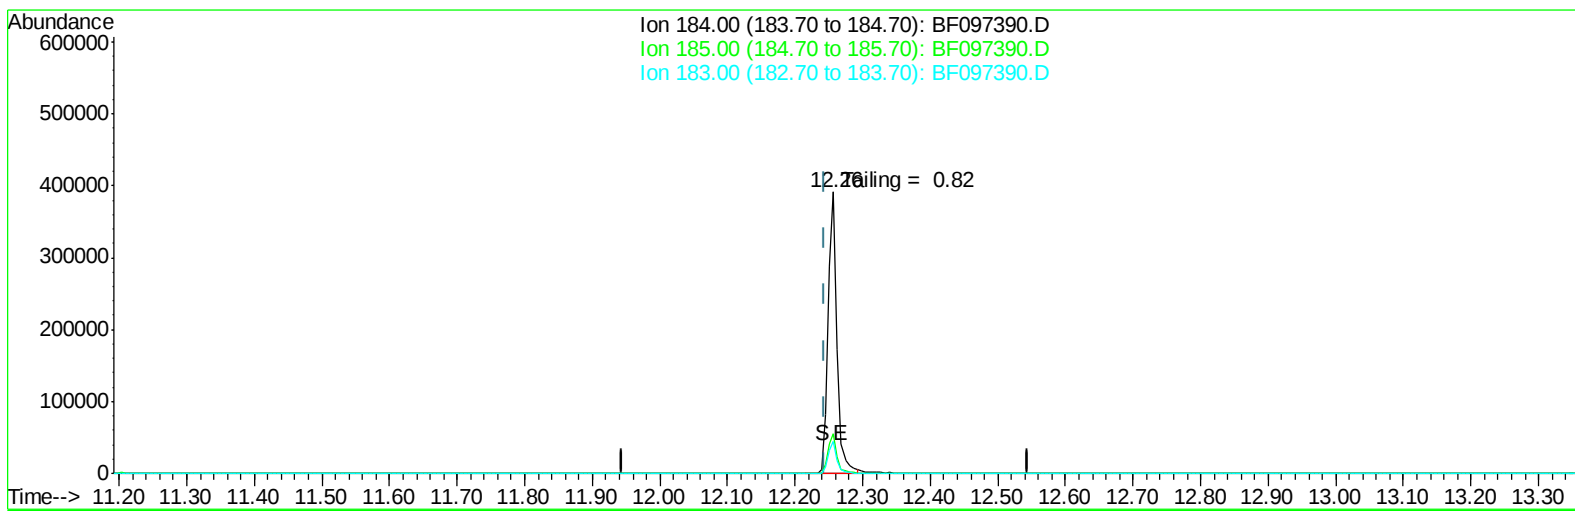

TIC: BF097390.D

(76) Benzidine

12.257min (+0.012) 0.00ng

response 367113

| Ion    | Exp%  | Act%   |
|--------|-------|--------|
| 184.00 | 100   | 100    |
| 185.00 | 19.40 | 13.91# |
| 183.00 | 12.20 | 11.54  |
| 0.00   | 0.00  | 0.00   |