

Data Path : Z:\HPCHEM1\BNA F\DATA\BF080517\
 Data File : BF097399.D
 Acq On : 5 Aug 2017 16:09
 Operator : SJ/JU
 Sample : I4594-01
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 72-12000-R4

Quant Time: Aug 06 04:38:09 2017
 Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF072517.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Aug 04 01:17:22 2017
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	6.42	152	116780	20.00	ng	-0.08
21) Naphthalene-d8	7.70	136	509029	20.00	ng	-0.08
38) Acenaphthene-d10	9.45	164	195916	20.00	ng	-0.08
63) Phenanthrene-d10	10.92	188	326449	20.00	ng	-0.08
75) Chrysene-d12	13.54	240	220923	20.00	ng	-0.09
86) Perylene-d12	14.88	264	192041	20.00	ng	-0.09
System Monitoring Compounds						
5) 2-Fluorophenol	5.02	112	691635	89.28	ng	-0.08
7) Phenol-d6	6.10	99	791055	89.45	ng	-0.07
23) Nitrobenzene-d5	7.00	82	453865	52.31	ng	-0.08
41) 2,4,6-Tribromophenol	10.24	330	153477	99.15	ng	-0.08
44) 2-Fluorobiphenyl	8.79	172	719158	62.30	ng	-0.08
78) Terphenyl-d14	12.50	244	470119	43.39	ng	-0.08
Target Compounds						
10) Phenol	6.11	94	21027	2.004	ng	79
49) Dimethylphthalate	9.19	163	136333	9.164	ng	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA F\DATA\BF080517\
Data File : BF097399.D
Acq On : 5 Aug 2017 16:09
Operator : SJ/JU
Sample : I4594-01
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
72-12000-R4

Quant Time: Aug 06 04:38:09 2017
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF072517.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Aug 04 01:17:22 2017
Response via : Initial Calibration

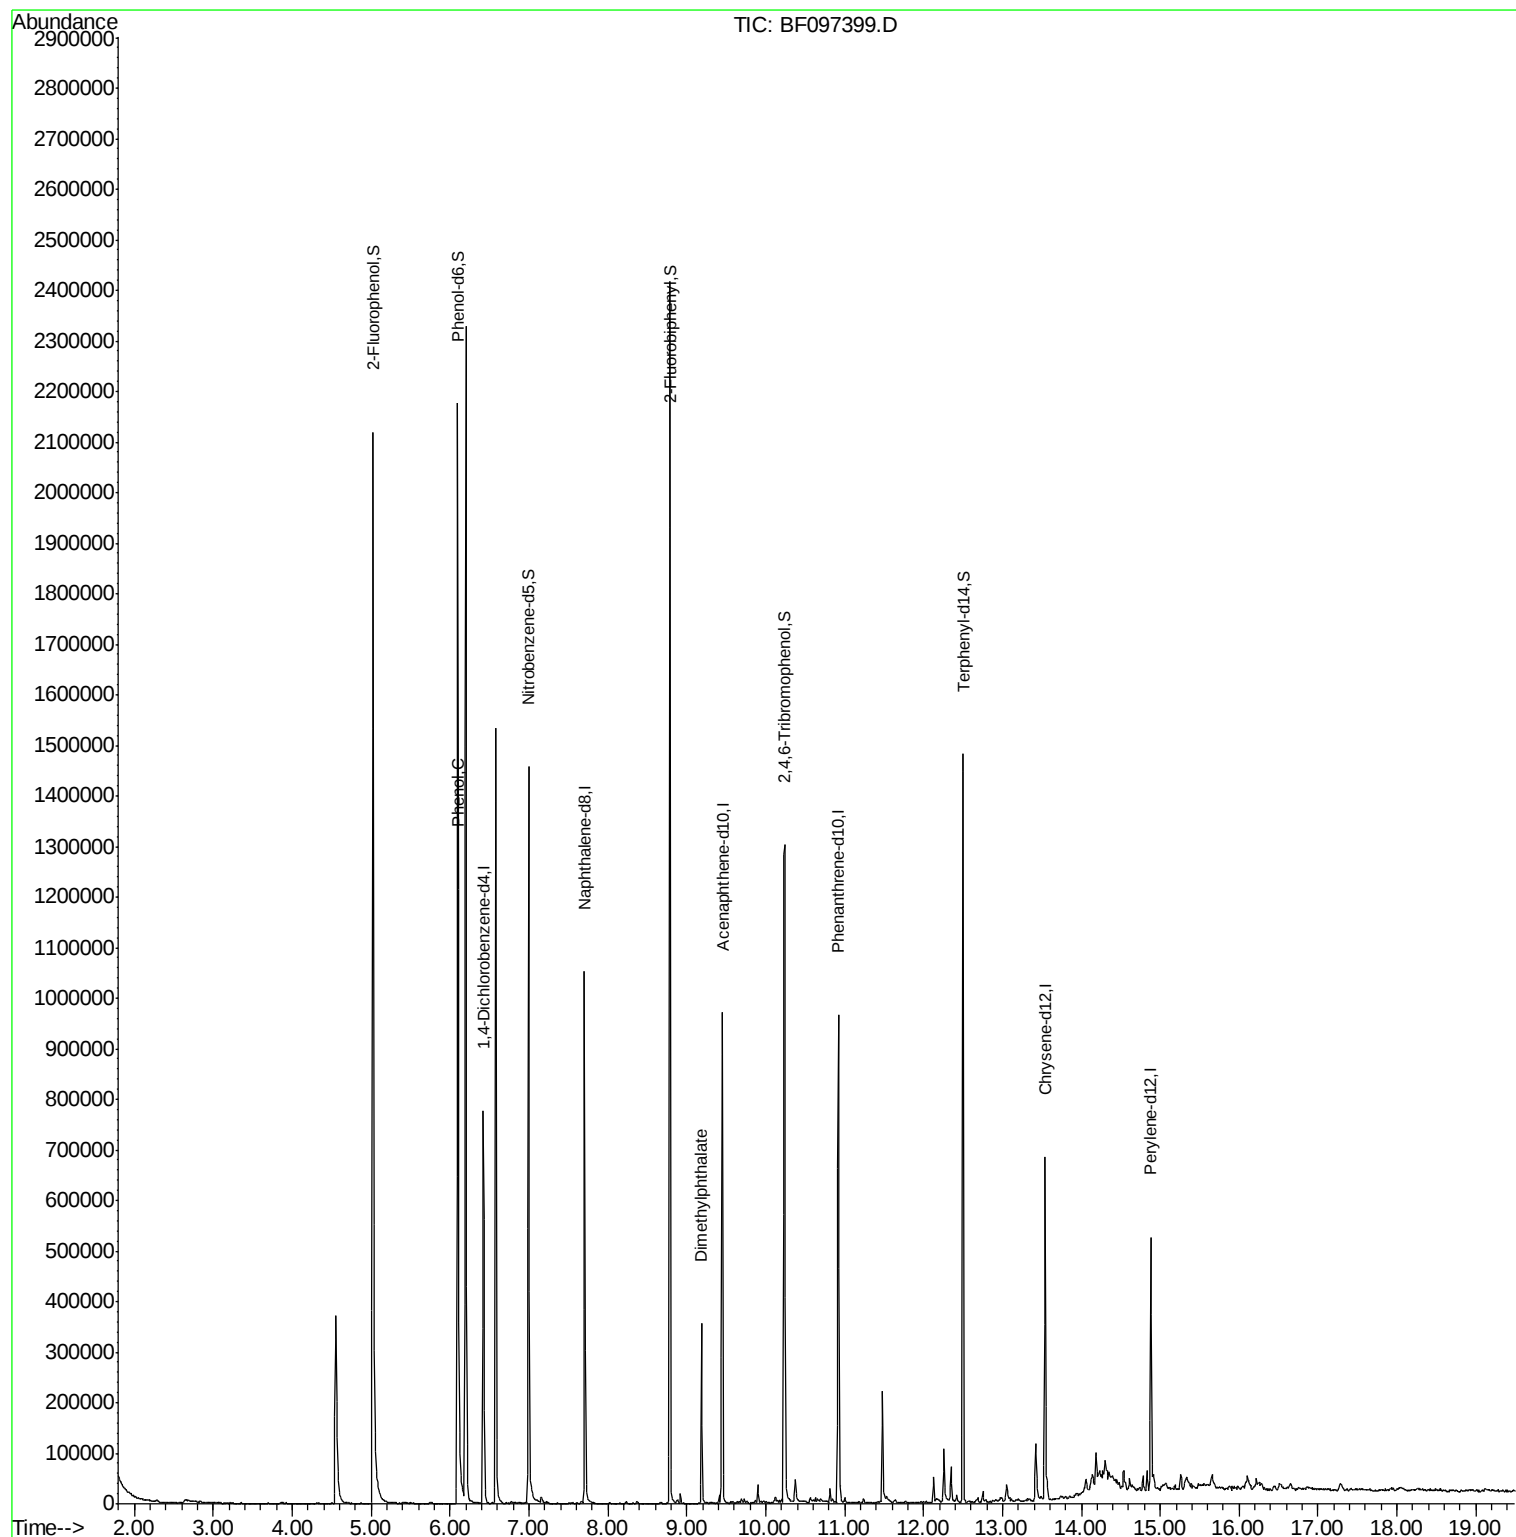

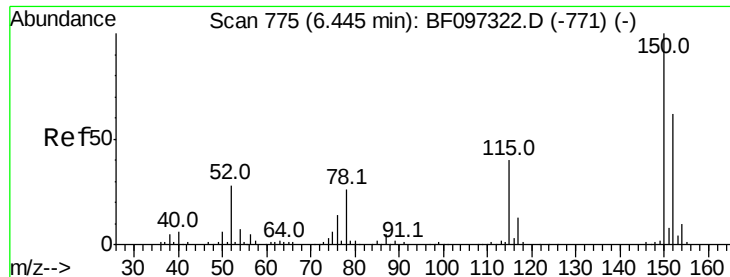


#1



1,4-Dichlorobenzene-d4
 Concen: 20.000 ng
 RT: 6.42 min Scan# 788
 Delta R.T. -0.08 min
 Lab File: BF097399.D
 Acq: 5 Aug 2017 16:09

Instrument :
 BNA_F
 ClientSampleId :
 72-12000-R4

Tot Ion:152 Resp: 116780
 Ion Ratio Lower Upper
 152 100
 150 157.9 126.2 189.2
 115 64.4 52.2 78.2

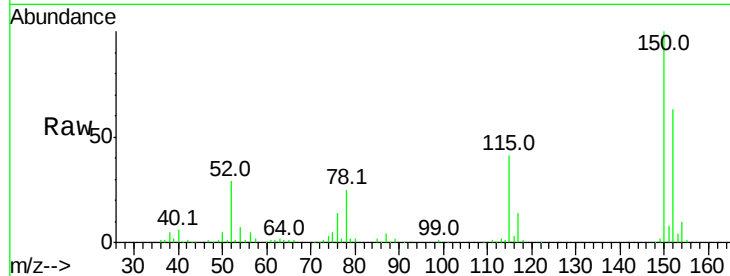


Abundance Ion 152.00 (151.70 to 152.70): E
 Ion 150.00 (149.70 to 150.70): E
 Ion 115.00 (114.70 to 115.70): E

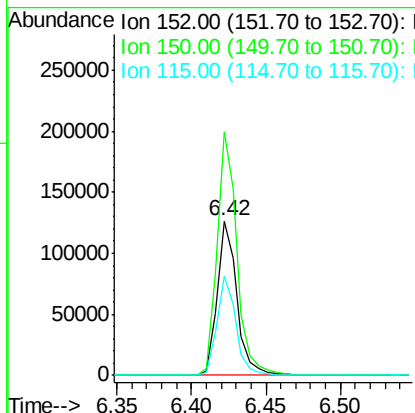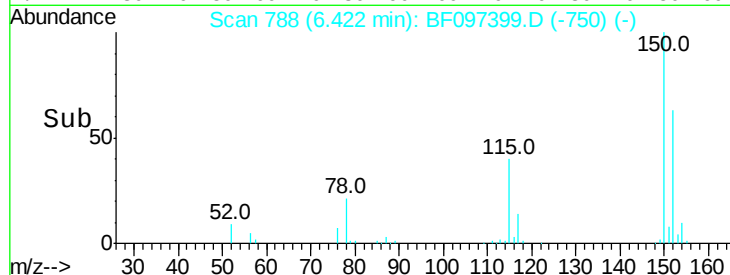



#5

2-Fluorophenol
 Concen: 89.282 ng
 RT: 5.02 min Scan# 550
 Delta R.T. -0.08 min
 Lab File: BF097399.D
 Acq: 5 Aug 2017 16:09

Tgt Ion:112 Resp: 691635
 Ion Ratio Lower Upper
 112 100
 64 67.1 46.0 69.0
 63 34.0 23.4 35.0

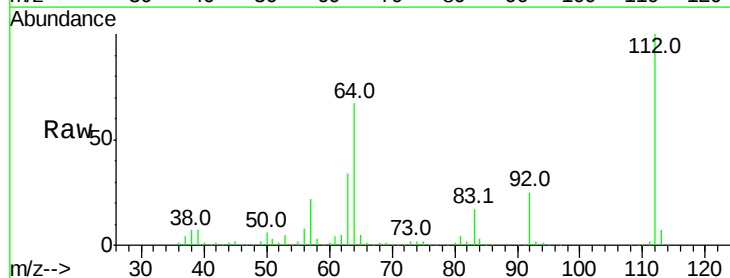

Abundance Ion 112.00 (111.70 to 112.70): E
 Ion 64.00 (63.70 to 64.70): BF0
 Ion 63.00 (62.70 to 63.70): BF0

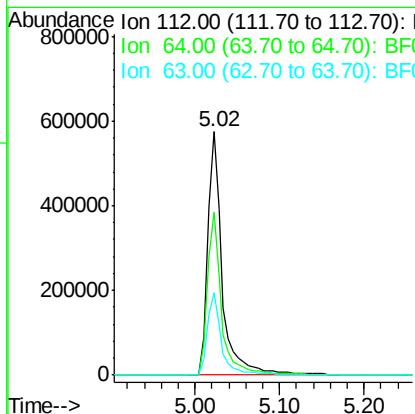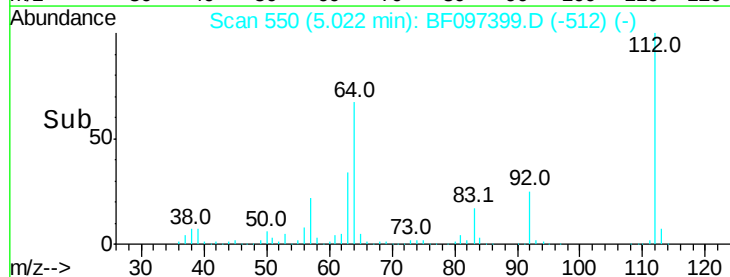



#7

Phenol-d6

Concen: 89.448 ng

RT: 6.10 min Scan# 733

Delta R.T. -0.07 min

Lab File: BF097399.D

Acq: 5 Aug 2017 16:09

Instrument :

BNA_F

ClientSampleId :

72-12000-R4


Tot Ion: 99 Resp: 791055

Ion Ratio Lower Upper

99 100

42 23.0 13.5 20.3#




71 33.2 24.5 36.7

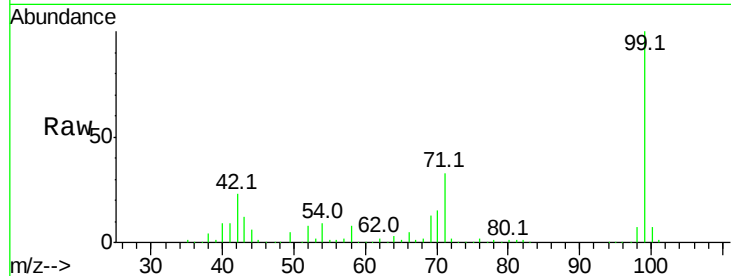

Abundance Ion 99.00 (98.70 to 99.70): BF0

Ion 42.00 (41.70 to 42.70): BF0

Ion 71.00 (70.70 to 71.70): BF0

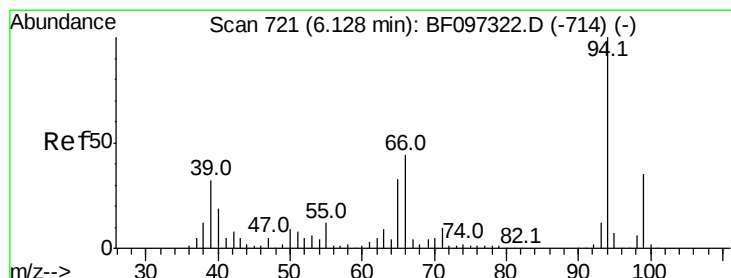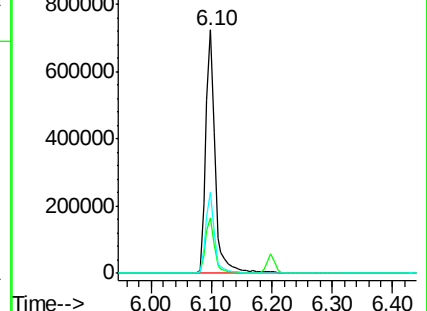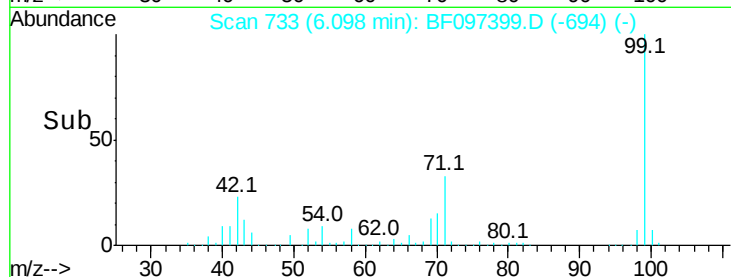

#10

Phenol

Concen: 2.004 ng

RT: 6.11 min Scan# 735

Delta R.T. -0.07 min

Lab File: BF097399.D

Acq: 5 Aug 2017 16:09


Tgt Ion: 94 Resp: 21027

Ion Ratio Lower Upper

94 100

65 35.4 9.9 49.9



66 61.1 23.1 63.1

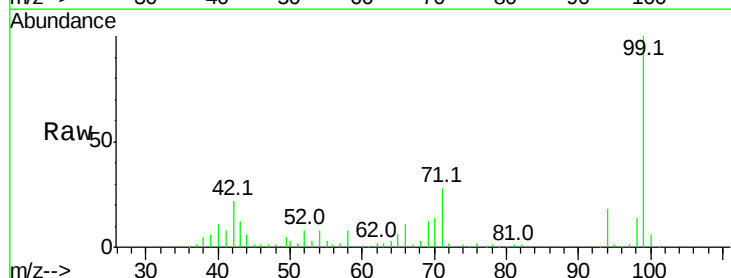


Abundance Ion 94.00 (93.70 to 94.70): BF0

Ion 65.00 (64.70 to 65.70): BF0

Ion 66.00 (65.70 to 66.70): BF0

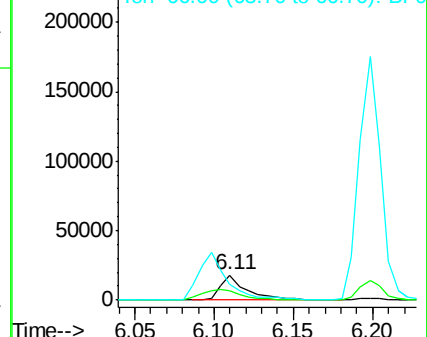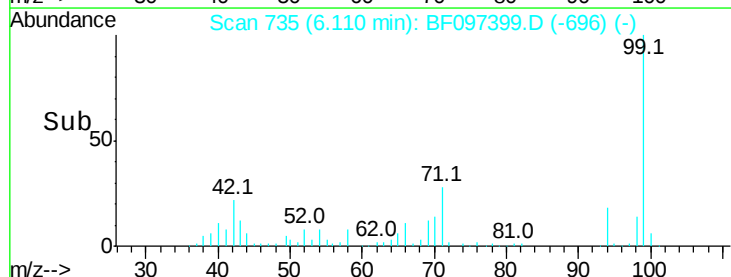

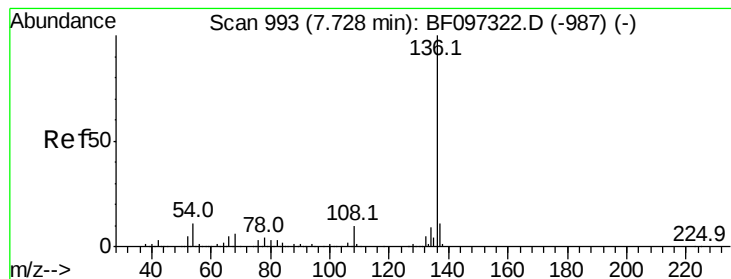

#21

Naphthalene-d8

Concen: 20.000 ng

RT: 7.70 min Scan# 1006

Delta R.T. -0.08 min

Lab File: BF097399.D

Acq: 5 Aug 2017 16:09

Instrument :

BNA_F

ClientSampleId :

72-12000-R4

Tot Ion:136 Resp: 509029


Ion Ratio Lower Upper

136 100

137 11.0 8.5 12.7

54 11.1 4.9 7.3#

68 5.8 4.1 6.1



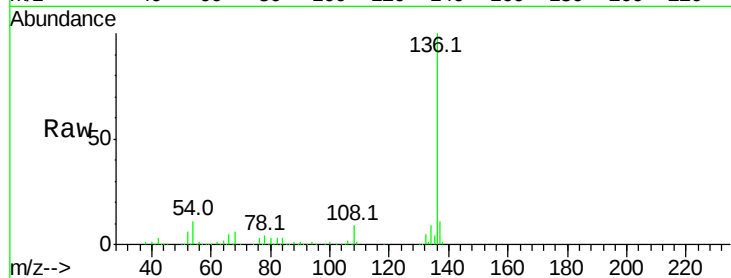


Abundance Ion 136.00 (135.70 to 136.70): E

Ion 137.00 (136.70 to 137.70): E

Ion 54.00 (53.70 to 54.70): BF0

Ion 68.00 (67.70 to 68.70): BF0

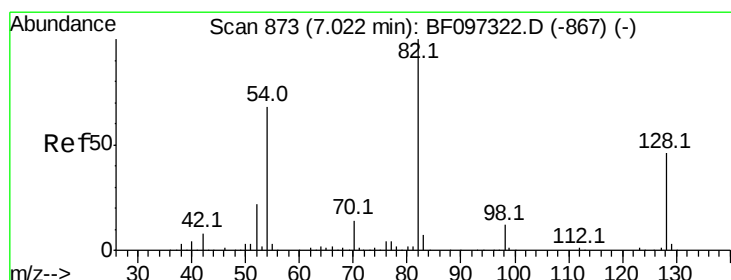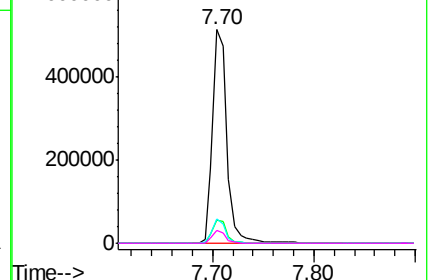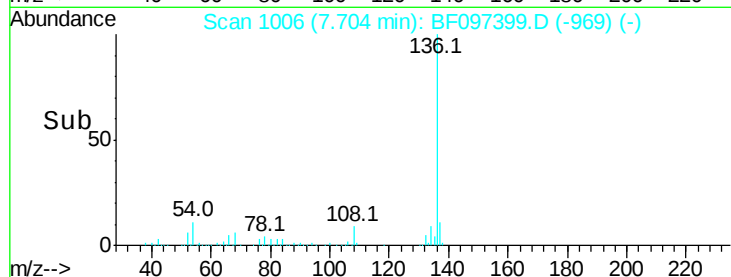

#23

Nitrobenzene-d5

Concen: 52.307 ng

RT: 7.00 min Scan# 886

Delta R.T. -0.08 min

Lab File: BF097399.D

Acq: 5 Aug 2017 16:09


Tgt Ion: 82 Resp: 453865

Ion Ratio Lower Upper

82 100

128 48.8 34.0 51.0



54 66.8 42.2 63.2#

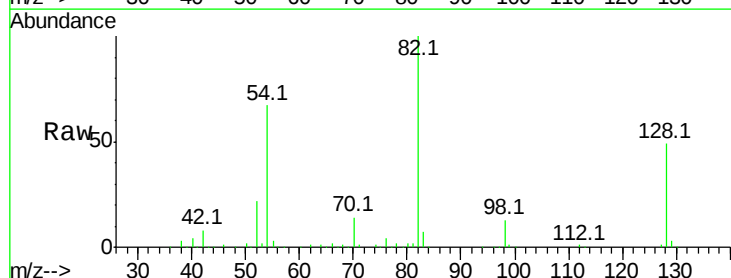


Abundance Ion 82.00 (81.70 to 82.70): BF0

Ion 128.00 (127.70 to 128.70): E

Ion 54.00 (53.70 to 54.70): BF0

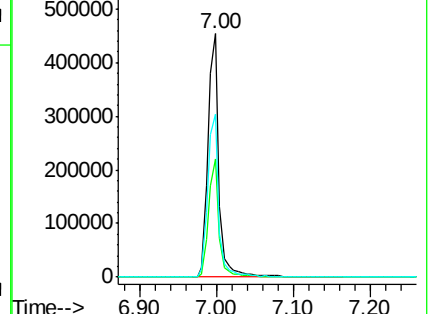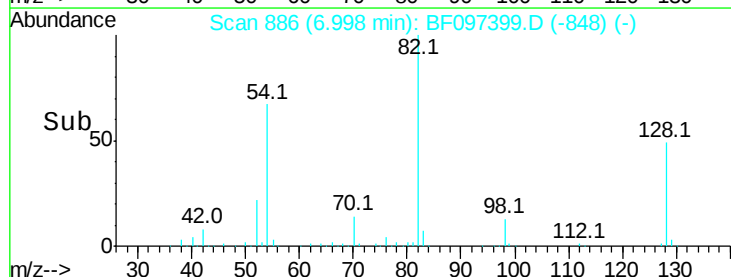


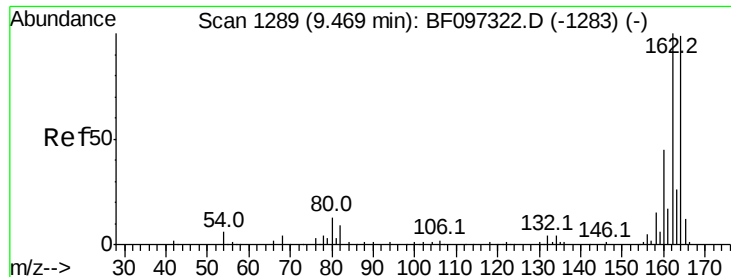




#38
 Acenaphthene-d10
 Concen: 20.000 ng
 RT: 9.45 min Scan# 1303
 Delta R.T. -0.08 min
 Lab File: BF097399.D
 Acq: 5 Aug 2017 16:09

Instrument :
 BNA_F
 ClientSampleId :
 72-12000-R4

Tot Ion	Ratio	Lower	Upper
164	100		
162	105.0	82.6	123.8
160	47.2	36.2	54.2

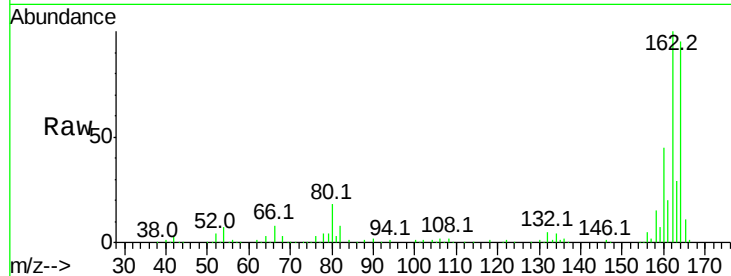


Abundance Ion 164.00 (163.70 to 164.70): E
 Ion 162.00 (161.70 to 162.70): E
 Ion 160.00 (159.70 to 160.70): E

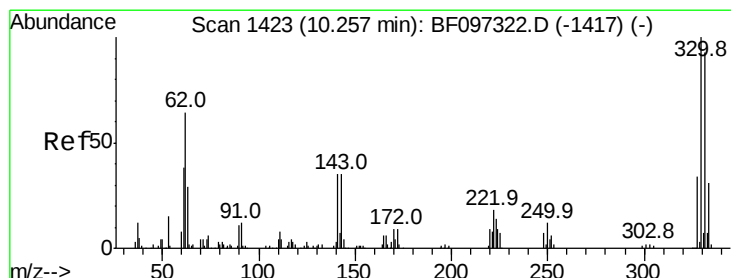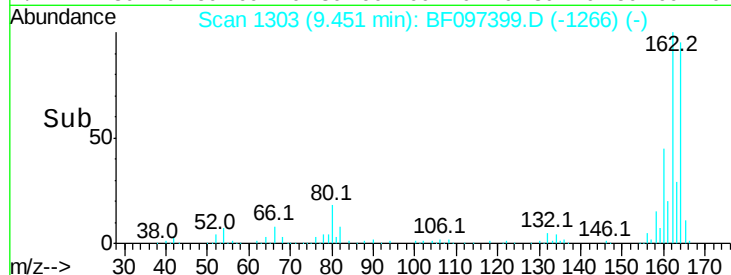
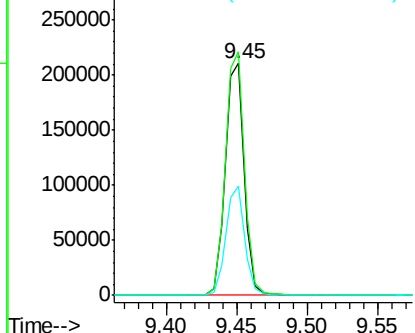



#41
 2,4,6-Tribromophenol
 Concen: 99.150 ng
 RT: 10.24 min Scan# 1437
 Delta R.T. -0.08 min
 Lab File: BF097399.D
 Acq: 5 Aug 2017 16:09

Tgt Ion	Ratio	Lower	Upper
330	100		
332	95.6	76.6	115.0
141	39.8	31.4	47.2

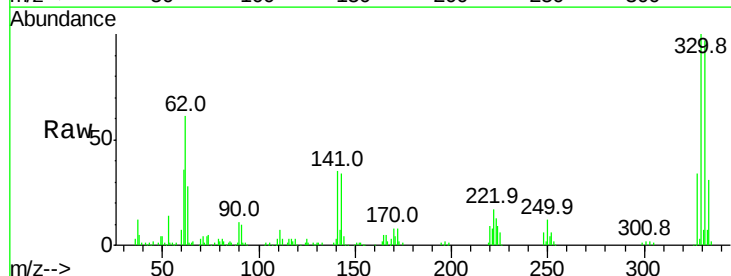

Abundance Ion 329.80 (329.50 to 330.50): E
 Ion 331.80 (331.50 to 332.50): E
 Ion 141.00 (140.70 to 141.70): E



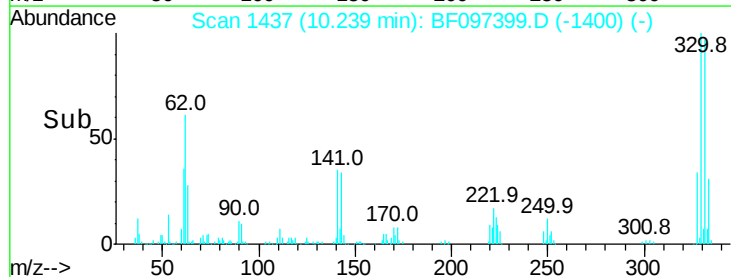
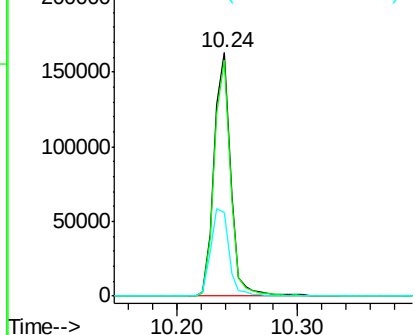


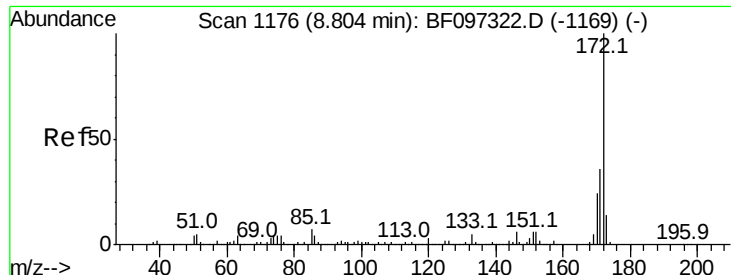

#44
2-Fluorobiphenyl
Concen: 62.296 ng
RT: 8.79 min Scan# 1190
Delta R.T. -0.08 min
Lab File: BF097399.D
Acq: 5 Aug 2017 16:09




Instrument :
BNA_F
ClientSampleId :
72-12000-R4


Tot Ion:172 Resp: 719158
Ion Ratio Lower Upper
172 100
171 36.5 29.6 44.4
170 24.7 19.8 29.8

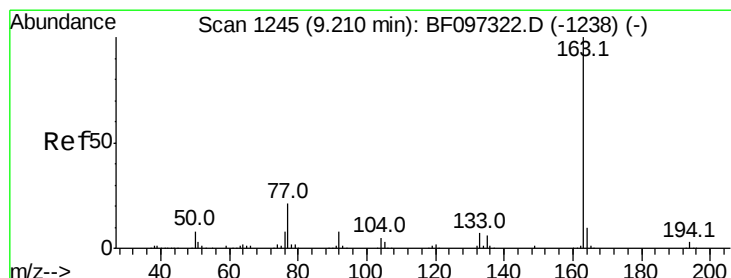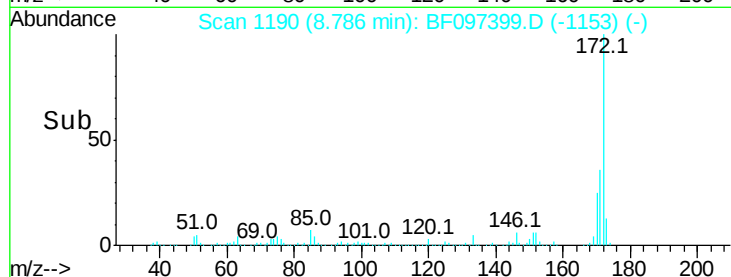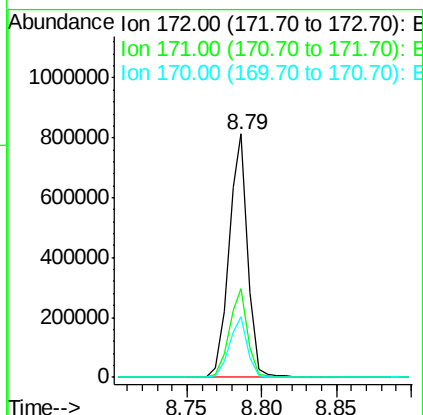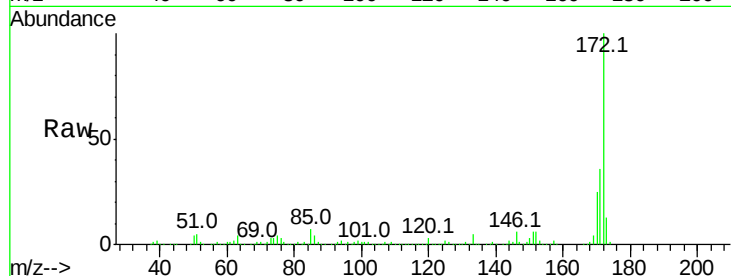

#49
Dimethylphthalate
Concen: 9.164 ng
RT: 9.19 min Scan# 1258
Delta R.T. -0.09 min
Lab File: BF097399.D
Acq: 5 Aug 2017 16:09

Tgt Ion:163 Resp: 136333
Ion Ratio Lower Upper
163 100
194 3.3 2.6 4.0
164 9.8 8.4 12.6

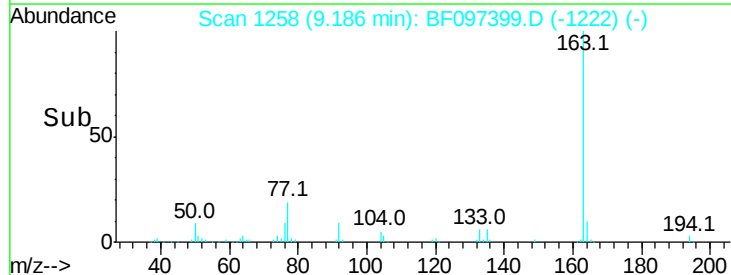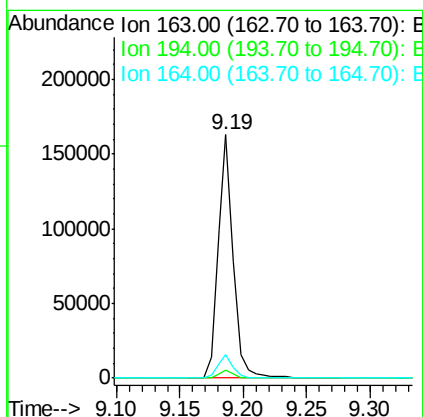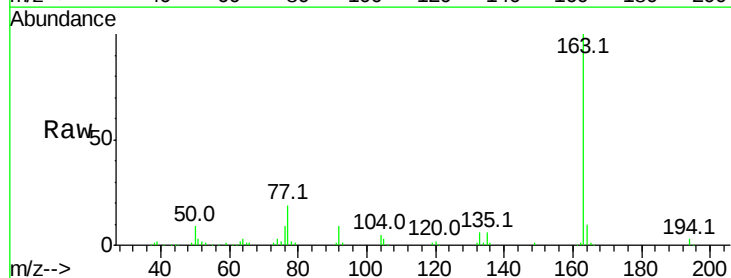

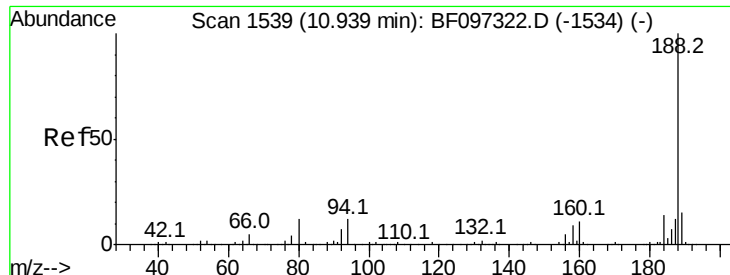

#63

Phenanthrene-d10

Concen: 20.000 ng

RT: 10.92 min Scan# 1553

Delta R.T. -0.08 min

Lab File: BF097399.D

Acq: 5 Aug 2017 16:09

Instrument :

BNA_F

ClientSampleId :

72-12000-R4


Tot Ion:188 Resp: 326449

Ion Ratio Lower Upper

188 100

94 11.8 9.4 14.2




80 10.9 10.2 15.2

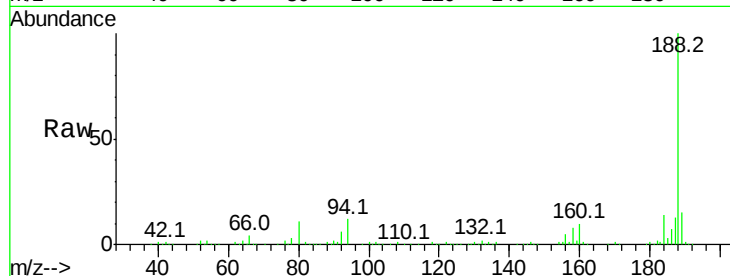

Abundance Ion 188.00 (187.70 to 188.70): E

Ion 94.00 (93.70 to 94.70): BF0

Ion 80.00 (79.70 to 80.70): BF0

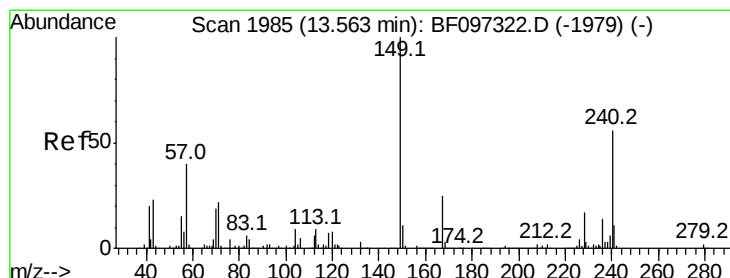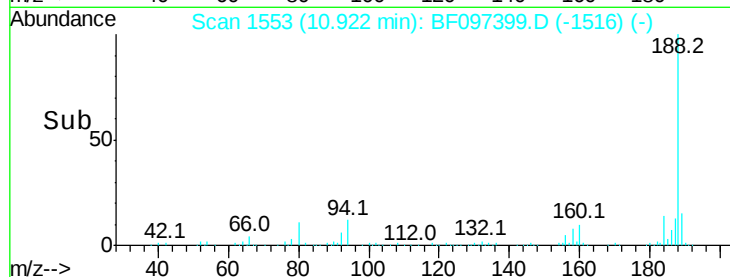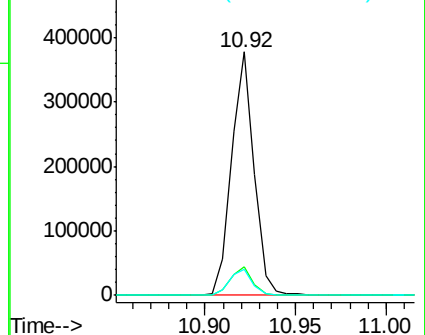

#75

Chrysene-d12

Concen: 20.000 ng

RT: 13.54 min Scan# 1998

Delta R.T. -0.09 min

Lab File: BF097399.D

Acq: 5 Aug 2017 16:09


Tgt Ion:240 Resp: 220923

Ion Ratio Lower Upper

240 100

120 16.5 5.8 8.8#



236 25.5 20.5 30.7

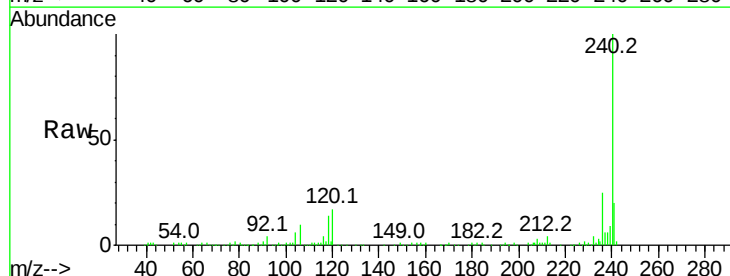


Abundance Ion 240.00 (239.70 to 240.70): E

Ion 120.00 (119.70 to 120.70): E

Ion 236.00 (235.70 to 236.70): E



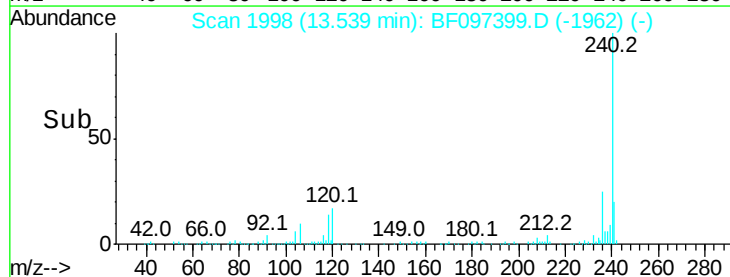
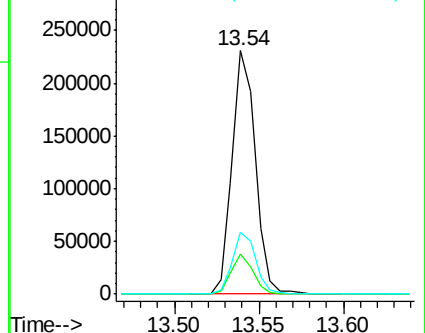


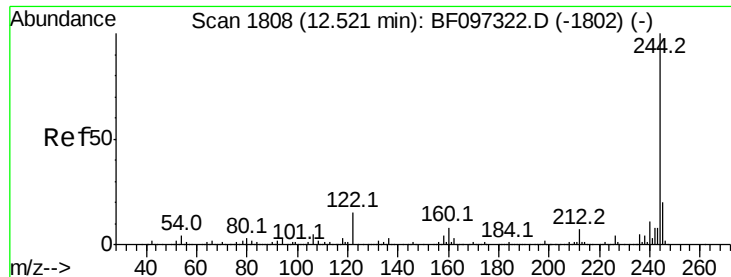

#78
 Terphenyl-d14
 Concen: 43.386 ng
 RT: 12.50 min Scan# 1822
 Delta R.T. -0.08 min
 Lab File: BF097399.D
 Acq: 5 Aug 2017 16:09

Instrument :
 BNA_F
 ClientSampleId :
 72-12000-R4

Tot Ion:244 Resp: 470119
 Ion Ratio Lower Upper
 244 100
 212 6.6 6.0 9.0
 122 13.1 10.3 15.5

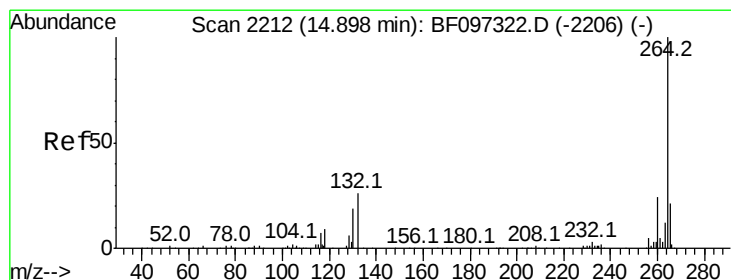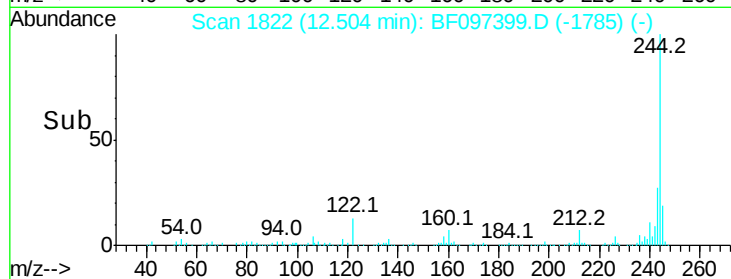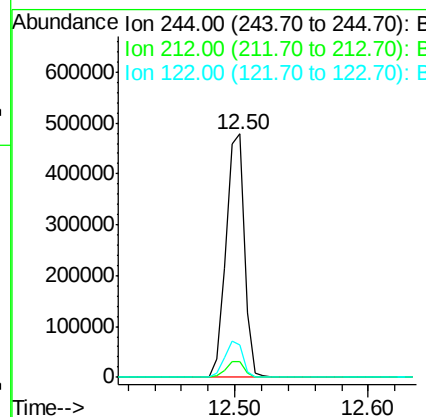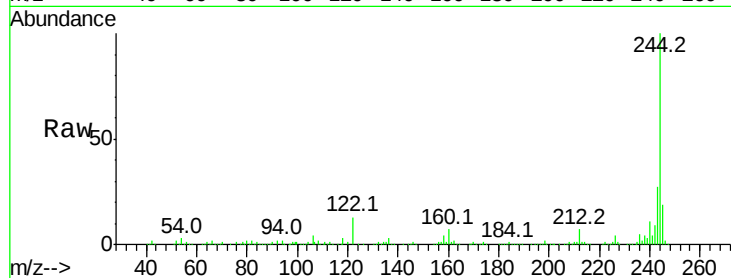

#86
 Perylene-d12
 Concen: 20.000 ng
 RT: 14.88 min Scan# 2226
 Delta R.T. -0.09 min
 Lab File: BF097399.D
 Acq: 5 Aug 2017 16:09

Tgt Ion:264 Resp: 192041
 Ion Ratio Lower Upper
 264 100
 260 24.3 19.5 29.3
 265 21.3 17.2 25.8

