

Data Path : Z:\HPCHEM1\BNA F\DATA\BF080517\
 Data File : BF097410.D
 Acq On : 5 Aug 2017 21:15
 Operator : SJ/JU
 Sample : I4610-10 10X
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 PL-02-080317-D

Quant Time: Aug 06 05:08:01 2017
 Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF072517.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Aug 04 01:17:22 2017
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	6.43	152	81069	20.00	ng	-0.07
21) Naphthalene-d8	7.71	136	326043	20.00	ng	-0.08
38) Acenaphthene-d10	9.45	164	111337	20.00	ng	-0.08
63) Phenanthrene-d10	10.92	188	182024	20.00	ng	-0.08
75) Chrysene-d12	13.54	240	159748	20.00	ng	-0.08
86) Perylene-d12	14.89	264	95323	20.00	ng	-0.09
System Monitoring Compounds						
5) 2-Fluorophenol	5.05	112	48856	9.08	ng	-0.05
7) Phenol-d6	6.12	99	55589	9.05	ng	-0.05
23) Nitrobenzene-d5	7.00	82	27767	5.00	ng	-0.07
41) 2,4,6-Tribromophenol	10.25	330	6958	7.91	ng	-0.08
44) 2-Fluorobiphenyl	8.79	172	49355	7.52	ng	-0.08
78) Terphenyl-d14	12.50	244	39952	5.10	ng	-0.09


Target Compounds Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA F\DATA\BF080517\
Data File : BF097410.D
Acq On : 5 Aug 2017 21:15
Operator : SJ/JU
Sample : I4610-10 10X
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PL-02-080317-D

Quant Time: Aug 06 05:08:01 2017
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF072517.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Aug 04 01:17:22 2017
Response via : Initial Calibration

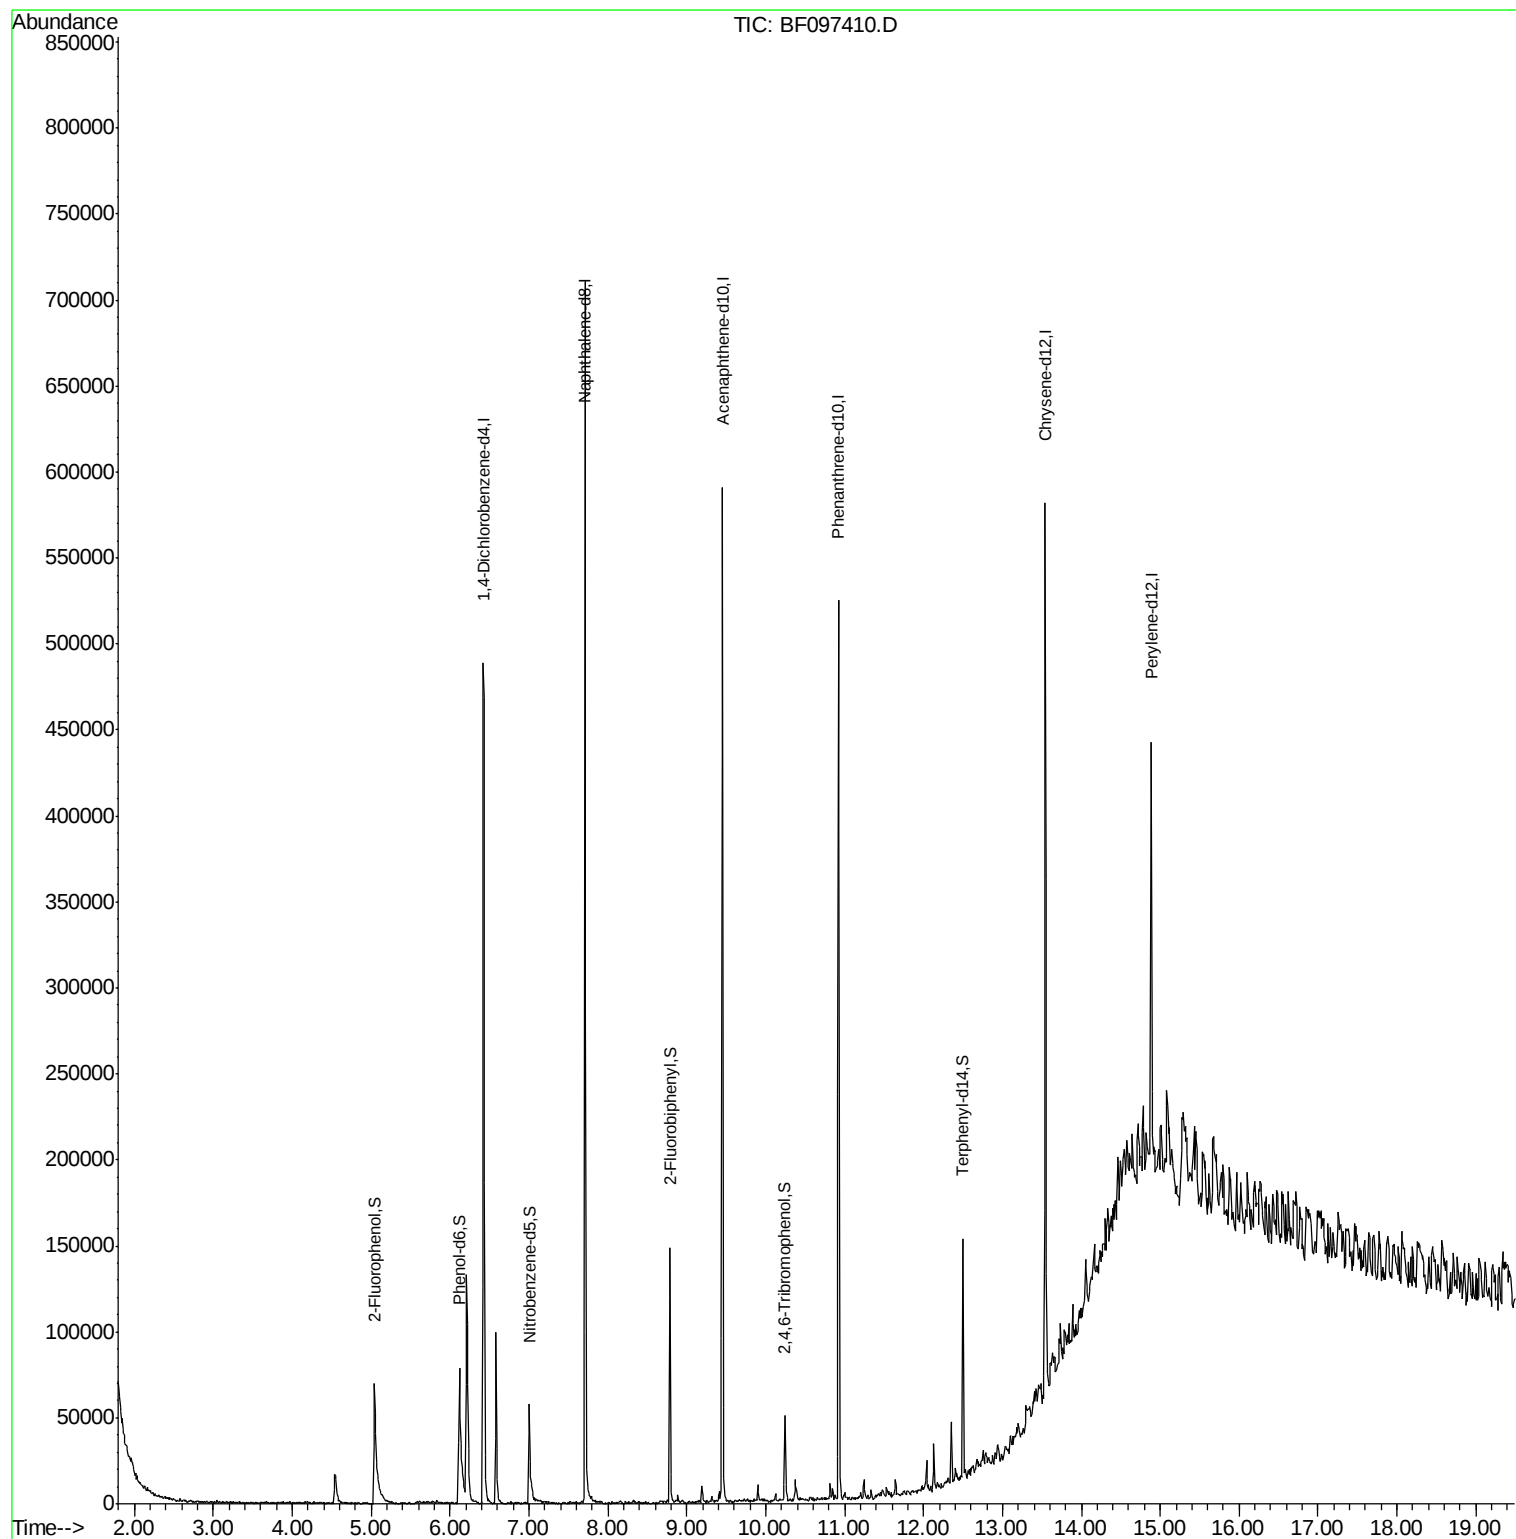

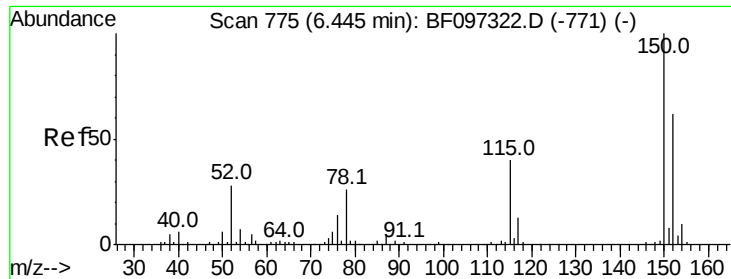


#1




1,4-Dichlorobenzene-d4
Concen: 20.000 ng
RT: 6.43 min Scan# 789
Delta R.T. -0.07 min
Lab File: BF097410.D
Acq: 5 Aug 2017 21:15

Instrument :
BNA_F
ClientSampleId :
PL-02-080317-D

Tot Ion:152 Resp: 81069
Ion Ratio Lower Upper
152 100
150 155.4 126.2 189.2
115 60.1 52.2 78.2

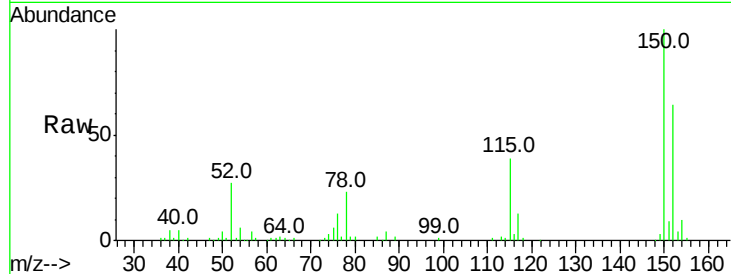


Abundance Ion 152.00 (151.70 to 152.70): E
Ion 150.00 (149.70 to 150.70): E
Ion 115.00 (114.70 to 115.70): E

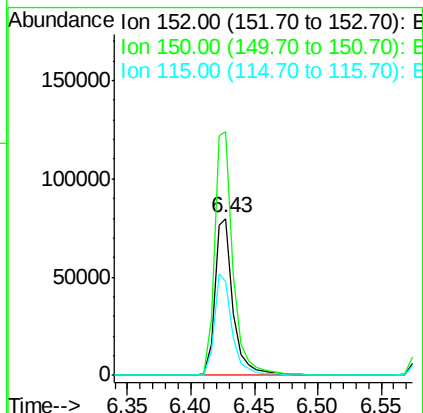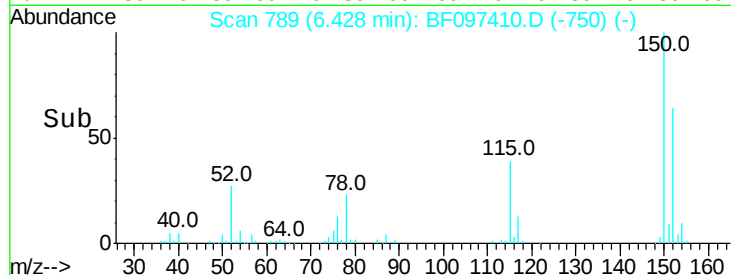



#5

2-Fluorophenol
Concen: 9.085 ng
RT: 5.05 min Scan# 554
Delta R.T. -0.05 min
Lab File: BF097410.D
Acq: 5 Aug 2017 21:15

Tgt Ion:112 Resp: 48856
Ion Ratio Lower Upper
112 100
64 63.2 46.0 69.0
63 29.8 23.4 35.0

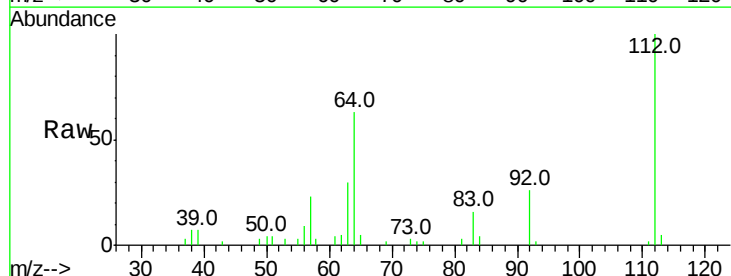

Abundance Ion 112.00 (111.70 to 112.70): E
Ion 64.00 (63.70 to 64.70): BF0
Ion 63.00 (62.70 to 63.70): BF0

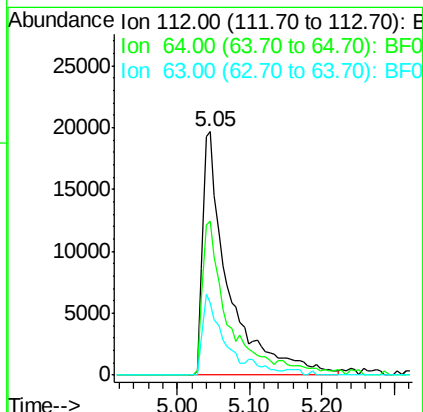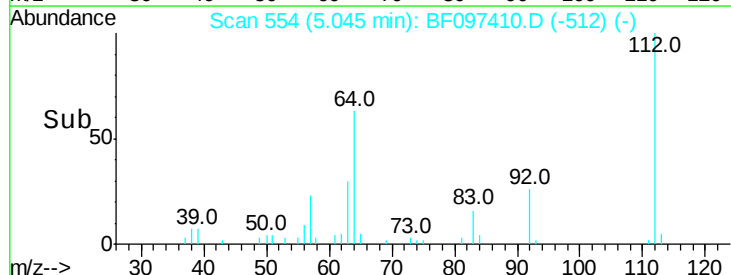



#7

Phenol-d6

Concen: 9.055 ng

RT: 6.12 min Scan# 736

Delta R.T. -0.05 min

Lab File: BF097410.D

Acq: 5 Aug 2017 21:15

Instrument :





BNA_F

ClientSampleId :

PL-02-080317-D

Tot Ion: 99 Resp: 55589

Ion	Ratio	Lower	Upper
99	100		
42	23.8	13.5	20.3#
71	31.6	24.5	36.7

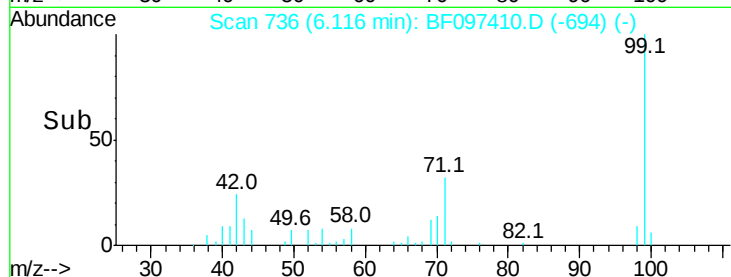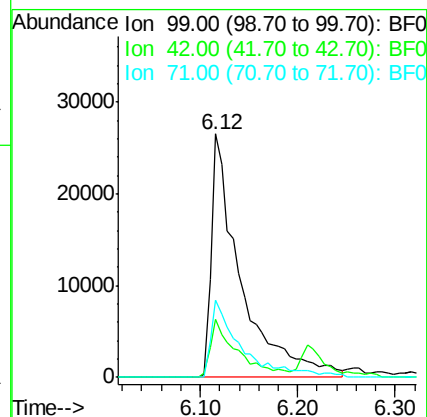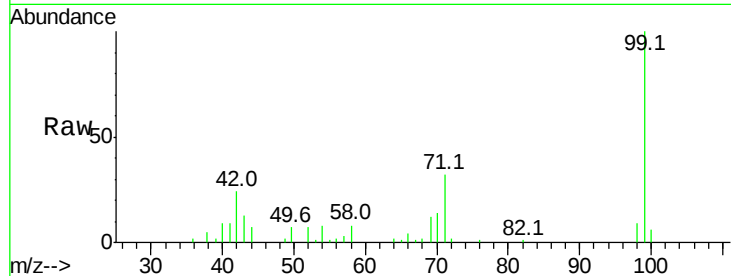

#21

Naphthalene-d8

Concen: 20.000 ng

RT: 7.71 min Scan# 1007




Delta R.T. -0.08 min

Lab File: BF097410.D

Acq: 5 Aug 2017 21:15

Tgt Ion: 136 Resp: 326043

Ion	Ratio	Lower	Upper
136	100		
137	10.5	8.5	12.7
54	9.9	4.9	7.3#
68	5.5	4.1	6.1


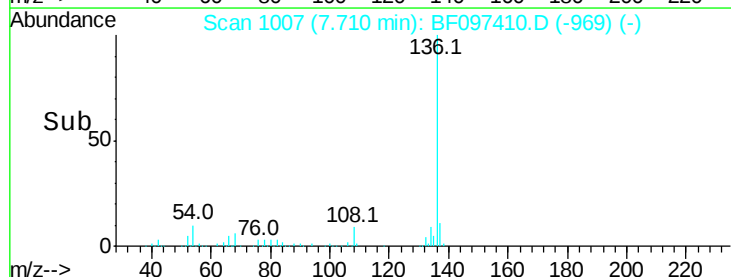
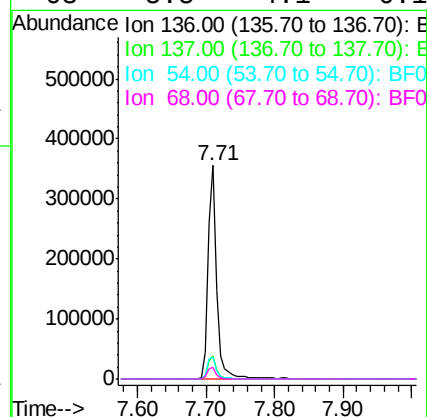





#23
 Nitrobenzene-d5
 Concen: 4.996 ng
 RT: 7.00 min Scan# 887
 Delta R.T. -0.07 min
 Lab File: BF097410.D
 Acq: 5 Aug 2017 21:15




Instrument :
 BNA_F
 ClientSampleId :
 PL-02-080317-D

Tot Ion: 82 Resp: 27767
 Ion Ratio Lower Upper
 82 100
 128 51.4 34.0 51.0#
 54 71.3 42.2 63.2#

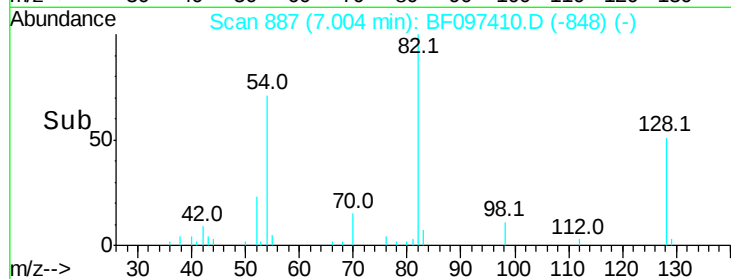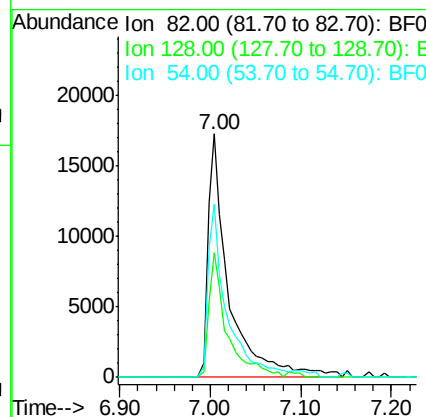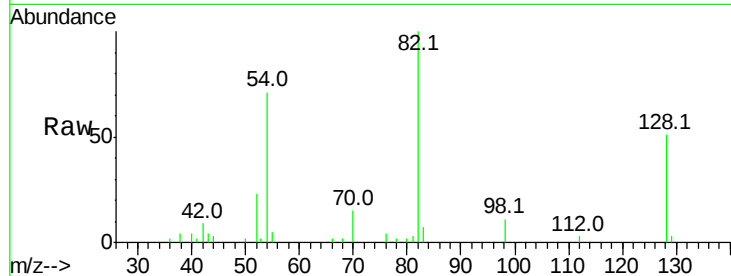

#38
 Acenaphthene-d10
 Concen: 20.000 ng
 RT: 9.45 min Scan# 1303
 Delta R.T. -0.08 min
 Lab File: BF097410.D
 Acq: 5 Aug 2017 21:15

Tgt Ion:164 Resp: 111337
 Ion Ratio Lower Upper
 164 100
 162 104.6 82.6 123.8
 160 45.9 36.2 54.2

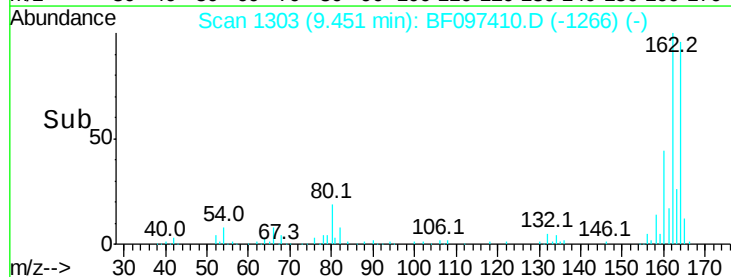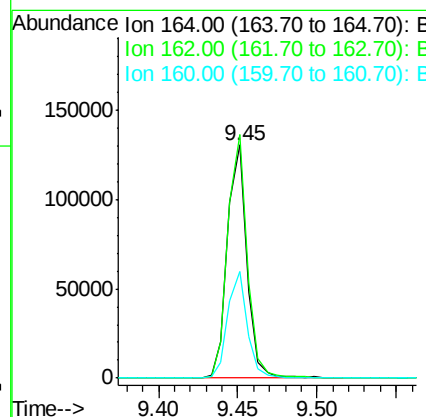







#41
 2,4,6-Tribromophenol
 Concen: 7.910 ng
 RT: 10.25 min Scan# 1438
 Delta R.T. -0.08 min
 Lab File: BF097410.D
 Acq: 5 Aug 2017 21:15

Instrument :
 BNA_F
 ClientSampleId :
 PL-02-080317-D

Tot Ion:330 Resp: 6958
 Ion Ratio Lower Upper
 330 100
 332 92.5 76.6 115.0
 141 39.9 31.4 47.2




Abundance Ion 329.80 (329.50 to 330.50): E
 Ion 331.80 (331.50 to 332.50): E
 Ion 141.00 (140.70 to 141.70): E

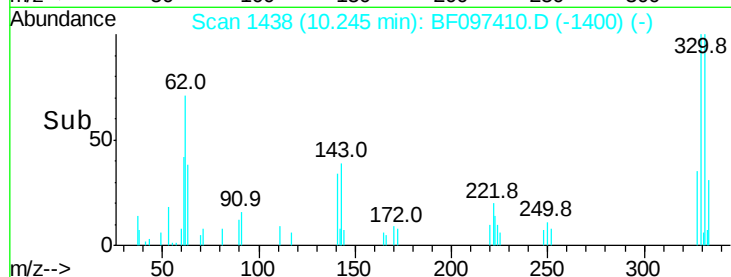
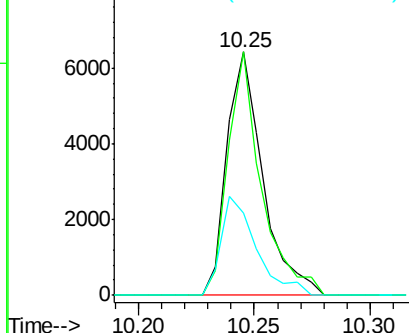



#44
 2-Fluorobiphenyl
 Concen: 7.523 ng
 RT: 8.79 min Scan# 1190
 Delta R.T. -0.08 min
 Lab File: BF097410.D
 Acq: 5 Aug 2017 21:15

Tgt Ion:172 Resp: 49355
 Ion Ratio Lower Upper
 172 100
 171 33.0 29.6 44.4
 170 23.7 19.8 29.8



Abundance Ion 172.00 (171.70 to 172.70): E
 Ion 171.00 (170.70 to 171.70): E
 Ion 170.00 (169.70 to 170.70): E

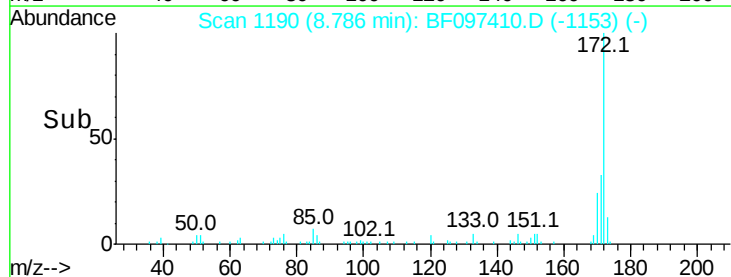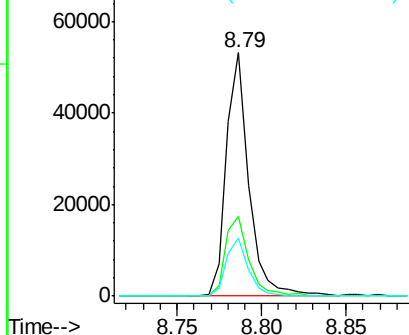


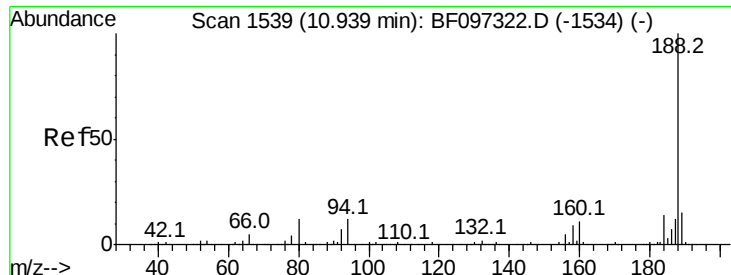




#63
Phenanthrene-d10
Concen: 20.000 ng
RT: 10.92 min Scan# 1553
Delta R.T. -0.08 min
Lab File: BF097410.D
Acq: 5 Aug 2017 21:15

Instrument :
BNA_F
ClientSampleId :
PL-02-080317-D

Tot Ion	Ratio	Lower	Upper
188	100		
94	11.3	9.4	14.2
80	12.4	10.2	15.2

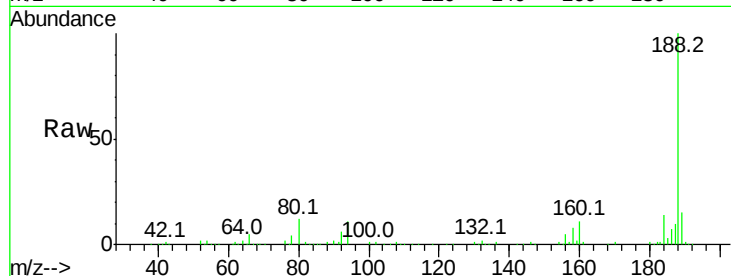


Abundance Ion 188.00 (187.70 to 188.70): E
Ion 94.00 (93.70 to 94.70): BF0
Ion 80.00 (79.70 to 80.70): BF0

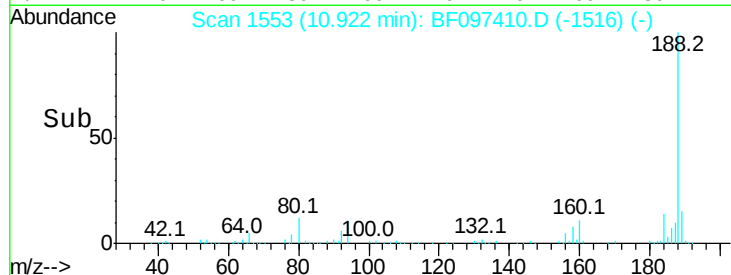
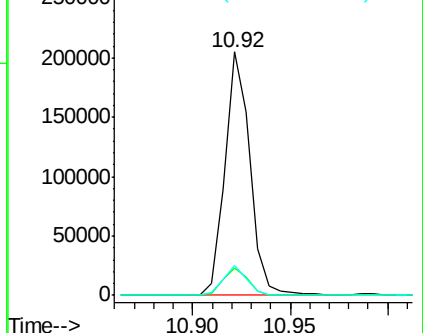



#75
Chrysene-d12
Concen: 20.000 ng
RT: 13.54 min Scan# 1999
Delta R.T. -0.08 min
Lab File: BF097410.D
Acq: 5 Aug 2017 21:15

Tgt Ion	Ratio	Lower	Upper
240	100		
120	14.5	5.8	8.8#
236	25.6	20.5	30.7

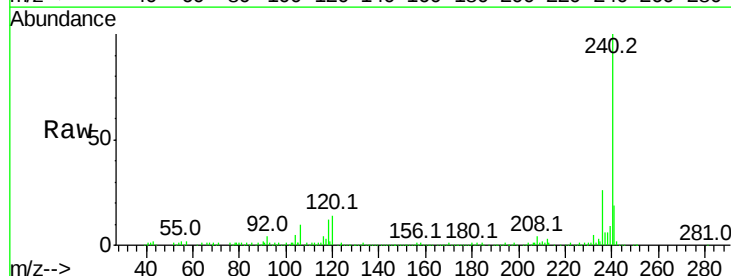

Abundance Ion 240.00 (239.70 to 240.70): E
Ion 120.00 (119.70 to 120.70): E
Ion 236.00 (235.70 to 236.70): E

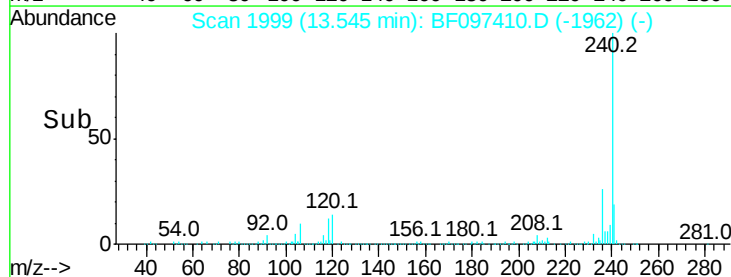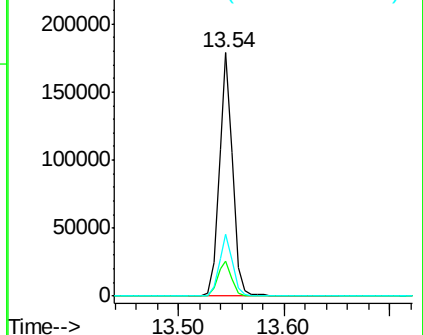

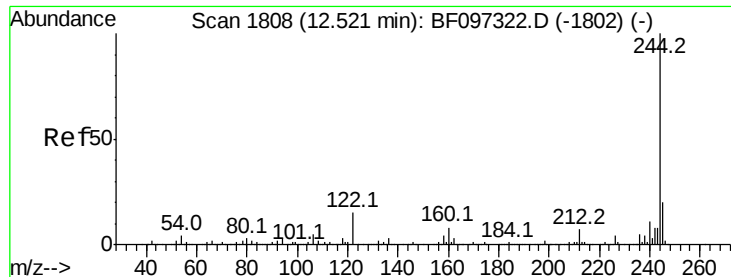

#78

Terphenyl-d14

Concen: 5.099 ng

RT: 12.50 min Scan# 1821

Delta R.T. -0.09 min

Lab File: BF097410.D

Acq: 5 Aug 2017 21:15

Instrument :

BNA_F

ClientSampleId :

PL-02-080317-D


Tot Ion:244 Resp: 39952

Ion Ratio Lower Upper

244 100

212 7.0 6.0 9.0




122 16.7 10.3 15.5#

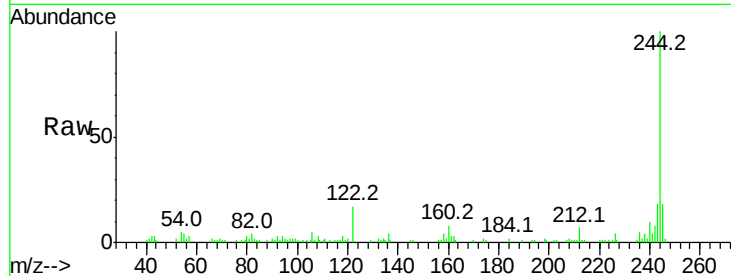

Abundance Ion 244.00 (243.70 to 244.70): E

Ion 212.00 (211.70 to 212.70): E

Ion 122.00 (121.70 to 122.70): E

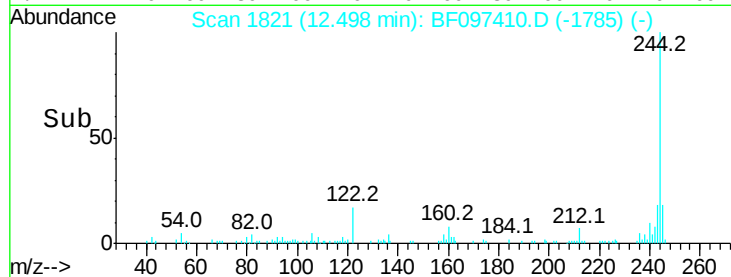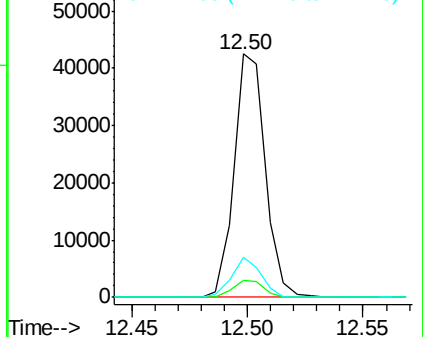

#86

Perylene-d12

Concen: 20.000 ng

RT: 14.89 min Scan# 2227

Delta R.T. -0.09 min

Lab File: BF097410.D

Acq: 5 Aug 2017 21:15


Tgt Ion:264 Resp: 95323

Ion Ratio Lower Upper

264 100

260 25.1 19.5 29.3

265 22.5 17.2 25.8



Abundance Ion 264.00 (263.70 to 264.70): E

Ion 260.00 (259.70 to 260.70): E

Ion 265.00 (264.70 to 265.70): E

