


Data Path : Z:\HPCHEM1\BNA F\Data\BF080517\
 Data File : BF097390.D
 Acq On : 5 Aug 2017 11:28
 Operator : SJ/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF072517.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Mon Aug 07 16:02:51 2017

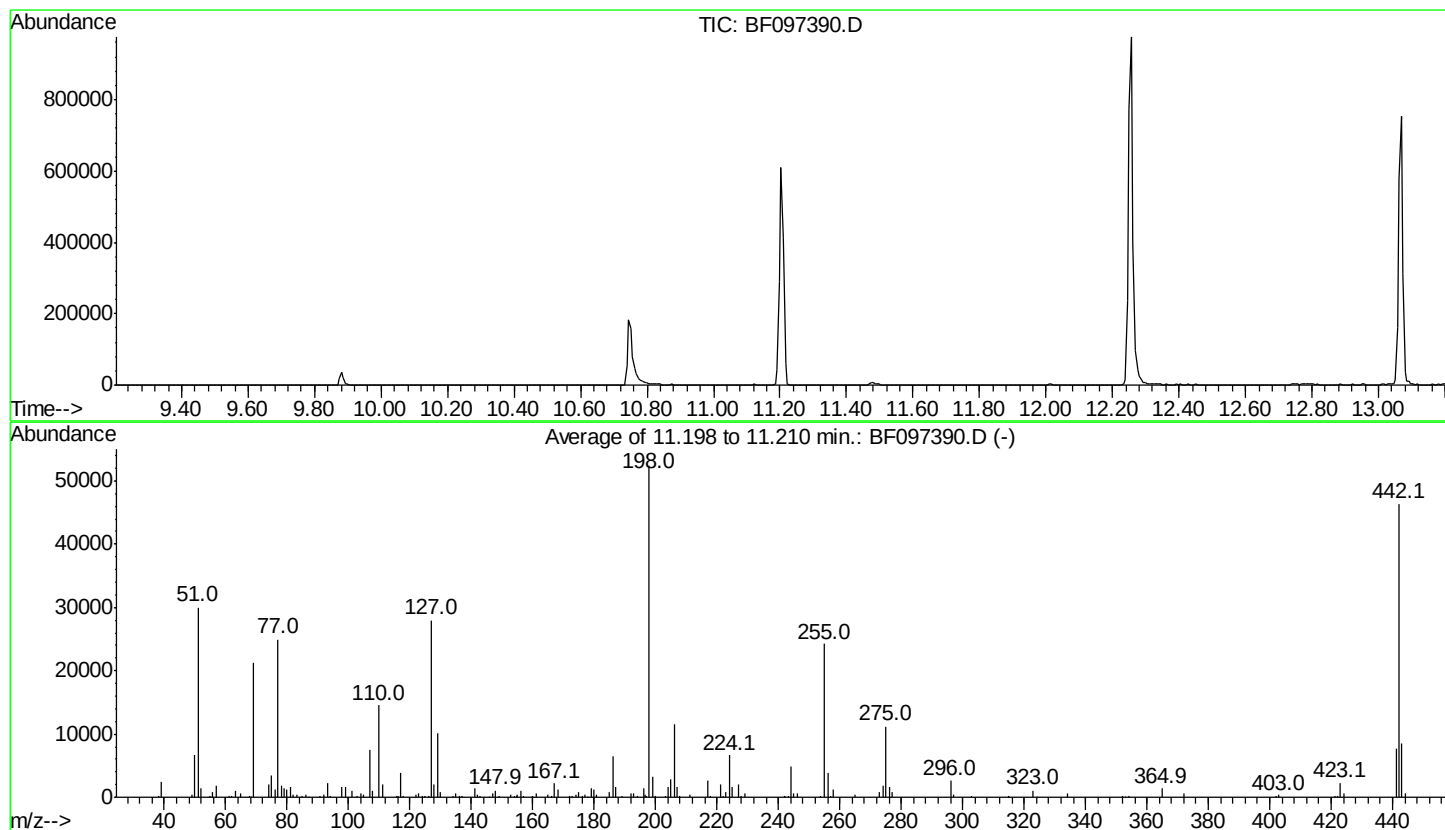

AutoFind: Scans 1600, 1601, 1602; Background Corrected with Scan 1595

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	57.3	30018	PASS
68	69	0.00	2	1.0	214	PASS
69	198	0.00	100	40.5	21241	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	53.4	28021	PASS
197	198	0.00	2	0.7	379	PASS
198	198	100	100	100.0	52426	PASS
199	198	5	9	6.3	3300	PASS
275	198	10	60	21.3	11144	PASS
365	198	1	100	2.6	1338	PASS
441	442	0.01	24	16.6	7721	PASS
442	198	50	100	88.5	46397	PASS
443	442	15	24	18.5	8578	PASS