


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF080520\
 Data File : BF121183.D
 Acq On : 5 Aug 2020 8:53
 Operator : JU/CG
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF071620.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed Jul 29 14:55:43 2020

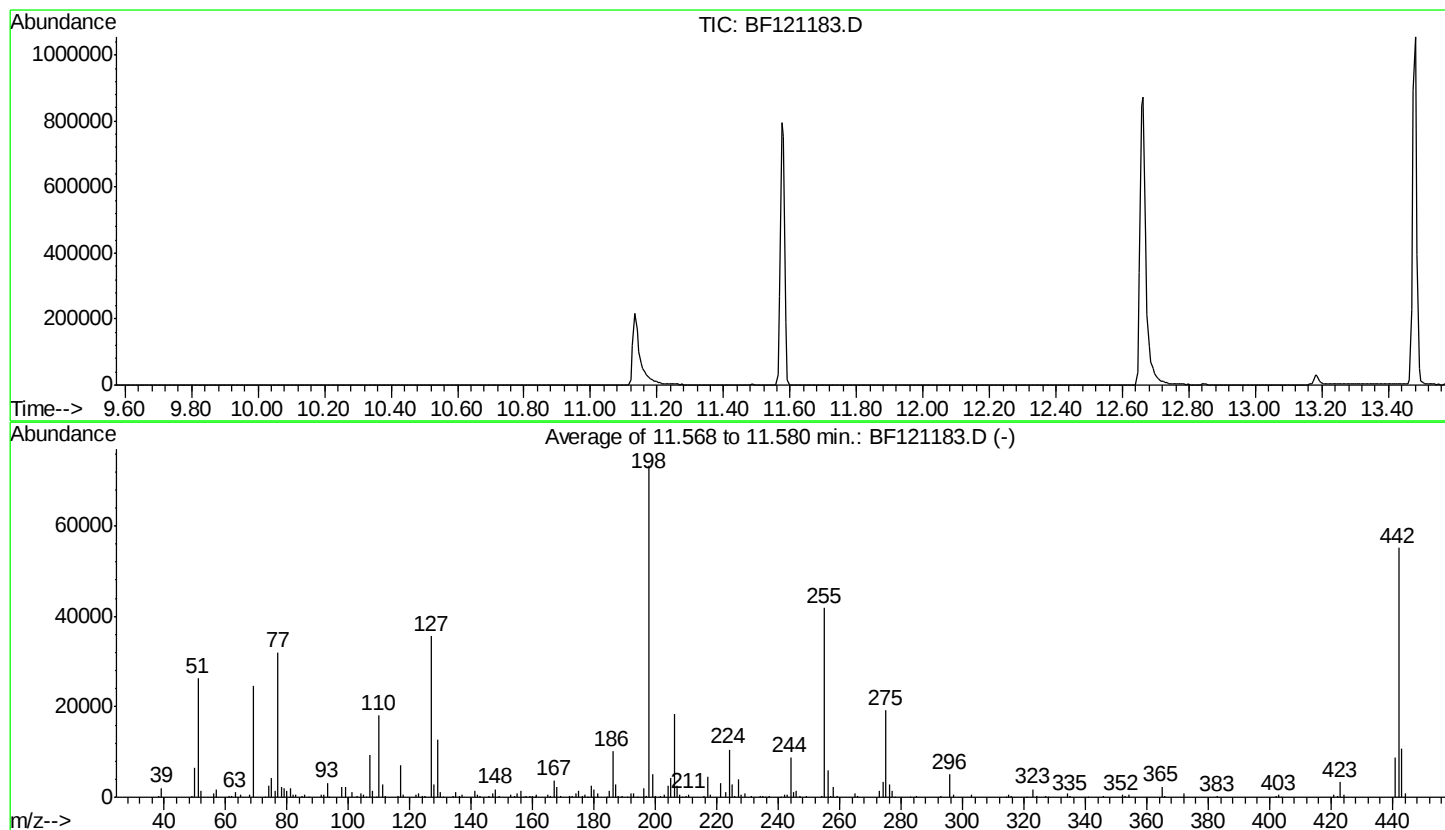

AutoFind: Scans 1612, 1613, 1614; Background Corrected with Scan 1607

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	35.8	26261	PASS
68	69	0.00	2	2.0	501	PASS
69	198	0.00	100	33.7	24684	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	48.5	35584	PASS
197	198	0.00	2	0.3	252	PASS
198	198	100	100	100.0	73341	PASS
199	198	5	9	7.0	5107	PASS
275	198	10	60	26.2	19211	PASS
365	198	1	100	3.1	2305	PASS
441	198	0.01	100	11.8	8690	PASS
442	198	50	100	75.2	55118	PASS
443	442	15	24	19.3	10657	PASS