
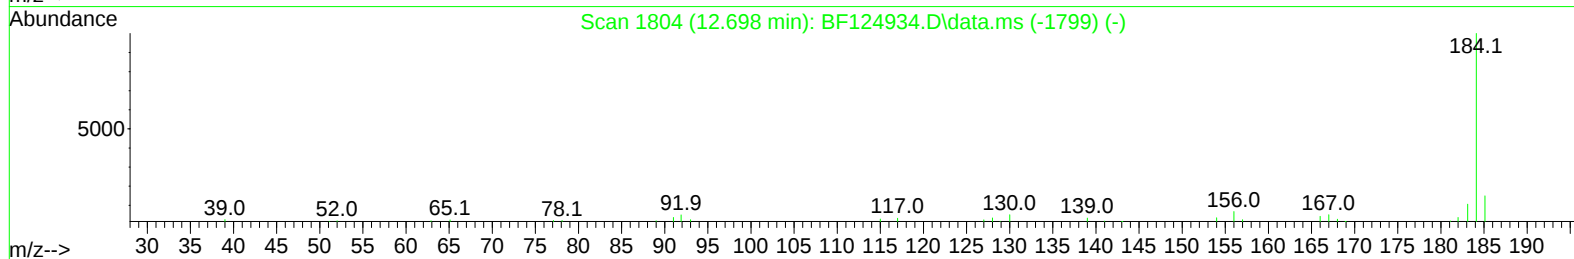
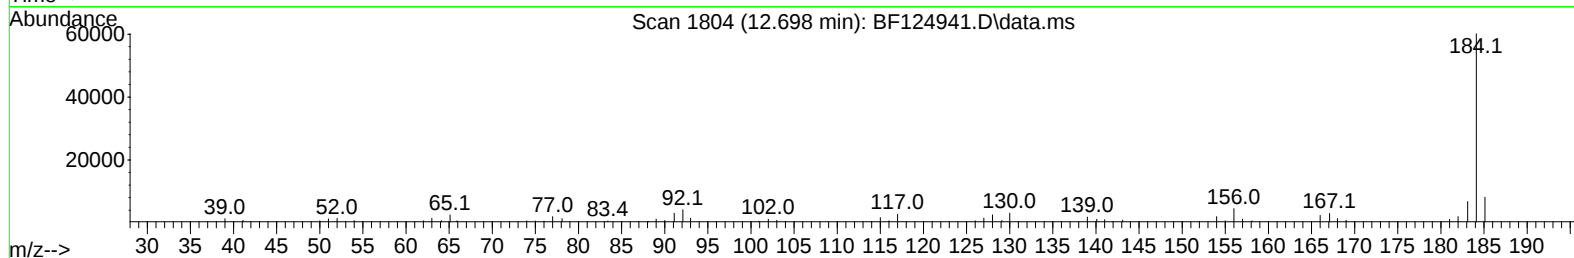


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF080521\
 Data File : BF124941.D
 Acq On : 5 Aug 2021 8:58
 Operator : JU/CG
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Aug 05 10:56:08 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF080421.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Aug 04 17:59:00 2021
 Response via : Initial Calibration

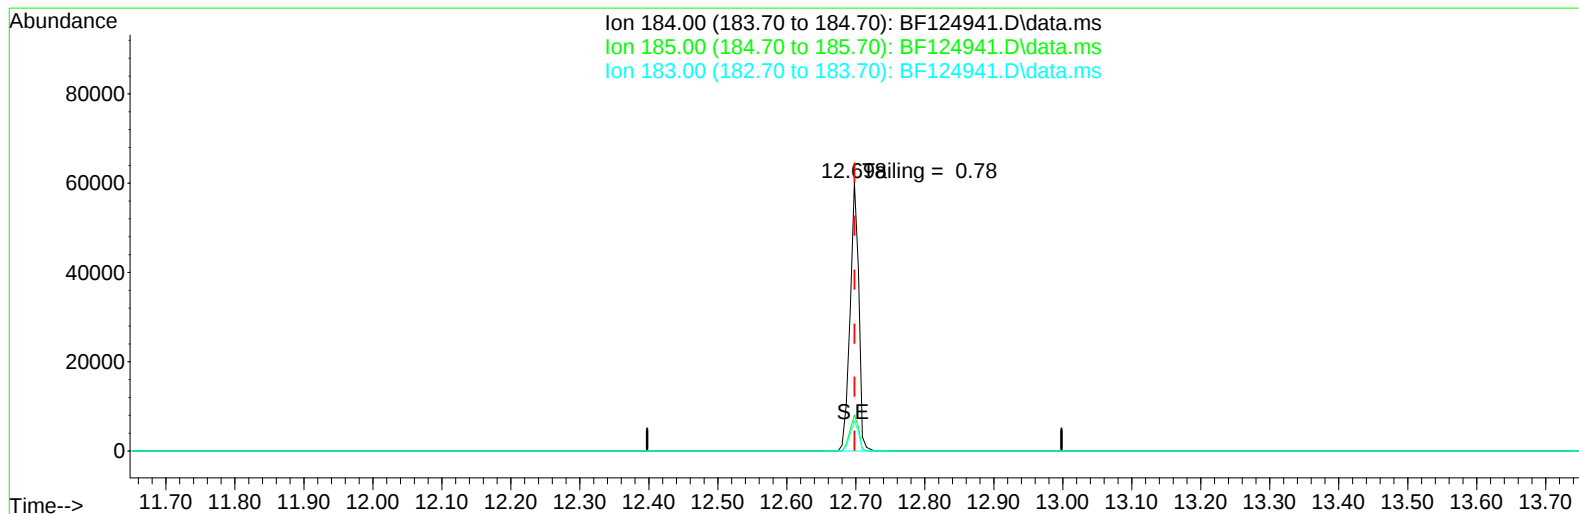

TIC: BF124941.D\data.ms

(77) Benzidine




12.698min (-0.000) 0.00 ng

response 52364

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	13.50	13.50
183.00	10.10	11.23
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF080521\
Data File : BF124941.D
Acq On : 5 Aug 2021 8:58
Operator : JU/CG
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Aug 05 10:56:08 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF080421.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Aug 04 17:59:00 2021
Response via : Initial Calibration

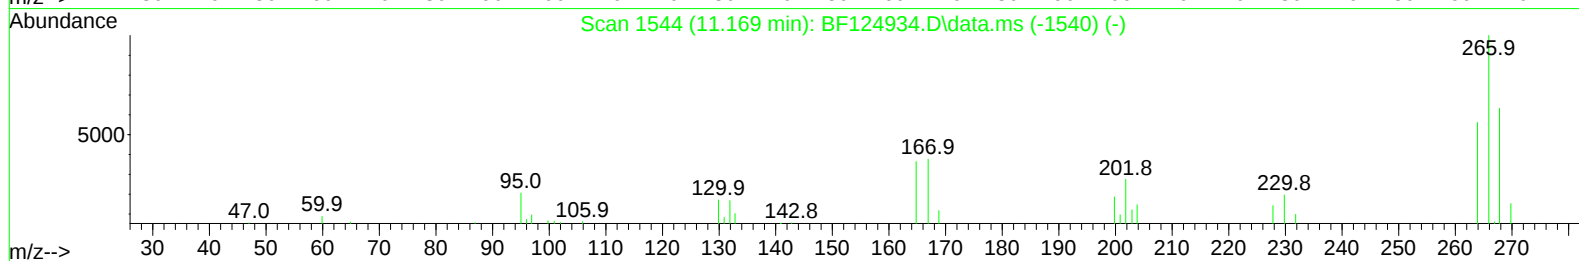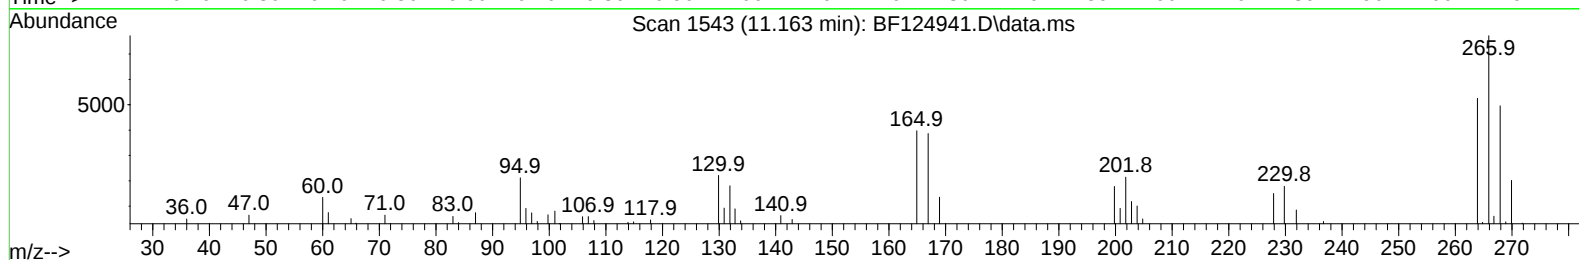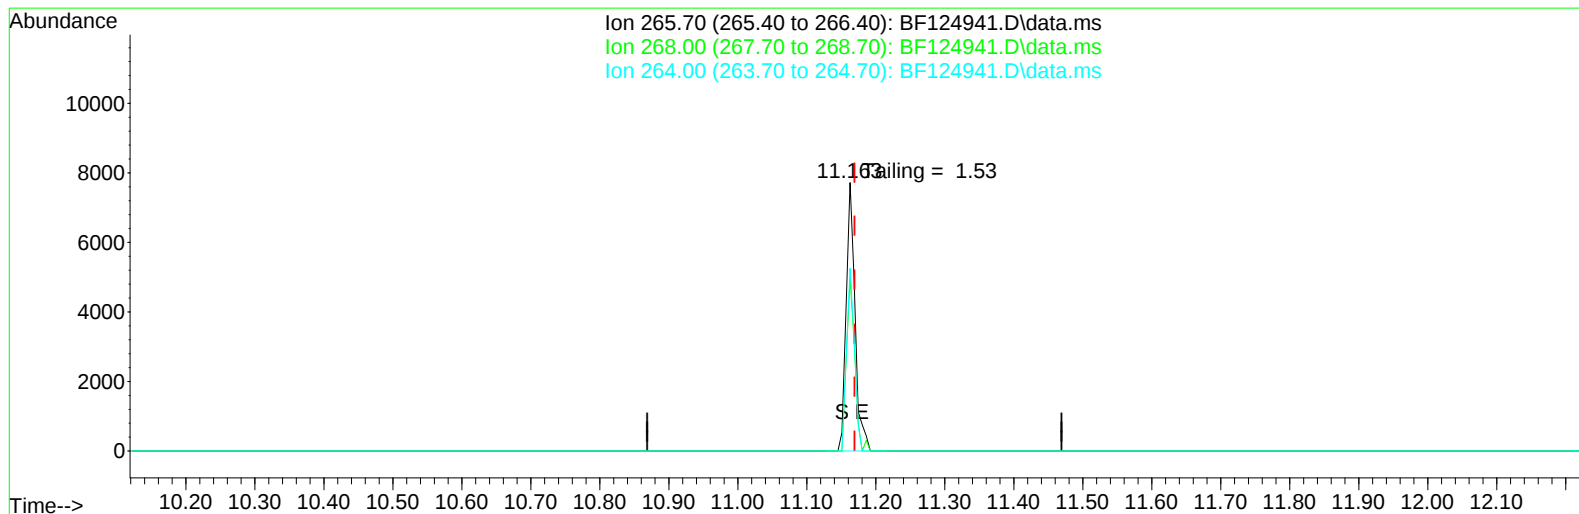

TIC: BF124941.D\data.ms

(70) Pentachlorophenol (C)

11.163min (-0.006) 0.00 ng

response 6882

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	61.10	64.20
264.00	69.90	68.01
0.00	0.00	0.00