

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF080521\
 Data File : BF124952.D
 Acq On : 5 Aug 2021 19:43
 Operator : JU/CG
 Sample : PB138104BL
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 PB138104BL

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF080421.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BF124952.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.093	509	511	516	rBB	2860	3270	1.05%	0.187%
2	5.469	570	575	578	rBV	215432	233621	75.31%	13.350%
3	6.469	739	745	748	rBB	217926	232493	74.95%	13.285%
4	6.834	804	807	810	rBB	60870	45542	14.68%	2.602%
5	7.398	898	903	906	rBV	134065	154326	49.75%	8.819%
6	8.116	1021	1025	1028	rBV	75666	63038	20.32%	3.602%
7	9.192	1203	1208	1211	rBV	289552	294892	95.07%	16.851%
8	9.875	1319	1324	1327	rBB	82360	72702	23.44%	4.154%
9	10.663	1453	1458	1461	rBV	189041	162360	52.34%	9.278%
10	11.357	1573	1576	1579	rVB	94552	71996	23.21%	4.114%
11	12.951	1842	1847	1849	rBV	315050	310199	100.00%	17.726%
12	13.998	2021	2025	2028	rBB	72636	58131	18.74%	3.322%
13	15.457	2269	2273	2278	rBB2	38863	47426	15.29%	2.710%




Sum of corrected areas: 1749996

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF080521\
Data File : BF124952.D
Acq On : 5 Aug 2021 19:43
Operator : JU/CG
Sample : PB138104BL
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB138104BL

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF080421.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

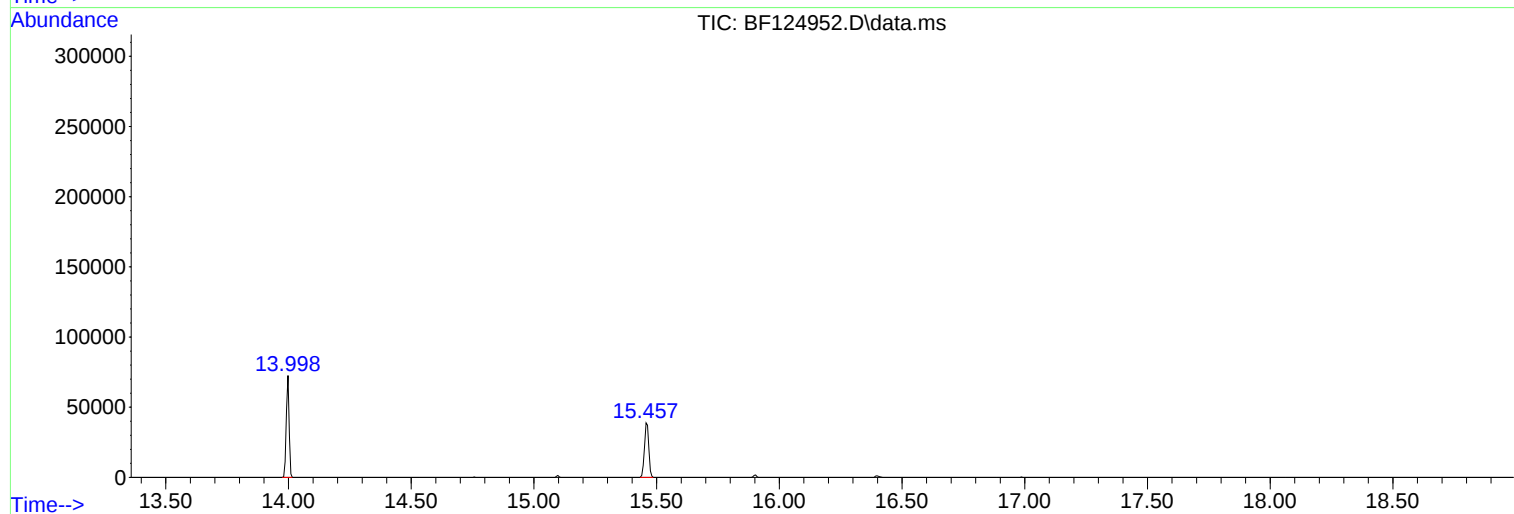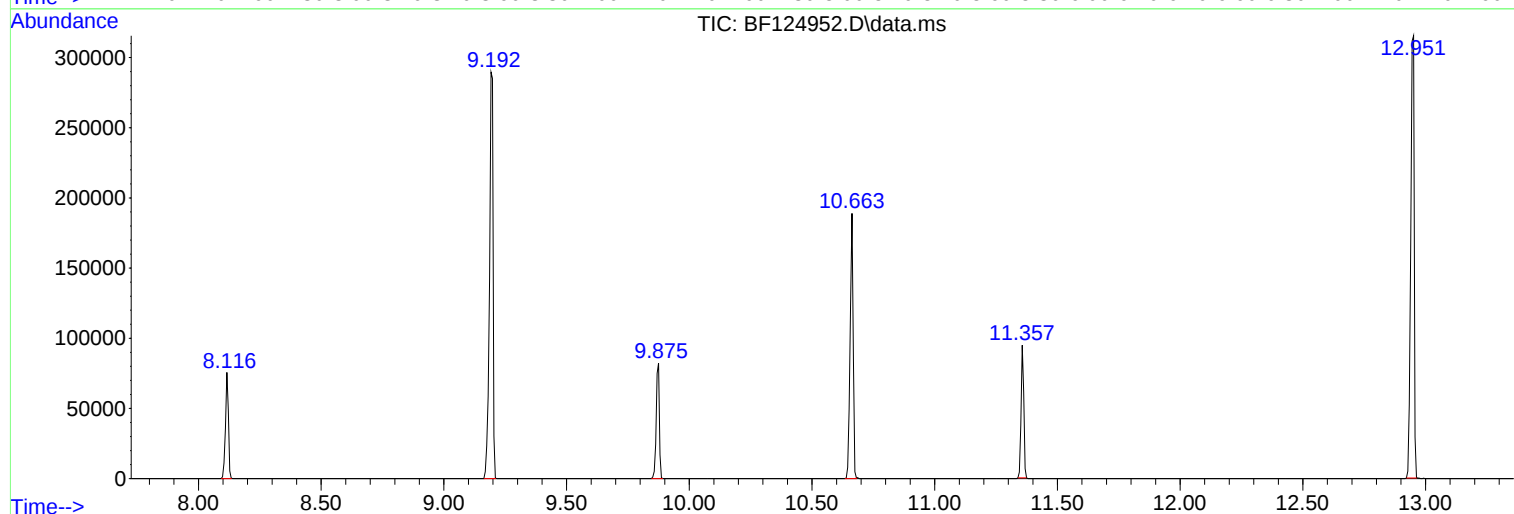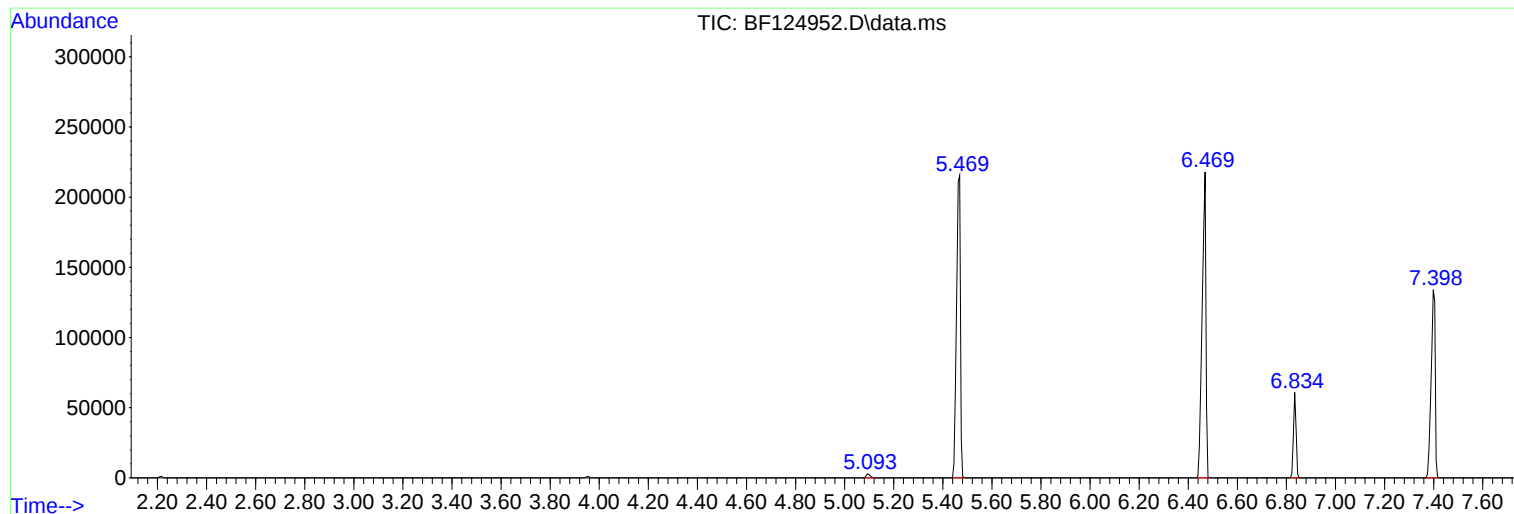

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF080521\
Data File : BF124952.D
Acq On : 5 Aug 2021 19:43
Operator : JU/CG
Sample : PB138104BL
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB138104BL

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF080421.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF080521\
Data File : BF124952.D
Acq On : 5 Aug 2021 19:43
Operator : JU/CG
Sample : PB138104BL
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB138104BL

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF080421.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------